

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017131.D
 Acq On : 13 Sep 2023 00:09
 Operator : MA/JU
 Sample : 04166-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKJ5

Quant Time: Sep 13 01:37:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 12 23:27:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	303772	20.000	ng/u1	0.00
20) Naphthalene-d8	10.781	136	1263665	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.610	164	806839	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.381	188	1837658	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	1664244	20.000	ng/u1	0.00
88) Perylene-d12	24.004	264	1632207	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	35038	4.847	ng/uL	0.00
4) Pyridine-d5	3.752	84	266406	12.883	ng/u1	0.00
7) Phenol-d5	7.105	99	247197	10.008	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67	559521	36.242	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	606565	30.782	ng/u1	0.00
15) 4-Methylphenol-d8	8.663	113	435009	21.250	ng/u1	0.00
21) Nitrobenzene-d5	9.158	128	367601	41.544	ng/u1	0.00
24) 2-Nitrophenol-d4	9.869	143	383733	40.622	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.393	165	684070	37.444	ng/u1	0.00
31) 4-Chloroaniline-d4	10.940	131	629842	22.873	ng/u1	0.00
46) Dimethylphthalate-d6	14.028	166	2326169	40.514	ng/u1	0.00
49) Acenaphthylene-d8	14.310	160	2527505	38.795	ng/u1	0.00
54) 4-Nitrophenol-d4	14.840	143	93128	8.392	ng/u1	0.00
60) Fluorene-d10	15.610	176	1988061	40.045	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.740	200	348448	33.939	ng/u1	0.00
73) Anthracene-d10	17.481	188	3251789	41.648	ng/u1	0.00
81) Pyrene-d10	19.722	212	3886263	44.526	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.839	264	3254239	42.242	ng/u1	-0.01
Target Compounds						
37) 1-Methylnaphthalene	12.657	142	135226	3.096	ng/u1	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017131.D
Acq On : 13 Sep 2023 00:09
Operator : MA/JU
Sample : 04166-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKJ5

Quant Time: Sep 13 01:37:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 12 23:27:27 2023
Response via : Initial Calibration

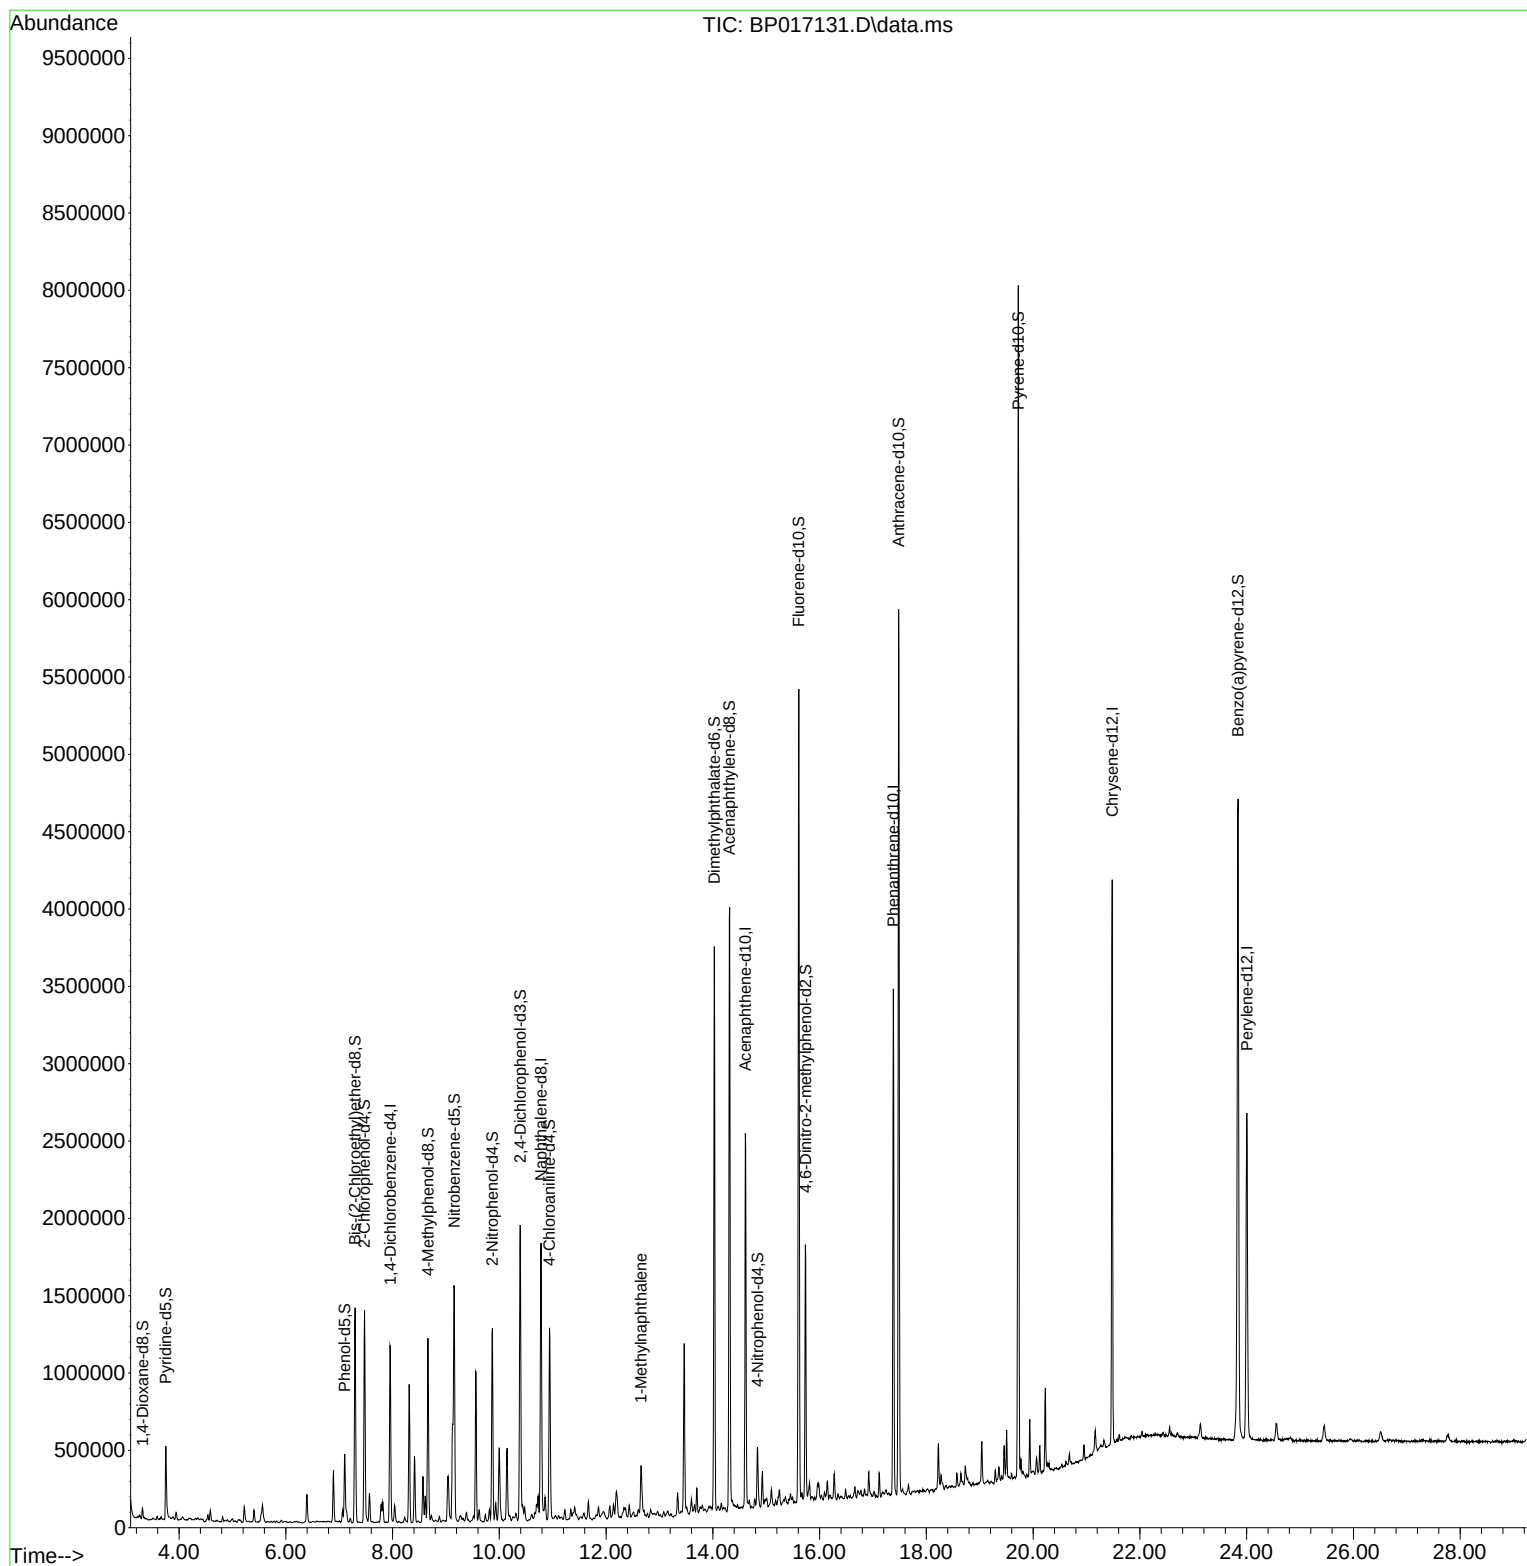

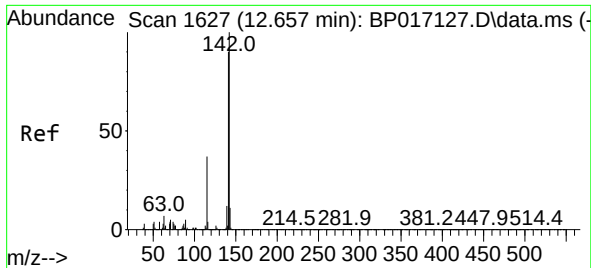

#37

1-Methylnaphthalene

Concen: 3.096 ng/ul

RT: 12.657 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP017131.D


Acq: 13 Sep 2023 00:09

Instrument :

BNA_P

ClientSampleId :

BBKJ5

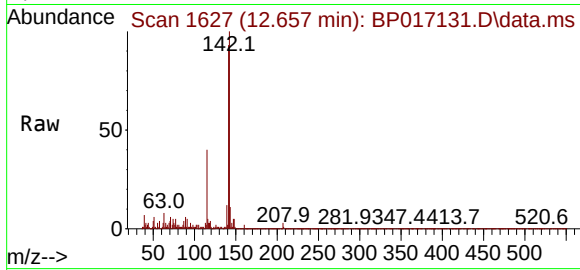

Tgt Ion:142 Resp: 135226

Ion Ratio Lower Upper

142 100

141 92.7 74.1 111.1

116 4.5 3.1 4.7

