

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017121.D
 Acq On : 12 Sep 2023 17:49
 Operator : MA/JU
 Sample : PB155306BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK306

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	34	38	45	rVB	66891	85228	2.33%	0.187%
2	3.746	108	112	131	rBV	758685	1168109	31.91%	2.562%
3	4.058	161	165	169	rBV	20019	24962	0.68%	0.055%
4	5.440	397	400	402	rBV4	2889	3755	0.10%	0.008%
5	5.764	452	455	458	rBV5	3160	4447	0.12%	0.010%
6	7.099	675	682	693	rBV	895793	1406010	38.41%	3.083%
7	7.287	706	714	724	rBV	739030	1161092	31.72%	2.546%
8	7.469	738	745	759	rBV	927017	1461310	39.92%	3.205%
9	7.952	818	827	835	rBV	780802	1252764	34.22%	2.747%
10	8.658	939	947	965	rBV	1069737	1716571	46.89%	3.764%
11	9.146	1023	1030	1044	rBV	802593	1320445	36.07%	2.896%
12	9.863	1143	1152	1159	rBV	679241	1070680	29.25%	2.348%
13	10.387	1233	1241	1253	rBV	1028364	1696390	46.34%	3.720%
14	10.781	1300	1308	1315	rBV	1007831	1707429	46.64%	3.744%
15	10.940	1326	1335	1347	rBV	1039876	1726112	47.15%	3.785%
16	11.781	1469	1478	1480	rBV10	2957	7060	0.19%	0.015%
17	11.952	1505	1507	1511	rVB5	3676	5121	0.14%	0.011%
18	12.363	1570	1577	1585	rVB3	17921	31701	0.87%	0.070%
19	12.581	1610	1614	1617	rBV6	3517	4950	0.14%	0.011%
20	12.799	1646	1651	1654	rBV7	2987	3722	0.10%	0.008%
21	13.040	1688	1692	1695	rVV6	2129	3800	0.10%	0.008%
22	13.463	1757	1764	1770	rBV3	14598	26817	0.73%	0.059%
23	13.569	1779	1782	1789	rVB9	3920	7106	0.19%	0.016%
24	13.840	1825	1828	1837	rVB10	5529	10516	0.29%	0.023%
25	14.028	1854	1860	1870	rBV	1686672	2289418	62.54%	5.021%
26	14.316	1902	1909	1923	rBV	1996846	2814725	76.89%	6.173%
27	14.616	1953	1960	1970	rBV	1468512	2128375	58.14%	4.668%
28	14.834	1990	1997	2013	rBV	543464	970524	26.51%	2.128%
29	15.010	2025	2027	2032	rVB6	4776	5723	0.16%	0.013%
30	15.416	2091	2096	2102	rVB7	6426	12001	0.33%	0.026%
31	15.610	2122	2129	2139	rBV	2399610	3489171	95.31%	7.652%
32	15.740	2145	2151	2160	rBV	588725	790712	21.60%	1.734%
33	15.845	2166	2169	2173	rVB6	8642	11764	0.32%	0.026%
34	16.393	2260	2262	2264	rBV3	4267	4492	0.12%	0.010%
35	16.675	2307	2310	2312	rVV4	4777	4528	0.12%	0.010%
36	16.898	2346	2348	2351	rBV4	3007	3680	0.10%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017121.D
 Acq On : 12 Sep 2023 17:49
 Operator : MA/JU
 Sample : PB155306BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK306

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	17.051	2372	2374	2377	rVB4	3569	3805	0.10%	0.008%
38	17.175	2391	2395	2400	rVV6	4942	8070	0.22%	0.018%
39	17.387	2425	2431	2442	rBV	1606008	2267776	61.95%	4.973%
40	17.487	2442	2448	2466	rVB	2480551	3471289	94.82%	7.613%
41	17.757	2491	2494	2497	rVB5	4565	5431	0.15%	0.012%
42	18.234	2573	2575	2579	rVB5	6485	5525	0.15%	0.012%
43	19.298	2753	2756	2761	rVB4	28076	36915	1.01%	0.081%
44	19.369	2765	2768	2776	rVB3	24140	37090	1.01%	0.081%
45	19.728	2824	2829	2844	rBV	2857447	3660768	100.00%	8.028%
46	21.486	3124	3128	3135	rBV	1527080	1985001	54.22%	4.353%
47	23.851	3524	3530	3544	rVB2	1734072	3521810	96.20%	7.723%
48	24.022	3553	3559	3572	rVB	1054284	2164461	59.13%	4.747%




Sum of corrected areas: 45599151

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017121.D
Acq On : 12 Sep 2023 17:49
Operator : MA/JU
Sample : PB155306BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

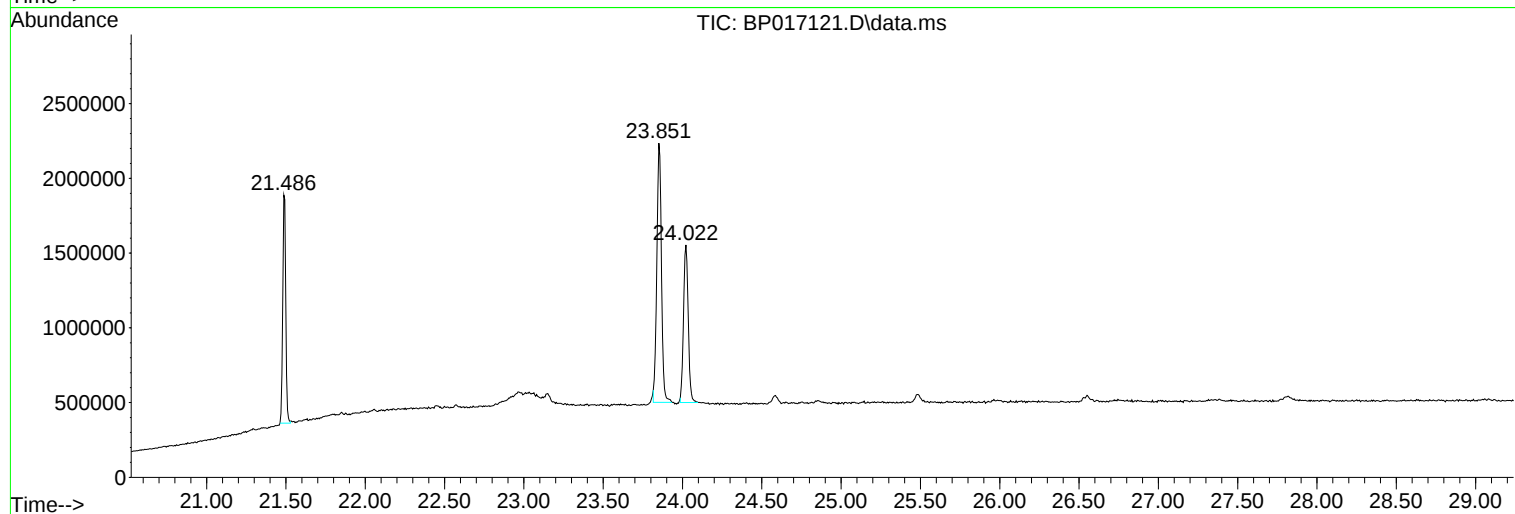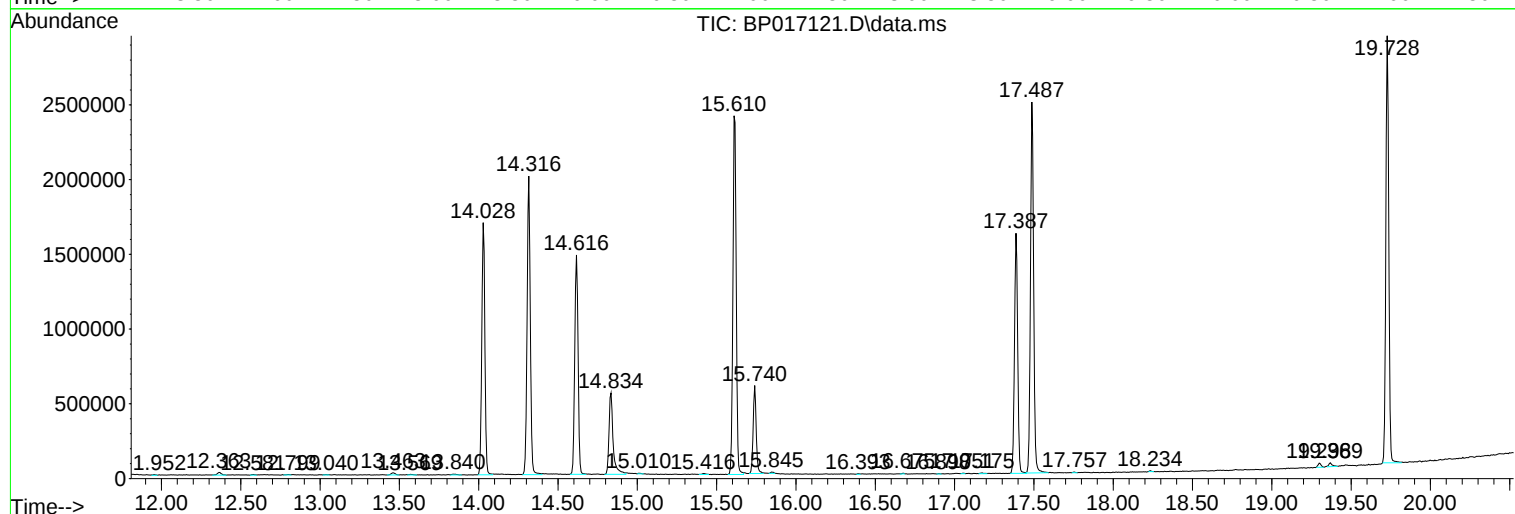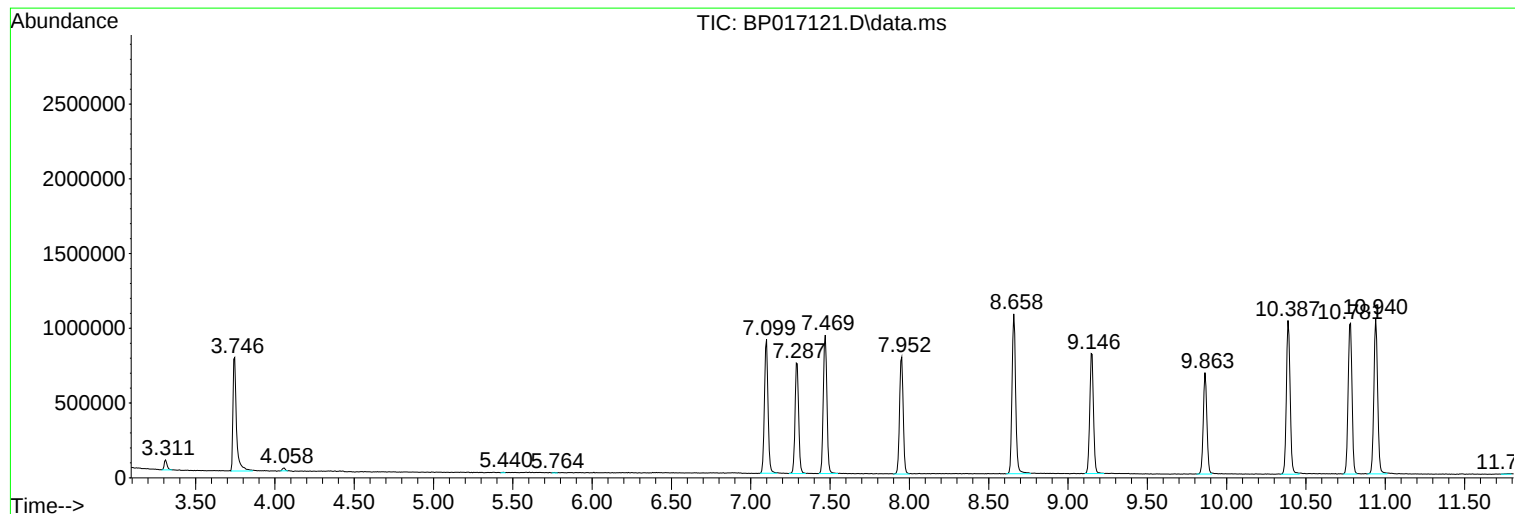

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017121.D
Acq On : 12 Sep 2023 17:49
Operator : MA/JU
Sample : PB155306BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017121.D
Acq On : 12 Sep 2023 17:49
Operator : MA/JU
Sample : PB155306BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc