

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017128.D
 Acq On : 12 Sep 2023 22:26
 Operator : MA/JU
 Sample : PB155340BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK340

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	48	rVB	47445	75021	1.22%	0.131%
2	3.752	109	113	136	rBV	642528	1105443	17.97%	1.923%
3	4.064	162	166	174	rVB2	12737	19983	0.32%	0.035%
4	6.899	645	648	653	rBV7	3811	7261	0.12%	0.013%
5	7.105	676	683	700	rBV	870602	1365235	22.20%	2.375%
6	7.299	709	716	728	rVB	708978	1099610	17.88%	1.913%
7	7.475	739	746	755	rBV	874761	1369129	22.26%	2.382%
8	7.958	821	828	836	rBV	756305	1210688	19.69%	2.106%
9	8.664	941	948	966	rBV	1058834	1708014	27.77%	2.972%
10	9.152	1022	1031	1040	rBV	802779	1300118	21.14%	2.262%
11	9.869	1144	1153	1161	rBV	665134	1082193	17.60%	1.883%
12	10.393	1233	1242	1257	rBV	1051948	1725103	28.05%	3.002%
13	10.781	1298	1308	1316	rBV	1065121	1767223	28.74%	3.075%
14	10.940	1328	1335	1358	rBV	1057099	1812798	29.48%	3.154%
15	12.363	1572	1577	1583	rBV2	18649	30503	0.50%	0.053%
16	13.457	1758	1763	1769	rBV2	13306	21422	0.35%	0.037%
17	14.028	1853	1860	1873	rBV	2006295	2673445	43.47%	4.652%
18	14.310	1900	1908	1928	rBV	2072519	3111150	50.59%	5.413%
19	14.610	1953	1959	1973	rBV	1642997	2430955	39.53%	4.230%
20	14.828	1990	1996	2016	rBV	790104	1319786	21.46%	2.296%
21	15.610	2122	2129	2140	rBV	2869275	4038306	65.66%	7.026%
22	15.734	2144	2150	2164	rVV	845026	1129960	18.37%	1.966%
23	15.846	2166	2169	2176	rVB4	14295	22835	0.37%	0.040%
24	16.393	2258	2262	2268	rBV9	5889	9209	0.15%	0.016%
25	16.663	2305	2308	2312	rBV6	4322	6991	0.11%	0.012%
26	17.381	2424	2430	2440	rBV	2191849	3070054	49.92%	5.342%
27	17.481	2441	2447	2460	rBV	3273502	4545251	73.91%	7.908%
28	19.292	2751	2755	2759	rVB3	36179	45897	0.75%	0.080%
29	19.363	2763	2767	2771	rVB	31046	40466	0.66%	0.070%
30	19.722	2822	2828	2838	rBV	4419074	5748237	93.47%	10.001%
31	21.480	3122	3127	3135	rBV	2732785	3589461	58.37%	6.245%
32	23.839	3520	3528	3546	rVB2	2963710	6149976	100.00%	10.700%
33	24.004	3549	3556	3567	rVB	1863827	3842646	62.48%	6.686%


Sum of corrected areas: 57474369

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017128.D
Acq On : 12 Sep 2023 22:26
Operator : MA/JU
Sample : PB155340BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK340

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

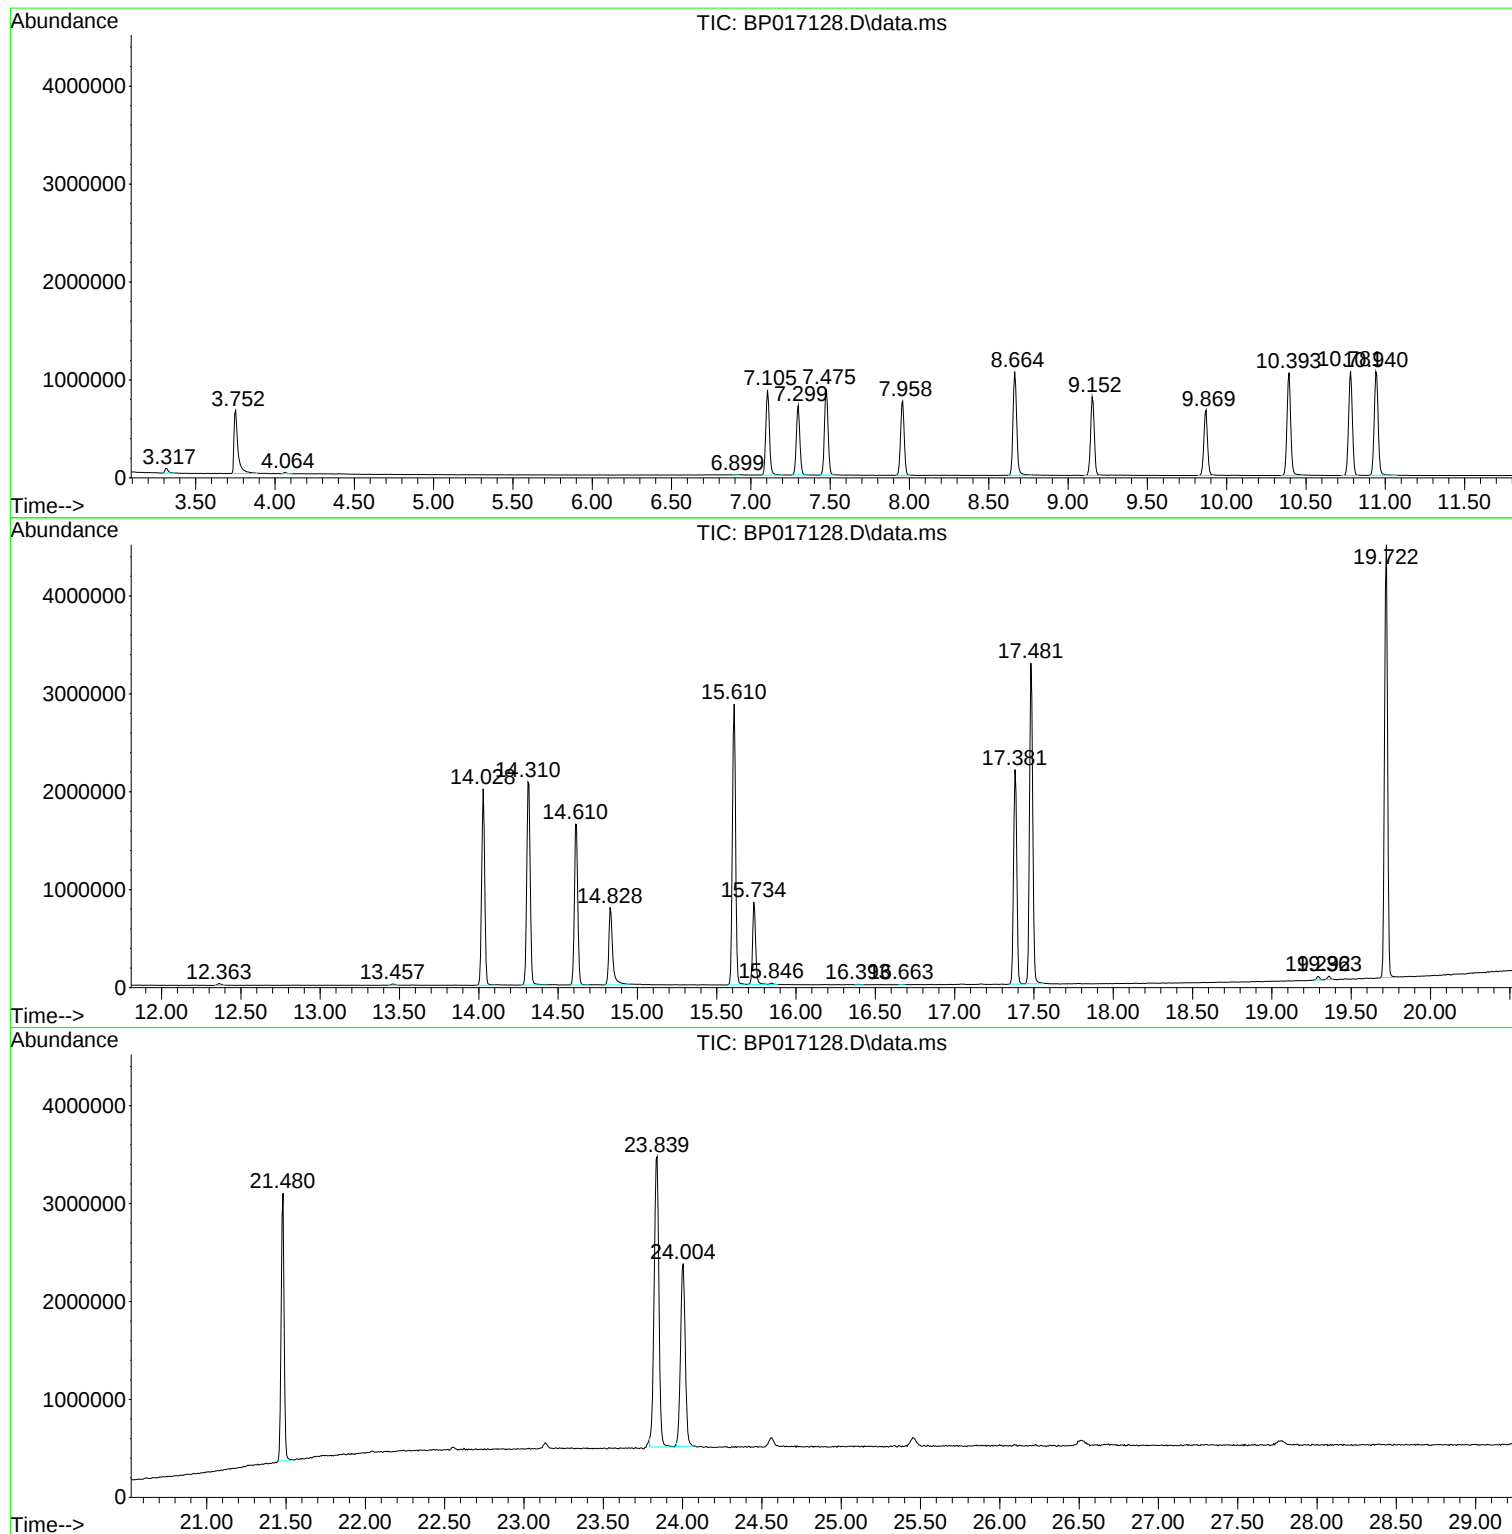

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017128.D
Acq On : 12 Sep 2023 22:26
Operator : MA/JU
Sample : PB155340BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK340

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017128.D
Acq On : 12 Sep 2023 22:26
Operator : MA/JU
Sample : PB155340BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK340

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc