

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017133.D
 Acq On : 13 Sep 2023 01:18
 Operator : MA/JU
 Sample : 04247-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	35	rVB5	14165	17719	0.15%	0.016%
2	3.317	35	39	52	rVB	93662	135902	1.16%	0.120%
3	3.752	110	113	129	rBV	309843	477737	4.06%	0.424%
4	3.946	141	146	152	rVB2	39531	60648	0.52%	0.054%
5	4.064	161	166	170	rBV	21046	31177	0.27%	0.028%
6	4.587	250	255	262	rBV	152984	230617	1.96%	0.204%
7	5.005	320	326	329	rBV	11336	17607	0.15%	0.016%
8	6.905	645	649	653	rBV7	8597	12851	0.11%	0.011%
9	7.105	676	683	695	rBV	421998	648263	5.51%	0.575%
10	7.299	708	716	726	rBV	1362147	2136038	18.16%	1.894%
11	7.475	739	746	760	rBV	1428612	2225039	18.92%	1.973%
12	7.952	821	827	838	rBV	1524695	2438203	20.73%	2.162%
13	8.663	940	948	960	rBV	1200063	1907657	16.22%	1.691%
14	9.152	1024	1031	1050	rBV	1641483	2654881	22.57%	2.354%
15	9.363	1063	1067	1074	rVB5	12038	19981	0.17%	0.018%
16	9.869	1143	1153	1160	rBV	1352667	2207534	18.77%	1.957%
17	10.393	1233	1242	1261	rBV	2141738	3574269	30.39%	3.169%
18	10.781	1300	1308	1316	rBV	2446500	4017918	34.16%	3.562%
19	10.940	1327	1335	1350	rBV	1564257	2681134	22.79%	2.377%
20	12.363	1571	1577	1582	rBV	37707	59587	0.51%	0.053%
21	13.457	1756	1763	1772	rBV2	59816	106067	0.90%	0.094%
22	13.545	1774	1778	1782	rBV	18348	31075	0.26%	0.028%
23	13.857	1825	1831	1836	rVB3	15469	23479	0.20%	0.021%
24	14.028	1854	1860	1872	rBV	4298130	5834307	49.60%	5.173%
25	14.316	1901	1909	1921	rBV	4734509	6916270	58.80%	6.132%
26	14.475	1933	1936	1941	rVB5	10437	14522	0.12%	0.013%
27	14.534	1941	1946	1952	rVB2	20352	32586	0.28%	0.029%
28	14.616	1952	1960	1968	rBV	4123655	5908220	50.23%	5.238%
29	14.834	1991	1997	2008	rBV	350789	611711	5.20%	0.542%
30	15.010	2024	2027	2031	rVV6	10365	13055	0.11%	0.012%
31	15.051	2031	2034	2039	rVB6	14855	20008	0.17%	0.018%
32	15.610	2122	2129	2142	rBV	6312593	8840821	75.16%	7.838%
33	15.739	2145	2151	2157	rBV	2086204	2812773	23.91%	2.494%
34	15.845	2165	2169	2173	rVB	25067	33152	0.28%	0.029%
35	16.269	2237	2241	2247	rBV2	18941	34217	0.29%	0.030%
36	16.398	2259	2263	2269	rVB9	8874	15212	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017133.D
 Acq On : 13 Sep 2023 01:18
 Operator : MA/JU
 Sample : 04247-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	16.881	2343	2345	2351	rVB5	14433	18976	0.16%	0.017%
38	17.069	2375	2377	2380	rVB2	15898	14948	0.13%	0.013%
39	17.110	2381	2384	2389	rVB5	20361	27843	0.24%	0.025%
40	17.169	2390	2394	2401	rBV4	15077	25618	0.22%	0.023%
41	17.381	2424	2430	2441	rBV	5090067	7415258	63.04%	6.574%
42	17.486	2441	2448	2460	rVV	6860515	9504938	80.81%	8.427%
43	17.598	2465	2467	2471	rBV3	11374	14693	0.12%	0.013%
44	17.769	2493	2496	2501	rBV3	31621	46708	0.40%	0.041%
45	17.810	2501	2503	2507	rVB3	25382	29998	0.26%	0.027%
46	18.010	2533	2537	2543	rVB5	30179	46399	0.39%	0.041%
47	18.222	2569	2573	2581	rBV	170357	253991	2.16%	0.225%
48	18.316	2586	2589	2592	rVB	28178	33980	0.29%	0.030%
49	18.486	2615	2618	2621	rBV4	23142	28130	0.24%	0.025%
50	18.598	2634	2637	2640	rBV2	20834	28755	0.24%	0.025%
51	19.292	2752	2755	2759	rVB2	87313	98573	0.84%	0.087%
52	19.363	2763	2767	2776	rVB2	113764	196159	1.67%	0.174%
53	19.457	2780	2783	2790	rBV	173547	252615	2.15%	0.224%
54	19.598	2804	2807	2811	rBV	86230	92141	0.78%	0.082%
55	19.722	2822	2828	2839	rBV	8899015	11762630	100.00%	10.429%
56	19.974	2868	2871	2876	rVB	101889	125104	1.06%	0.111%
57	20.227	2911	2914	2919	rBV	86804	107837	0.92%	0.096%
58	21.163	3070	3073	3081	rVB2	137388	214313	1.82%	0.190%
59	21.480	3122	3127	3133	rBV	5814544	7698650	65.45%	6.826%
60	23.845	3518	3529	3542	rVB	5032288	10764129	91.51%	9.544%
61	24.010	3549	3557	3568	rVB	3445044	7184435	61.08%	6.370%




Sum of corrected areas: 112789058

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017133.D
Acq On : 13 Sep 2023 01:18
Operator : MA/JU
Sample : 04247-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

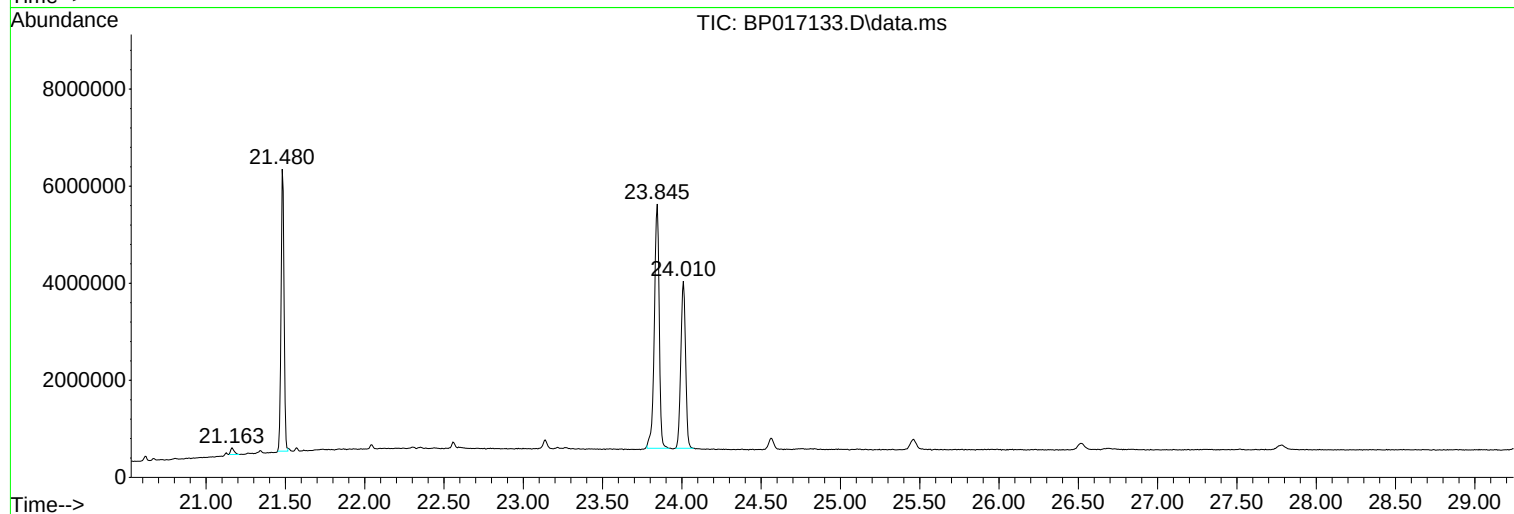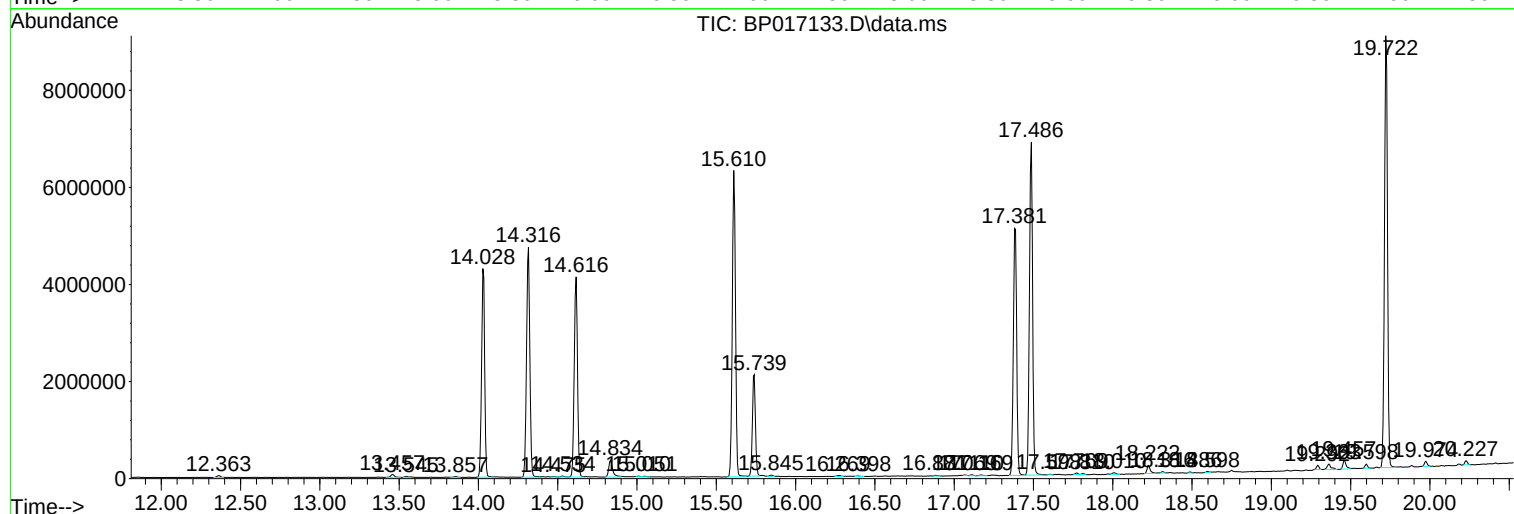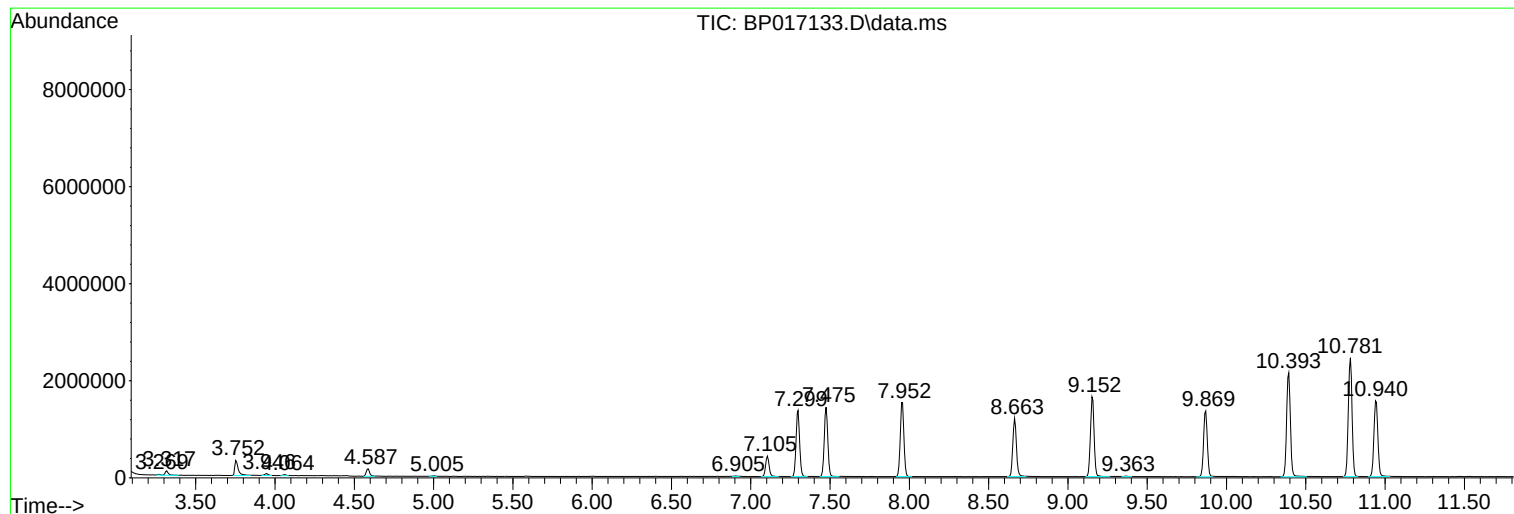

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017133.D
Acq On : 13 Sep 2023 01:18
Operator : MA/JU
Sample : 04247-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017133.D
Acq On : 13 Sep 2023 01:18
Operator : MA/JU
Sample : 04247-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------