

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017134.D
 Acq On : 13 Sep 2023 01:52
 Operator : MA/JU
 Sample : 04247-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017134.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	26	31	35	rBV3	26206	38739	0.71%	0.072%
2	3.317	35	39	46	rVB	61428	85446	1.57%	0.158%
3	3.752	109	113	128	rBV	338167	530692	9.73%	0.984%
4	3.946	142	146	154	rVB2	22152	36828	0.68%	0.068%
5	4.064	162	166	170	rVB	15284	22265	0.41%	0.041%
6	4.287	201	204	210	rVB7	7638	12225	0.22%	0.023%
7	4.446	229	231	242	rVB7	8303	14896	0.27%	0.028%
8	4.587	249	255	263	rBV	195568	298685	5.48%	0.554%
9	4.999	321	325	329	rVB5	4589	7316	0.13%	0.014%
10	7.105	676	683	693	rBV	282697	442175	8.11%	0.820%
11	7.293	708	715	726	rBV	759824	1201012	22.03%	2.227%
12	7.475	739	746	756	rBV	492114	772874	14.18%	1.433%
13	7.952	818	827	840	rBV	1109056	1757151	32.23%	3.259%
14	8.663	941	948	960	rBV	593199	959504	17.60%	1.779%
15	9.152	1022	1031	1043	rBV	883858	1434368	26.31%	2.660%
16	9.363	1063	1067	1074	rVB8	7924	13903	0.26%	0.026%
17	9.863	1146	1152	1163	rBV	334250	559784	10.27%	1.038%
18	10.393	1235	1242	1251	rBV	586395	972266	17.83%	1.803%
19	10.781	1300	1308	1321	rVB	1730925	2838954	52.07%	5.265%
20	10.940	1328	1335	1347	rBV	1001352	1693337	31.06%	3.140%
21	11.469	1418	1425	1431	rBV6	5525	12356	0.23%	0.023%
22	12.193	1543	1548	1551	rBV7	2835	5675	0.10%	0.011%
23	12.363	1571	1577	1583	rBV	17052	28363	0.52%	0.053%
24	13.457	1756	1763	1768	rBV2	31663	58107	1.07%	0.108%
25	13.575	1780	1783	1790	rVB9	5784	8798	0.16%	0.016%
26	14.028	1853	1860	1873	rBV	1793910	2462921	45.18%	4.567%
27	14.310	1901	1908	1923	rBV	1906749	2751801	50.47%	5.103%
28	14.610	1952	1959	1974	rBV	2755892	4057136	74.42%	7.524%
29	14.839	1992	1998	2007	rBV	80631	168726	3.09%	0.313%
30	14.998	2022	2025	2031	rVB8	4936	9911	0.18%	0.018%
31	15.610	2121	2129	2138	rBV	2354593	3340006	61.26%	6.194%
32	15.734	2145	2150	2159	rVB	100031	145838	2.67%	0.270%
33	15.845	2165	2169	2173	rVB3	11689	15608	0.29%	0.029%
34	16.828	2334	2336	2342	rBV6	4961	9858	0.18%	0.018%
35	17.051	2370	2374	2376	rBV5	3752	6071	0.11%	0.011%
36	17.257	2406	2409	2413	rBV5	7293	11177	0.21%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017134.D
 Acq On : 13 Sep 2023 01:52
 Operator : MA/JU
 Sample : 04247-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	17.381	2424	2430	2439	rBV	3650024	5024226	92.15%	9.317%
38	17.481	2441	2447	2457	rVV	2399516	3343466	61.33%	6.200%
39	18.222	2569	2573	2580	rBV2	48080	76581	1.40%	0.142%
40	19.292	2752	2755	2759	rBV3	33868	40665	0.75%	0.075%
41	19.363	2764	2767	2772	rVB2	41998	53934	0.99%	0.100%
42	19.598	2804	2807	2814	rBV3	51516	58000	1.06%	0.108%
43	19.722	2822	2828	2834	rBV	3066173	3947260	72.40%	7.320%
44	20.622	2978	2981	2985	rVB2	55188	60657	1.11%	0.112%
45	21.480	3122	3127	3137	rBV	4247829	5451931	100.00%	10.111%
46	23.839	3521	3528	3542	rVB2	1709840	3645156	66.86%	6.760%
47	24.004	3549	3556	3568	rVB	2572559	5436439	99.72%	10.082%




Sum of corrected areas: 53923087

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017134.D
Acq On : 13 Sep 2023 01:52
Operator : MA/JU
Sample : 04247-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJL6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

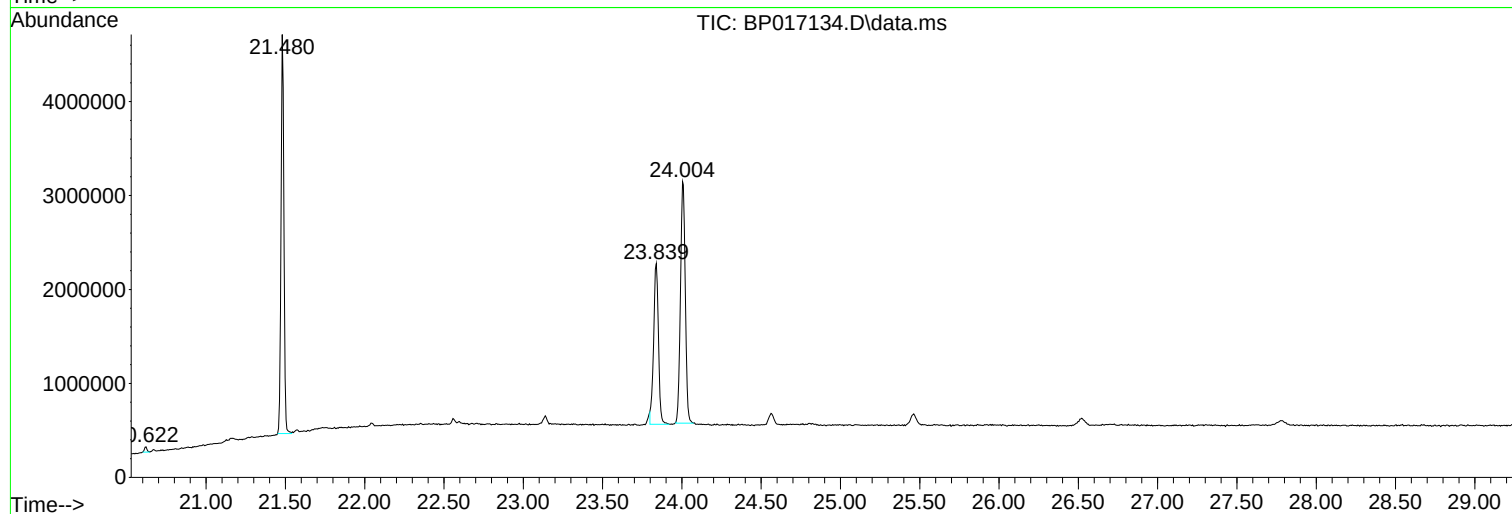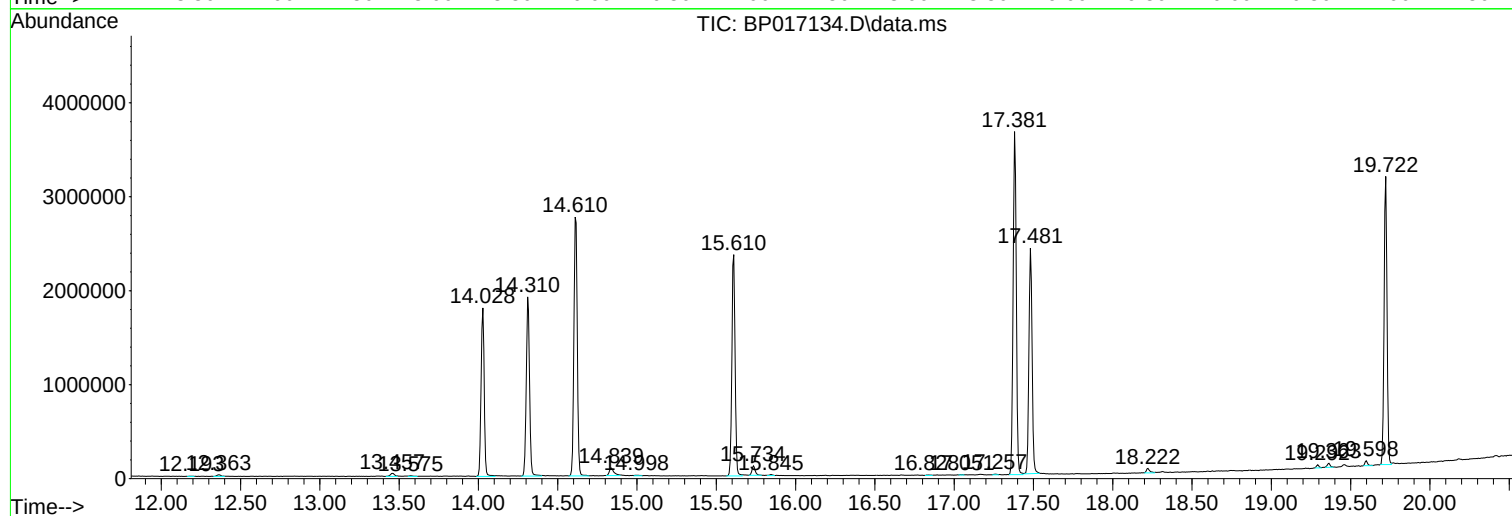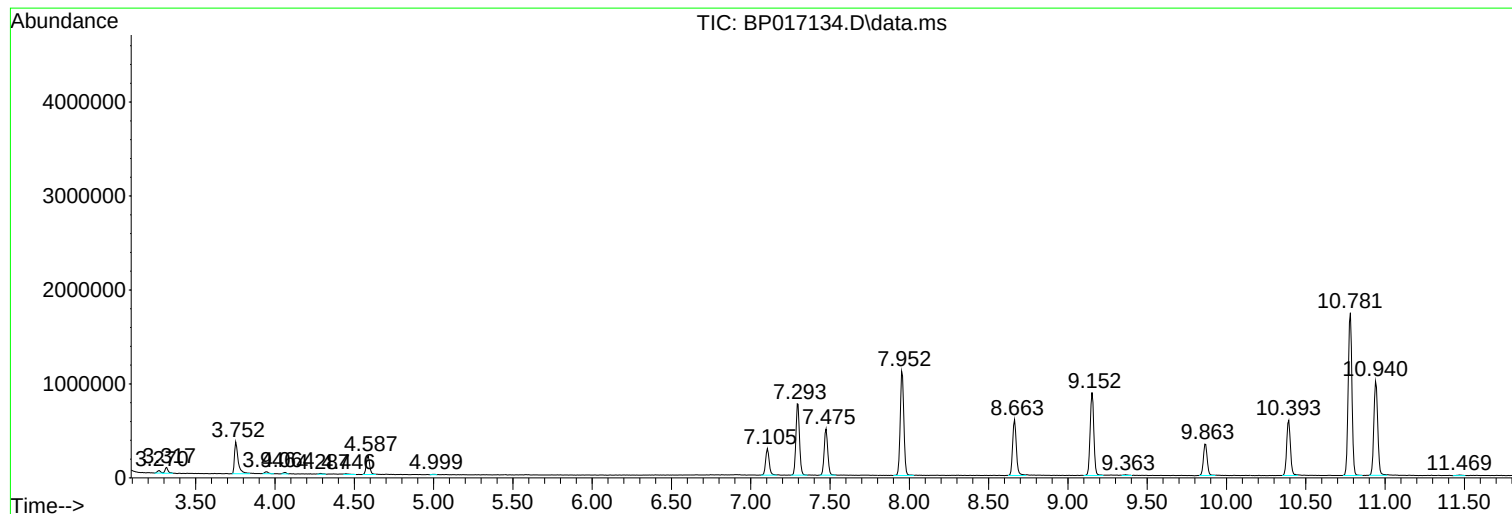

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017134.D
Acq On : 13 Sep 2023 01:52
Operator : MA/JU
Sample : 04247-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJL6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.587	3.40 ng/ul	298685	1,4-Dichlorobenzene-d4	7.952

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			2,4-Dichloro-6-fluoropyrimidine	166	C4HC12FN2	003833-57-6	27

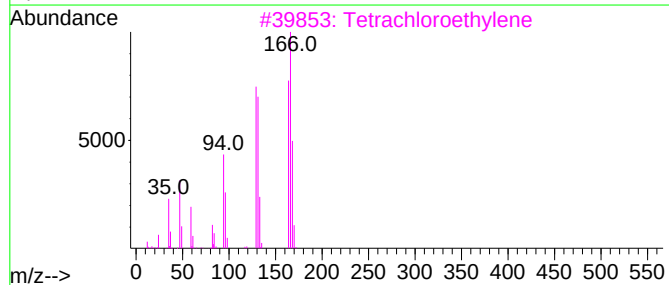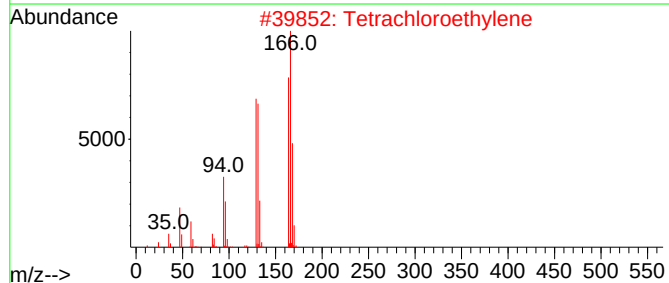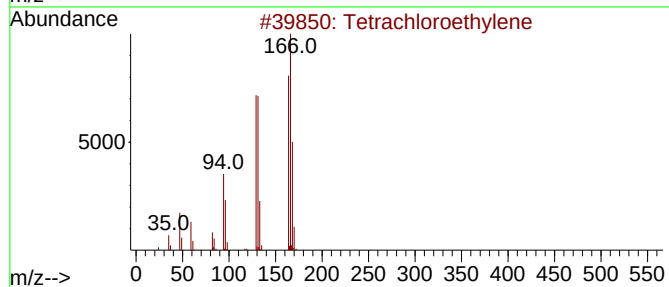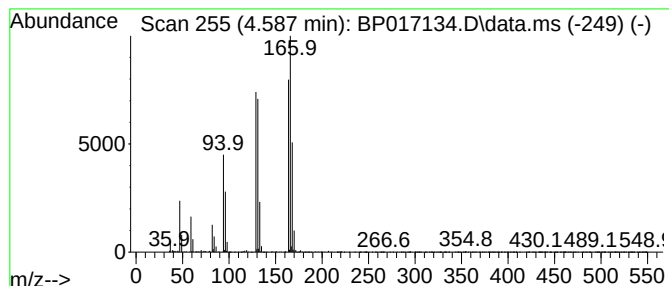

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017134.D
Acq On : 13 Sep 2023 01:52
Operator : MA/JU
Sample : 04247-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJL6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.587	3.4	ng/u1	298685	1	7.952	1757150	20.0