

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017139.D
 Acq On : 13 Sep 2023 09:22
 Operator : MA/JU
 Sample : PB155418BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK418

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	34	37	47	rVB	56364	82234	1.35%	0.148%
2	3.740	107	111	127	rBV	538110	898162	14.80%	1.619%
3	4.052	160	164	168	rVB	15454	18978	0.31%	0.034%
4	7.087	671	680	694	rBV	837073	1335900	22.01%	2.407%
5	7.281	707	713	722	rVB	695149	1072833	17.68%	1.933%
6	7.457	736	743	754	rBV	840761	1331358	21.94%	2.399%
7	7.940	817	825	835	rBV	653826	1025813	16.90%	1.849%
8	8.652	939	946	962	rVV	1025271	1675265	27.60%	3.019%
9	9.140	1021	1029	1037	rBV	799737	1285591	21.18%	2.317%
10	9.857	1143	1151	1161	rBV	655423	1077694	17.76%	1.942%
11	10.381	1232	1240	1253	rBV	1057680	1732652	28.55%	3.122%
12	10.769	1298	1306	1315	rVB	931224	1534667	25.28%	2.765%
13	10.934	1326	1334	1345	rBV	516805	884490	14.57%	1.594%
14	12.357	1566	1576	1583	rBV3	21200	45823	0.75%	0.083%
15	13.457	1757	1763	1769	rVB6	14152	26290	0.43%	0.047%
16	13.563	1777	1781	1785	rBV7	5933	9347	0.15%	0.017%
17	13.610	1785	1789	1790	rBV4	7240	7352	0.12%	0.013%
18	14.028	1853	1860	1870	rBV	1983194	2751601	45.33%	4.958%
19	14.310	1901	1908	1920	rBV	2219923	3171335	52.25%	5.715%
20	14.610	1953	1959	1967	rBV	1513419	2165590	35.68%	3.902%
21	14.828	1989	1996	2017	rBV	847029	1379631	22.73%	2.486%
22	15.234	2059	2065	2072	rBV	6561	16781	0.28%	0.030%
23	15.392	2082	2092	2101	rBV4	31611	102738	1.69%	0.185%
24	15.610	2122	2129	2144	rBV	3003132	4172903	68.75%	7.520%
25	15.734	2144	2150	2160	rBV	850979	1173233	19.33%	2.114%
26	15.851	2166	2170	2177	rVB6	15728	36919	0.61%	0.067%
27	16.069	2205	2207	2212	rVB5	7196	7728	0.13%	0.014%
28	16.392	2260	2262	2268	rVB7	5061	6133	0.10%	0.011%
29	16.516	2278	2283	2285	rBV5	8169	12156	0.20%	0.022%
30	16.663	2304	2308	2315	rVB	46062	67407	1.11%	0.121%
31	17.051	2371	2374	2382	rVB9	11565	22111	0.36%	0.040%
32	17.169	2390	2394	2398	rVB4	5852	8993	0.15%	0.016%
33	17.380	2424	2430	2439	rBV	1932045	2781393	45.83%	5.012%
34	17.486	2441	2448	2463	rVB	3332938	4707324	77.56%	8.483%
35	17.745	2488	2492	2496	rBV	37938	47701	0.79%	0.086%
36	18.016	2534	2538	2542	rBV6	10375	14301	0.24%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017139.D
Acq On : 13 Sep 2023 09:22
Operator : MA/JU
Sample : PB155418BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK418

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION

37	18.098	2550	2552	2561	rBV9	6048	9731	0.16%	0.018%
38	18.222	2571	2573	2585	rBV9	10059	24915	0.41%	0.045%
39	18.351	2592	2595	2598	rBV2	11502	12693	0.21%	0.023%
40	18.663	2645	2648	2652	rVB2	34689	39505	0.65%	0.071%
41	19.292	2752	2755	2760	rBV2	40990	53485	0.88%	0.096%
42	19.363	2764	2767	2770	rBV	35459	47120	0.78%	0.085%
43	19.433	2776	2779	2783	rBV	38196	49548	0.82%	0.089%
44	19.727	2823	2829	2835	rBV	4369608	5871922	96.74%	10.581%
45	21.486	3123	3128	3139	rBV	2540872	3276058	53.98%	5.904%
46	23.851	3523	3530	3550	rVB2	2982447	6069548	100.00%	10.937%
47	24.015	3552	3558	3571	rVB	1627305	3348345	55.17%	6.034%




Sum of corrected areas: 55493297

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017139.D
Acq On : 13 Sep 2023 09:22
Operator : MA/JU
Sample : PB155418BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK418

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

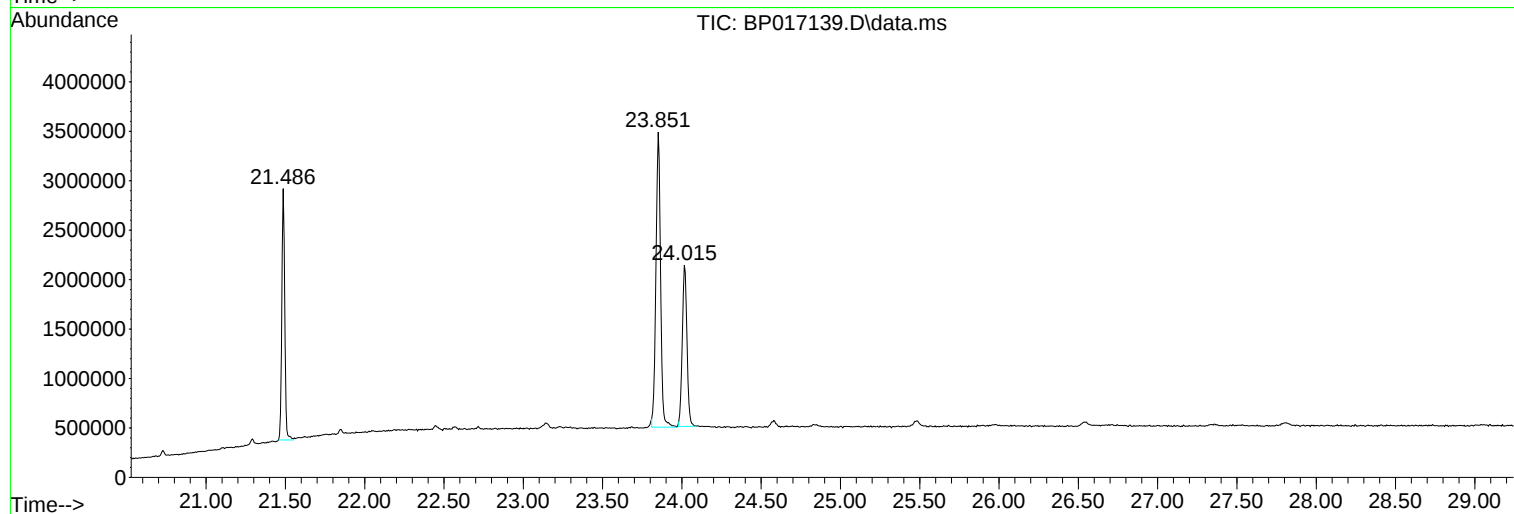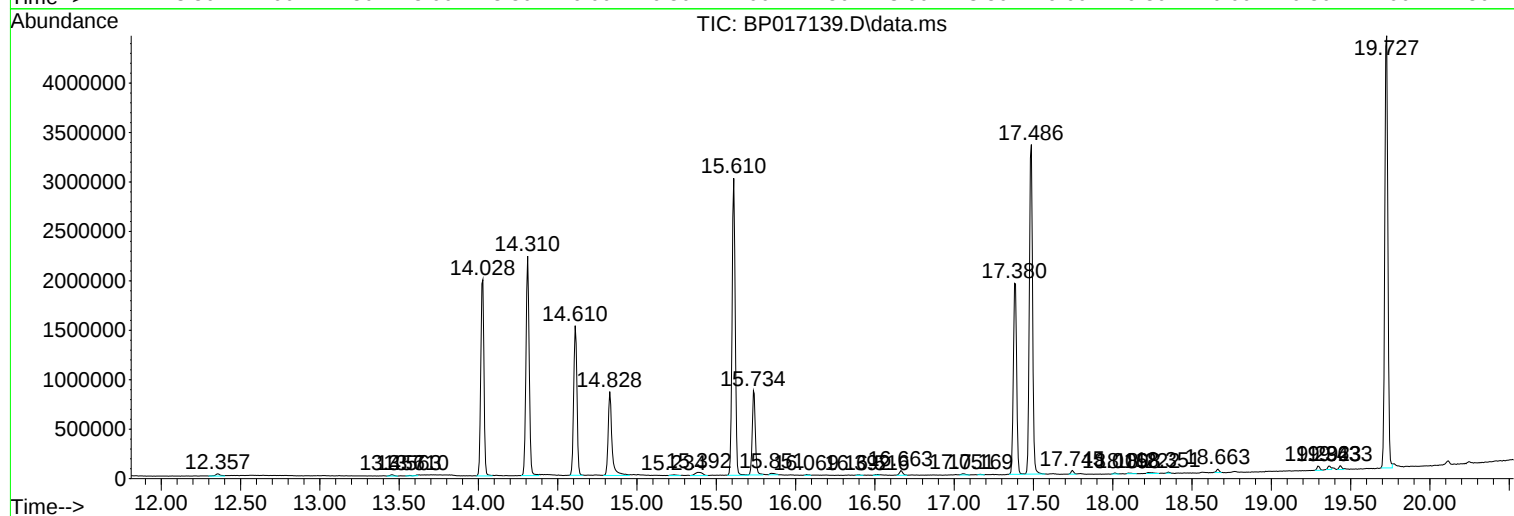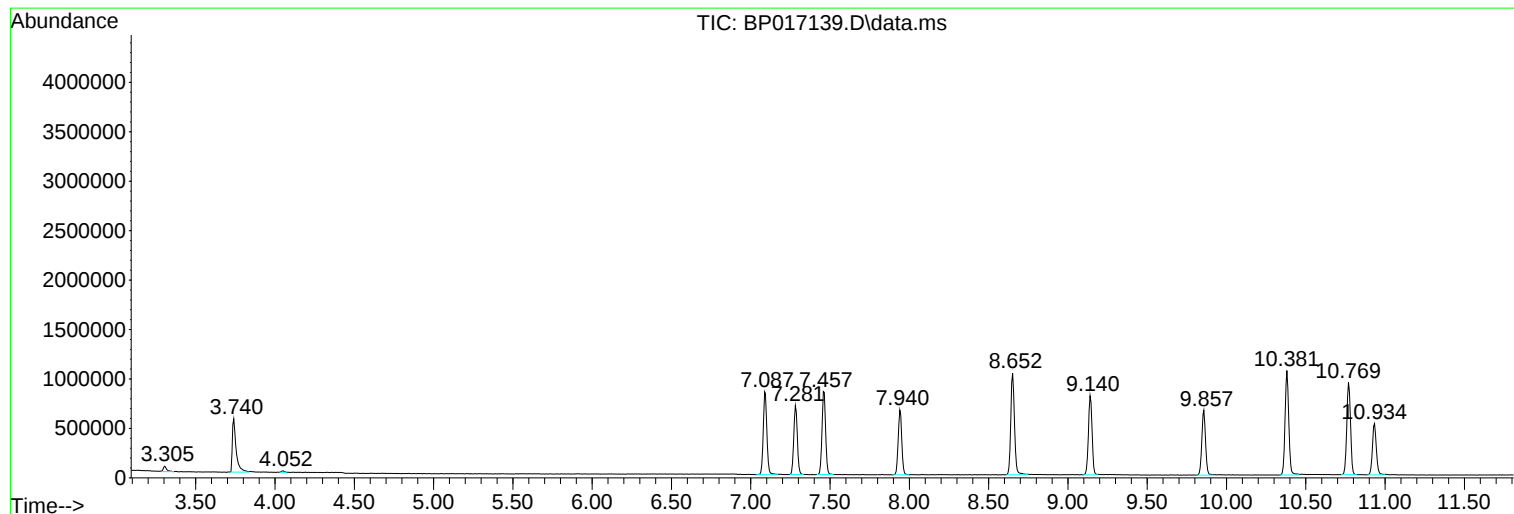

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017139.D
Acq On : 13 Sep 2023 09:22
Operator : MA/JU
Sample : PB155418BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK418

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017139.D
Acq On : 13 Sep 2023 09:22
Operator : MA/JU
Sample : PB155418BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK418

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------