

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017147.D
 Acq On : 13 Sep 2023 13:58
 Operator : MA/JU
 Sample : 04324-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017147.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	35	rBV	46390	59721	0.90%	0.107%
2	3.317	35	39	43	rVB	49378	55060	0.83%	0.098%
3	3.752	110	113	129	rVB	202254	312628	4.69%	0.559%
4	3.946	141	146	155	rVB	46102	71102	1.07%	0.127%
5	4.058	162	165	170	rVB2	11084	12814	0.19%	0.023%
6	4.587	248	255	273	rBV	3866609	5980265	89.73%	10.688%
7	4.999	319	325	329	rBV3	8612	15612	0.23%	0.028%
8	5.587	422	425	431	rVB2	6755	10292	0.15%	0.018%
9	7.105	675	683	695	rBV	233265	382317	5.74%	0.683%
10	7.293	707	715	726	rBV	885936	1381066	20.72%	2.468%
11	7.475	738	746	757	rBV	866160	1376496	20.65%	2.460%
12	7.952	821	827	836	rBV	639366	1003962	15.06%	1.794%
13	8.663	941	948	959	rBV	641539	1031003	15.47%	1.843%
14	9.152	1023	1031	1042	rBV	986495	1561833	23.43%	2.791%
15	9.863	1145	1152	1166	rBV	778722	1225251	18.38%	2.190%
16	10.387	1233	1241	1257	rBV	1105656	1846064	27.70%	3.299%
17	10.775	1301	1307	1315	rBV	797978	1320724	19.82%	2.360%
18	10.940	1329	1335	1347	rBV	539031	898649	13.48%	1.606%
19	11.775	1469	1477	1488	rBV	139227	292520	4.39%	0.523%
20	12.357	1572	1576	1583	rVV2	16143	27806	0.42%	0.050%
21	12.934	1669	1674	1679	rBV8	6429	13043	0.20%	0.023%
22	13.457	1756	1763	1769	rBV3	25177	44194	0.66%	0.079%
23	13.581	1779	1784	1788	rBV8	4416	7951	0.12%	0.014%
24	14.028	1853	1860	1873	rBV	1968630	2688043	40.33%	4.804%
25	14.310	1899	1908	1924	rBV	2304723	3245703	48.70%	5.801%
26	14.522	1941	1944	1952	rVB8	8774	15926	0.24%	0.028%
27	14.610	1952	1959	1968	rBV	1142361	1599979	24.01%	2.860%
28	14.834	1991	1997	2010	rBV	109645	230291	3.46%	0.412%
29	15.610	2122	2129	2139	rBV	2888023	4108696	61.65%	7.343%
30	15.734	2144	2150	2161	rVV	925699	1209957	18.15%	2.163%
31	15.845	2165	2169	2175	rVB6	12038	23065	0.35%	0.041%
32	16.387	2259	2261	2266	rVB6	5917	8359	0.13%	0.015%
33	16.887	2337	2346	2349	rBV5	27227	46501	0.70%	0.083%
34	17.192	2395	2398	2404	rVB3	11542	15040	0.23%	0.027%
35	17.381	2423	2430	2440	rBV	1374686	1883900	28.27%	3.367%
36	17.481	2440	2447	2461	rBV	3397125	4596019	68.96%	8.214%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017147.D
Acq On : 13 Sep 2023 13:58
Operator : MA/JU
Sample : 04324-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHF8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION

37	18.222	2569	2573	2579	rBV	49986	72097	1.08%	0.129%
38	19.292	2751	2755	2759	rBV	44002	56212	0.84%	0.100%
39	19.357	2763	2766	2773	rVB	42675	65070	0.98%	0.116%
40	19.457	2780	2783	2792	rBV3	48853	67604	1.01%	0.121%
41	19.722	2822	2828	2835	rBV	4566424	5758803	86.40%	10.293%
42	21.480	3122	3127	3137	rBV	1729630	2191981	32.89%	3.918%
43	23.845	3521	3529	3543	rVB2	3234565	6664960	100.00%	11.912%
44	24.010	3550	3557	3571	rVB	1180017	2472711	37.10%	4.419%




Sum of corrected areas: 55951290

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017147.D
Acq On : 13 Sep 2023 13:58
Operator : MA/JU
Sample : 04324-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

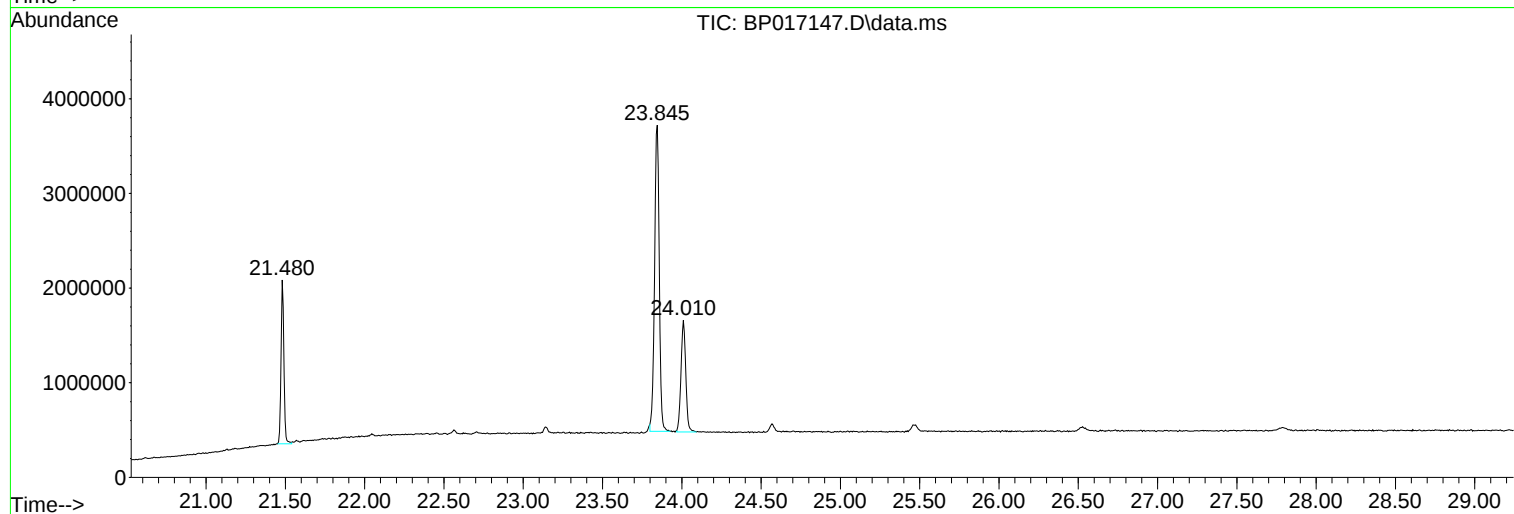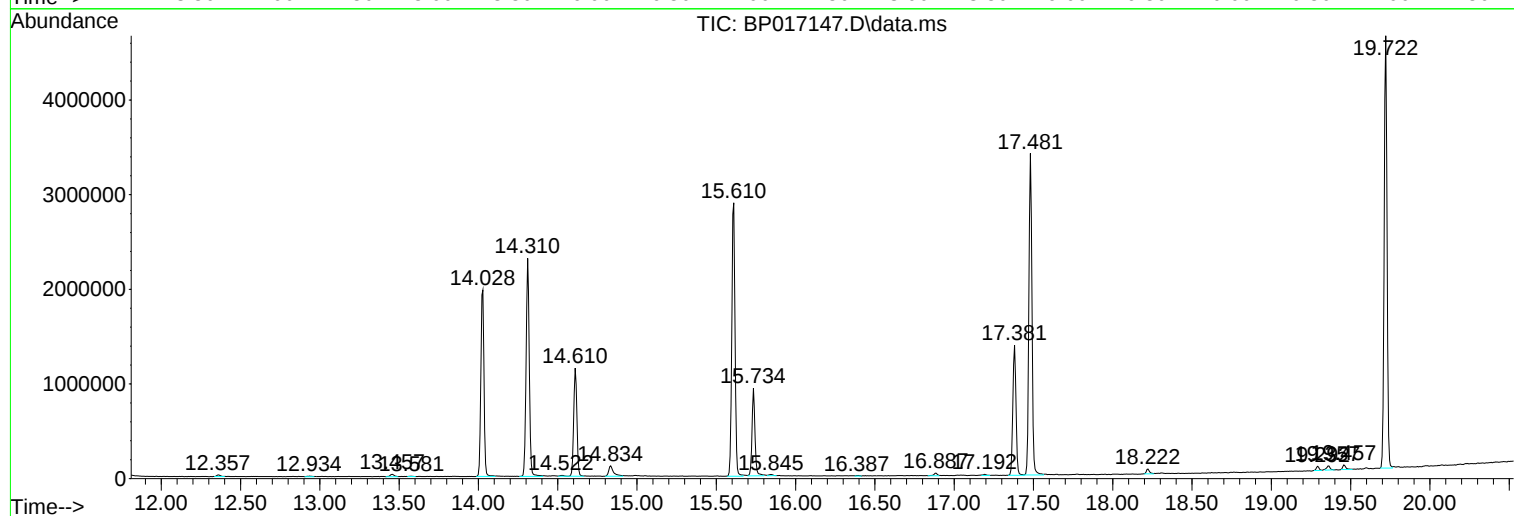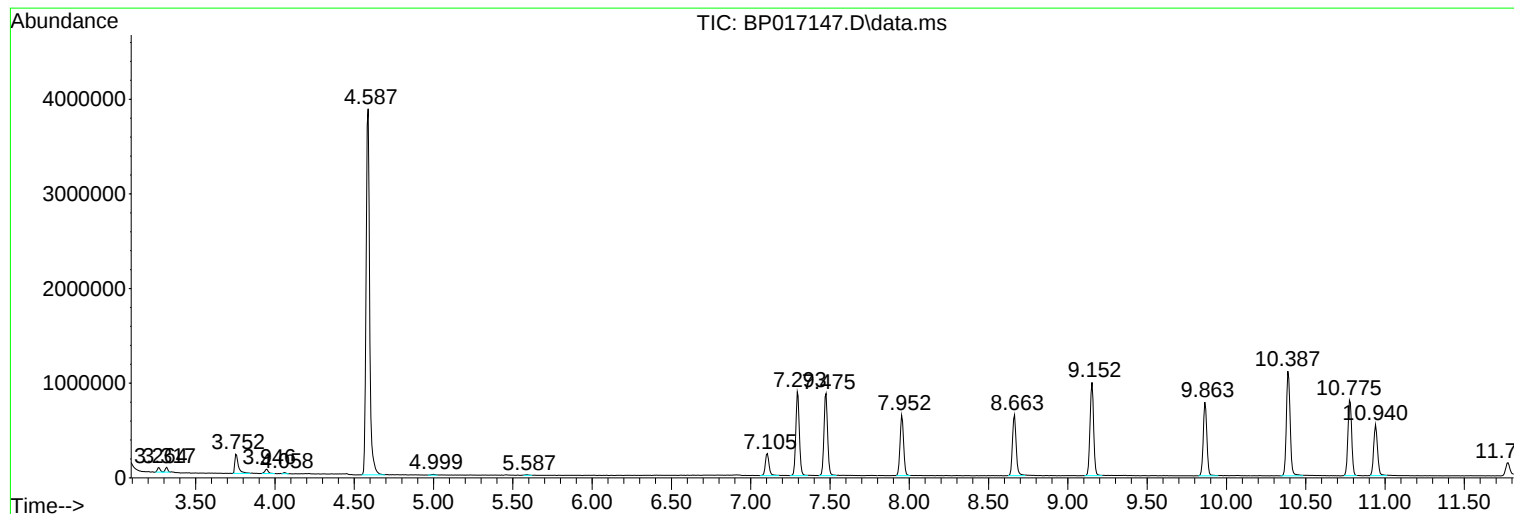

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017147.D
Acq On : 13 Sep 2023 13:58
Operator : MA/JU
Sample : 04324-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHF8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.587	119.13 ng/ul	5980270	1,4-Dichlorobenzene-d4	7.952

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

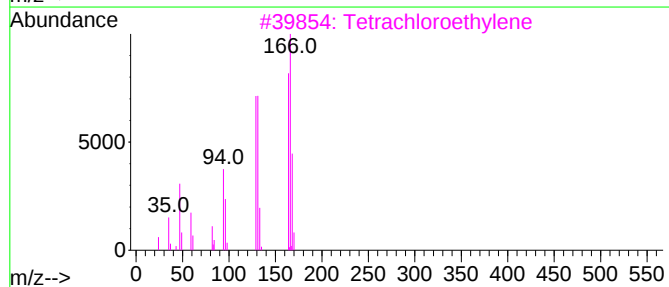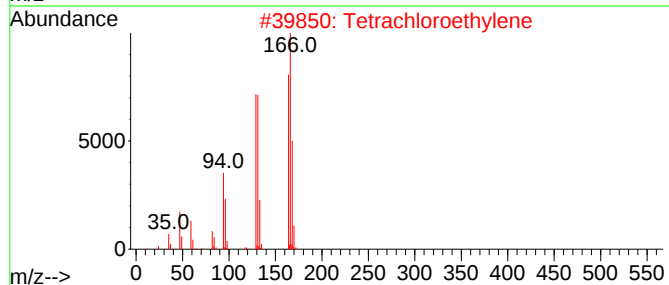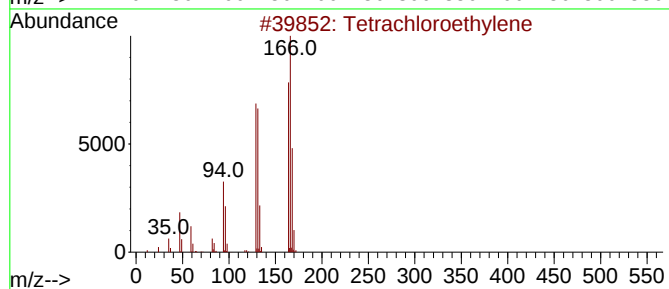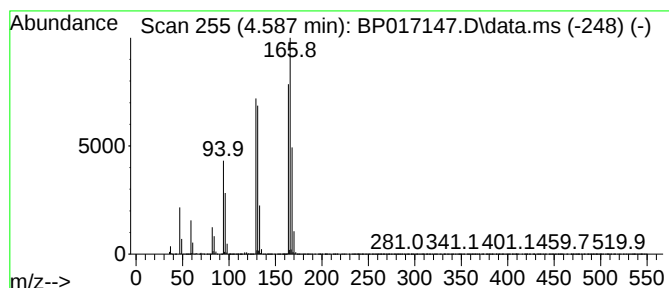

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017147.D
Acq On : 13 Sep 2023 13:58
Operator : MA/JU
Sample : 04324-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.587	119.1	ng/ul	5980270	1	7.952	1003960	20.0