

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017148.D
 Acq On : 13 Sep 2023 14:32
 Operator : MA/JU
 Sample : 04324-08
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	35	rBV	45864	59887	1.09%	0.116%
2	3.317	35	39	43	rVV	44609	51556	0.94%	0.100%
3	3.752	109	113	127	rBV	222273	340942	6.19%	0.662%
4	3.946	141	146	154	rVB	41248	65413	1.19%	0.127%
5	4.064	162	166	171	rVB	11258	17290	0.31%	0.034%
6	4.587	248	255	269	rBV	3678222	5510628	100.00%	10.700%
7	4.999	321	325	329	rBV5	5794	9747	0.18%	0.019%
8	5.587	421	425	429	rVB4	5658	9776	0.18%	0.019%
9	6.905	644	649	653	rBV8	4115	6950	0.13%	0.013%
10	7.105	676	683	691	rBV	194739	311058	5.64%	0.604%
11	7.293	709	715	724	rBV	777032	1207343	21.91%	2.344%
12	7.475	739	746	756	rBV	739488	1166981	21.18%	2.266%
13	7.952	821	827	839	rVB	658522	1031699	18.72%	2.003%
14	8.663	940	948	963	rBV	562160	923425	16.76%	1.793%
15	9.152	1023	1031	1044	rBV	900581	1422931	25.82%	2.763%
16	9.863	1143	1152	1161	rBV	706669	1133523	20.57%	2.201%
17	10.387	1233	1241	1254	rBV	1016636	1702898	30.90%	3.306%
18	10.781	1300	1308	1315	rBV	870143	1464359	26.57%	2.843%
19	10.940	1326	1335	1347	rBV	557501	944663	17.14%	1.834%
20	11.775	1470	1477	1487	rBV	106638	222309	4.03%	0.432%
21	12.363	1567	1577	1584	rBV	18658	31608	0.57%	0.061%
22	13.457	1756	1763	1769	rBV2	32847	53223	0.97%	0.103%
23	13.575	1777	1783	1786	rBV8	3443	6231	0.11%	0.012%
24	14.028	1853	1860	1867	rBV	2190979	2885656	52.37%	5.603%
25	14.310	1901	1908	1917	rBV	2255594	3206199	58.18%	6.225%
26	14.528	1940	1945	1951	rVB4	11395	18541	0.34%	0.036%
27	14.610	1953	1959	1967	rBV	1299788	1882465	34.16%	3.655%
28	14.834	1991	1997	2012	rBV	98182	203258	3.69%	0.395%
29	15.051	2031	2034	2041	rVB9	5480	7284	0.13%	0.014%
30	15.351	2082	2085	2091	rVB7	3948	6779	0.12%	0.013%
31	15.498	2107	2110	2115	rVB7	5647	7886	0.14%	0.015%
32	15.610	2120	2129	2144	rBV	3073464	4290079	77.85%	8.330%
33	15.734	2144	2150	2166	rVV	959909	1300135	23.59%	2.524%
34	15.845	2166	2169	2175	rVB4	15455	23774	0.43%	0.046%
35	16.881	2340	2345	2350	rBV3	26251	37823	0.69%	0.073%
36	17.039	2366	2372	2375	rBV6	5442	11956	0.22%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017148.D
Acq On : 13 Sep 2023 14:32
Operator : MA/JU
Sample : 04324-08
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHG0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION

37	17.192	2395	2398	2401	rVB5	7217	9724	0.18%	0.019%
38	17.381	2424	2430	2440	rBV	1542376	2119953	38.47%	4.116%
39	17.481	2441	2447	2460	rVV	3574702	4882198	88.60%	9.480%
40	18.222	2569	2573	2578	rBV2	41800	60247	1.09%	0.117%
41	19.292	2751	2755	2761	rBV3	36755	48403	0.88%	0.094%
42	19.357	2764	2766	2774	rVB	38997	50226	0.91%	0.098%
43	19.457	2780	2783	2787	rBV4	24906	31153	0.57%	0.060%
44	19.722	2822	2828	2834	rBV	4014138	5214656	94.63%	10.125%
45	21.480	3122	3127	3135	rBV	1297364	1708890	31.01%	3.318%
46	23.839	3521	3528	3539	rVB	2035072	4136480	75.06%	8.032%
47	24.004	3550	3556	3568	rVB	813988	1663707	30.19%	3.230%




Sum of corrected areas: 51501912

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017148.D
Acq On : 13 Sep 2023 14:32
Operator : MA/JU
Sample : 04324-08
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

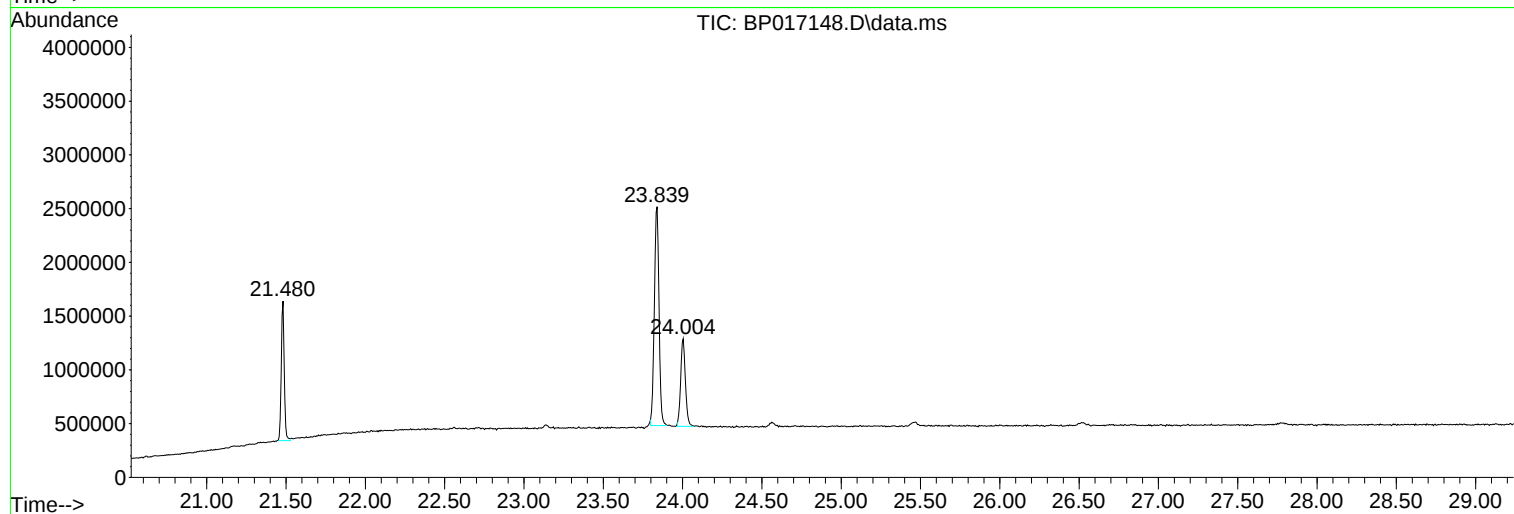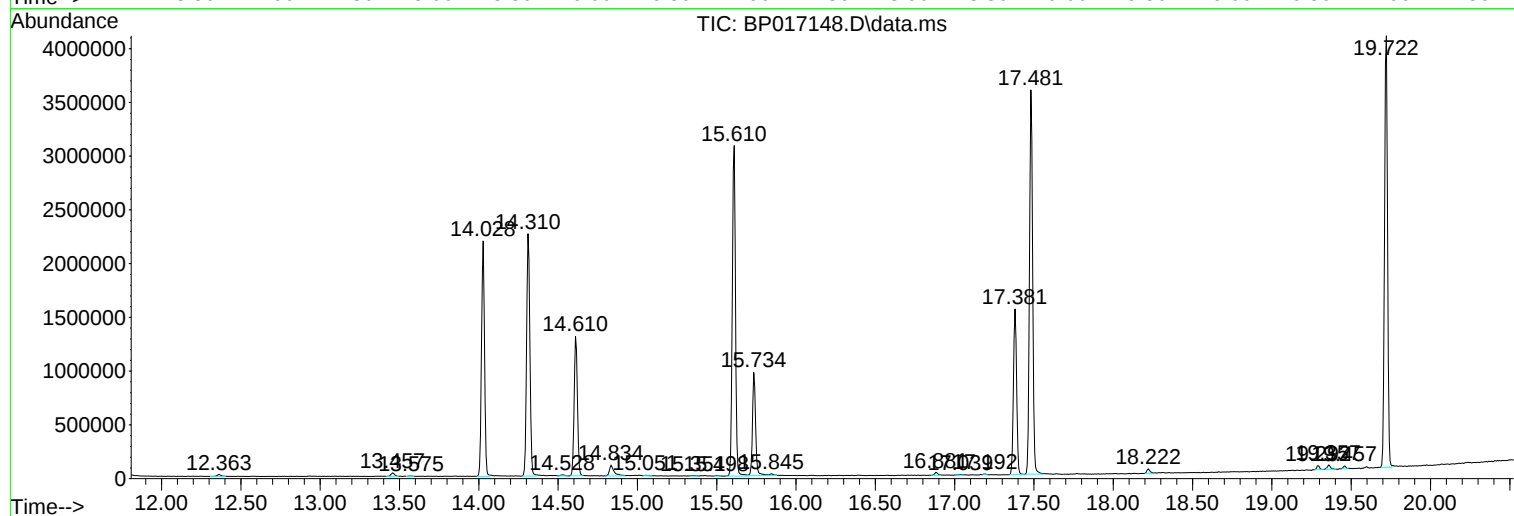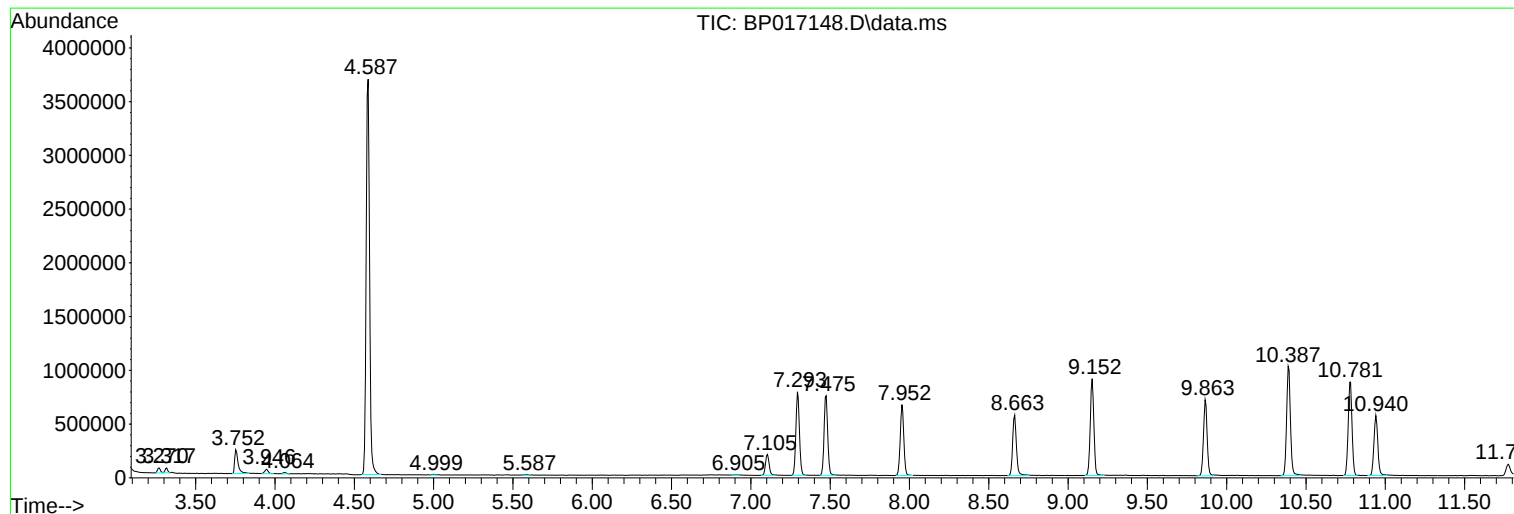

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017148.D
Acq On : 13 Sep 2023 14:32
Operator : MA/JU
Sample : 04324-08
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHG0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.587	106.83 ng/ul	5510630	1,4-Dichlorobenzene-d4	7.952

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	87
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

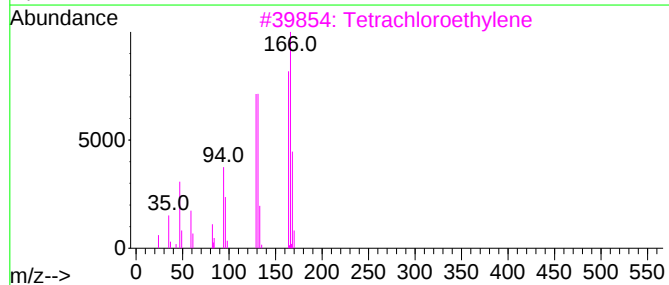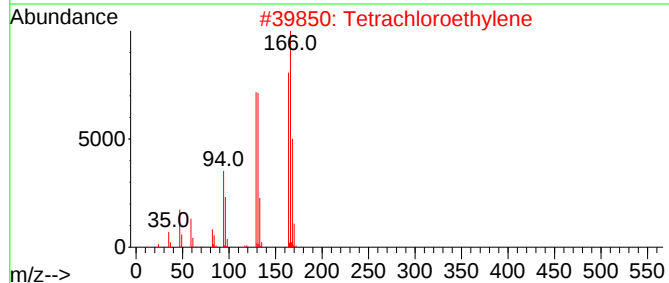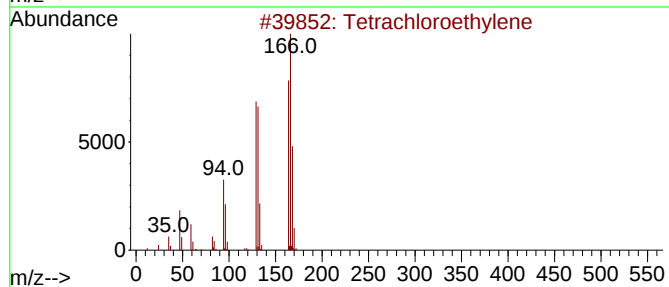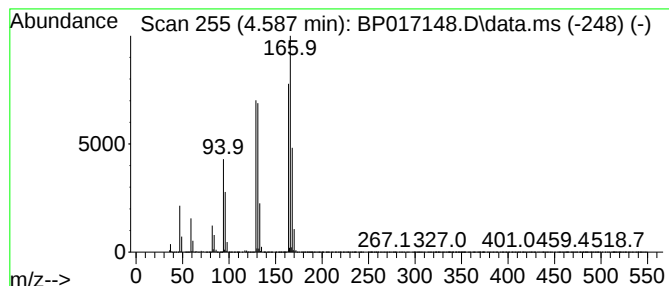

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017148.D
Acq On : 13 Sep 2023 14:32
Operator : MA/JU
Sample : 04324-08
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.587	106.8	ng/ul	5510630	1	7.952	1031700	20.0