

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017150.D
 Acq On : 13 Sep 2023 15:41
 Operator : MA/JU
 Sample : PB155390BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK390

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017150.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	49	rVB	67068	93655	2.11%	0.184%
2	3.746	108	112	126	rBV	678958	1025244	23.15%	2.010%
3	4.058	160	165	171	rVB2	20700	31297	0.71%	0.061%
4	6.905	646	649	652	rBV5	3294	4757	0.11%	0.009%
5	7.105	675	683	693	rBV	959663	1496084	33.78%	2.932%
6	7.293	708	715	727	rVB	793402	1228849	27.75%	2.409%
7	7.475	739	746	759	rBV	962305	1529991	34.55%	2.999%
8	7.952	819	827	835	rBV	898252	1388525	31.35%	2.722%
9	8.334	890	892	898	rBV5	3441	4970	0.11%	0.010%
10	8.663	941	948	959	rBV	1118267	1823500	41.17%	3.574%
11	9.152	1023	1031	1041	rBV	892338	1427749	32.24%	2.798%
12	9.863	1143	1152	1165	rBV	739717	1183195	26.72%	2.319%
13	10.387	1234	1241	1253	rBV	1109532	1838064	41.50%	3.603%
14	10.781	1299	1308	1315	rBV	1176060	1969566	44.47%	3.860%
15	10.940	1328	1335	1347	rBV	712334	1174965	26.53%	2.303%
16	12.357	1572	1576	1584	rVB2	17128	29440	0.66%	0.058%
17	13.457	1758	1763	1768	rVB7	8653	12757	0.29%	0.025%
18	13.575	1781	1783	1791	rVB8	4816	5671	0.13%	0.011%
19	14.028	1852	1860	1873	rBV	2026625	2758047	62.27%	5.406%
20	14.310	1901	1908	1917	rBV	2257979	3209091	72.46%	6.290%
21	14.610	1952	1959	1971	rBV	1759372	2571549	58.06%	5.040%
22	14.740	1980	1981	1990	rVB9	2925	4928	0.11%	0.010%
23	14.828	1990	1996	2015	rBV	682133	1164904	26.30%	2.283%
24	15.610	2121	2129	2140	rBV	2971657	4139500	93.47%	8.114%
25	15.734	2144	2150	2163	rVV	794310	1086213	24.53%	2.129%
26	15.845	2165	2169	2176	rVB2	14720	26475	0.60%	0.052%
27	17.045	2370	2373	2374	rBV3	4741	5734	0.13%	0.011%
28	17.169	2389	2394	2398	rBV6	7012	13860	0.31%	0.027%
29	17.381	2422	2430	2438	rBV	2143159	2954684	66.71%	5.791%
30	17.481	2441	2447	2459	rVV2	3103104	4240808	95.75%	8.312%
31	17.781	2494	2498	2502	rBV7	3370	5525	0.12%	0.011%
32	18.222	2570	2573	2577	rBV6	5416	8818	0.20%	0.017%
33	19.292	2751	2755	2760	rBV4	33776	41969	0.95%	0.082%
34	19.363	2763	2767	2771	rVB	26223	38062	0.86%	0.075%
35	19.722	2822	2828	2835	rBV	3565593	4428871	100.00%	8.681%
36	21.480	3122	3127	3134	rBV	1828651	2395687	54.09%	4.696%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017150.D
Acq On : 13 Sep 2023 15:41
Operator : MA/JU
Sample : PB155390BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK390

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION

37	23.839	3521	3528	3539	rVB2	1674541	3368900	76.07%	6.603%
38	24.004	3550	3556	3568	rVB	1119751	2287589	51.65%	4.484%




Sum of corrected areas: 51019493

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017150.D
Acq On : 13 Sep 2023 15:41
Operator : MA/JU
Sample : PB155390BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

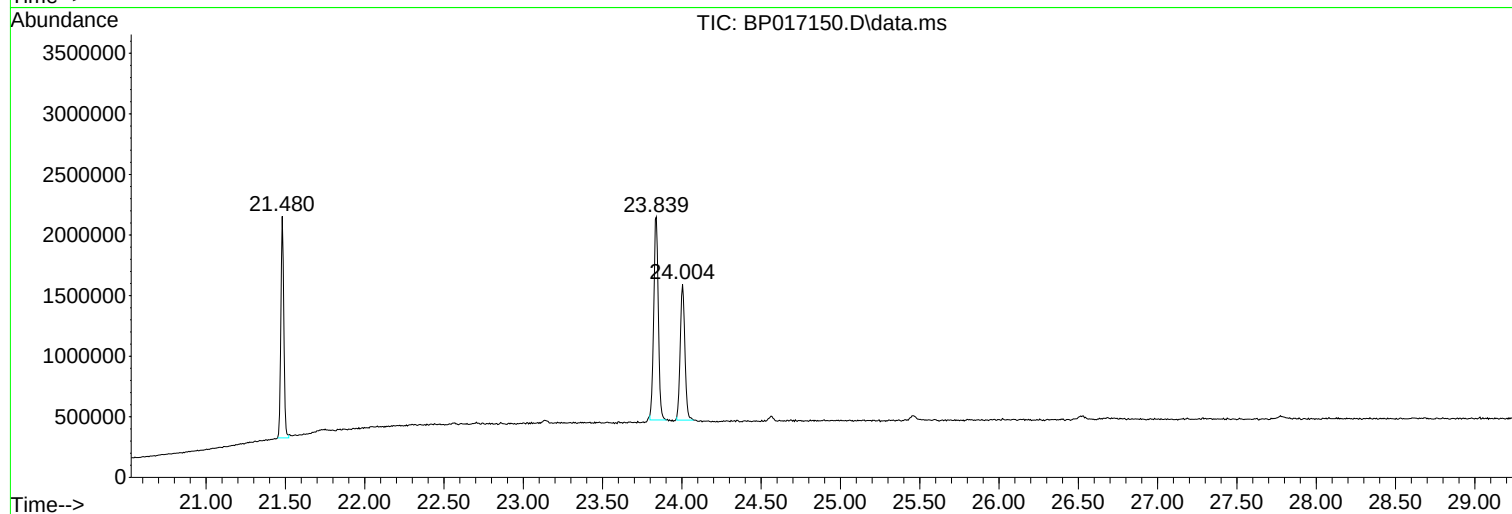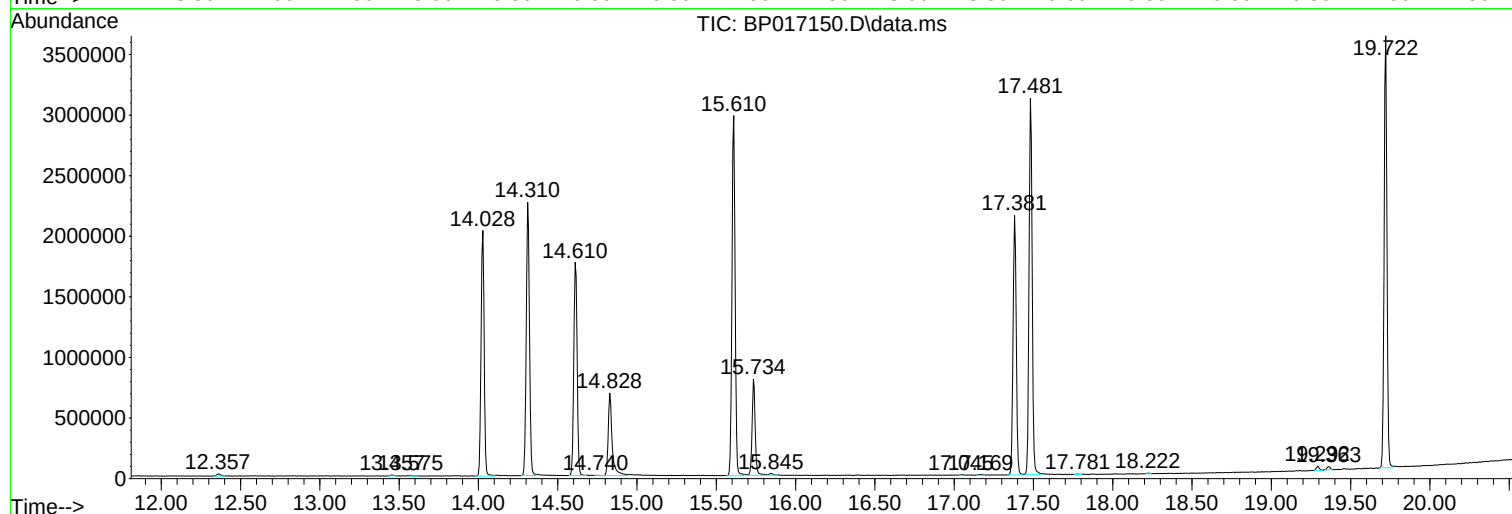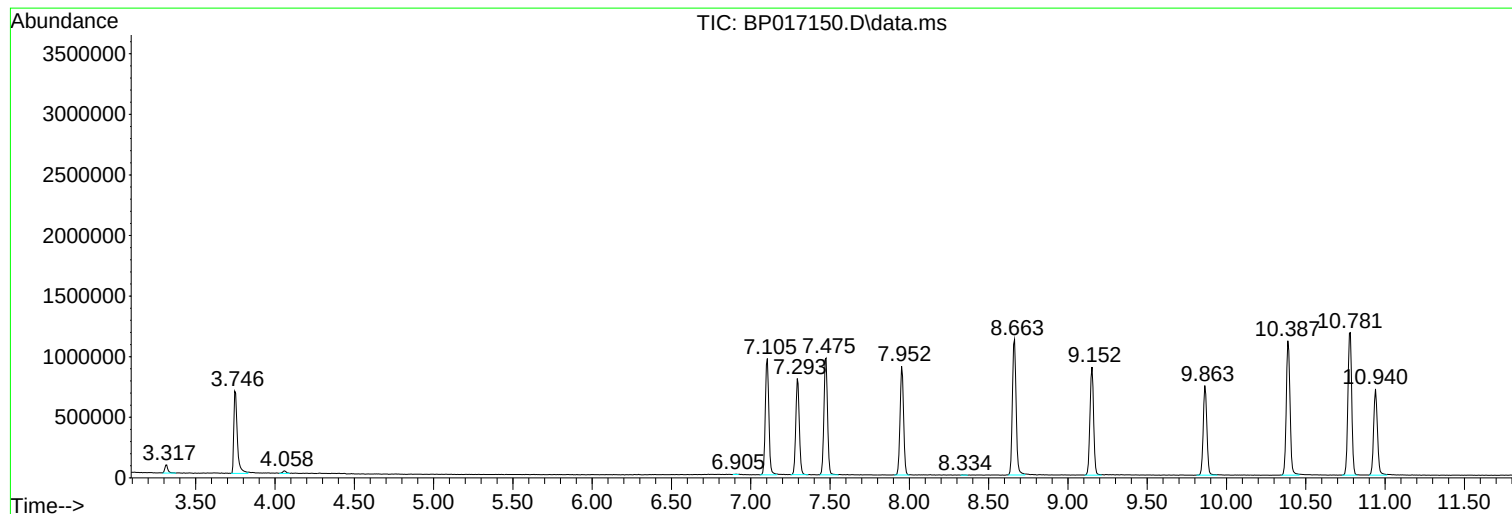

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017150.D
Acq On : 13 Sep 2023 15:41
Operator : MA/JU
Sample : PB155390BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017150.D
Acq On : 13 Sep 2023 15:41
Operator : MA/JU
Sample : PB155390BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------