

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017156.D
 Acq On : 13 Sep 2023 19:09
 Operator : MA/JU
 Sample : 04324-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017156.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	35	rBV3	24981	33859	0.53%	0.060%
2	3.311	35	38	43	rVV	40033	49867	0.78%	0.088%
3	3.752	109	113	128	rBV	244471	392426	6.15%	0.690%
4	3.946	141	146	154	rVB	36910	59317	0.93%	0.104%
5	4.058	162	165	172	rVB3	12067	18111	0.28%	0.032%
6	4.587	248	255	267	rBV	3411021	5310548	83.25%	9.335%
7	4.999	321	325	331	rBV4	6703	10300	0.16%	0.018%
8	5.587	422	425	430	rVB3	7542	10291	0.16%	0.018%
9	6.910	643	650	658	rVB3	5338	15320	0.24%	0.027%
10	7.105	676	683	691	rBV	202787	330143	5.18%	0.580%
11	7.293	707	715	726	rBV	730332	1128378	17.69%	1.984%
12	7.469	739	745	755	rBV	695263	1124263	17.62%	1.976%
13	7.952	818	827	836	rBV	666484	1032442	16.18%	1.815%
14	8.663	940	948	960	rBV	566976	933680	14.64%	1.641%
15	9.151	1023	1031	1040	rBV	838738	1352771	21.21%	2.378%
16	9.357	1063	1066	1072	rVB8	4256	7520	0.12%	0.013%
17	9.863	1145	1152	1163	rBV	667067	1058533	16.59%	1.861%
18	10.063	1181	1186	1192	rVB10	4022	7378	0.12%	0.013%
19	10.387	1234	1241	1254	rBV	987049	1661626	26.05%	2.921%
20	10.775	1300	1307	1316	rBV	901105	1506147	23.61%	2.648%
21	10.940	1328	1335	1344	rBV	546936	920053	14.42%	1.617%
22	11.540	1431	1437	1442	rBV10	3528	8376	0.13%	0.015%
23	11.775	1470	1477	1486	rBV	159157	301369	4.72%	0.530%
24	12.363	1570	1577	1584	rBV	17665	30509	0.48%	0.054%
25	13.363	1744	1747	1754	rVB7	4188	7963	0.12%	0.014%
26	13.457	1757	1763	1769	rBV3	22016	40984	0.64%	0.072%
27	14.028	1852	1860	1871	rBV	2021789	2737861	42.92%	4.813%
28	14.310	1901	1908	1926	rBV	2259456	3187474	49.97%	5.603%
29	14.528	1941	1945	1951	rVB4	9104	13060	0.20%	0.023%
30	14.610	1952	1959	1971	rVB	1432819	2055416	32.22%	3.613%
31	14.834	1990	1997	2014	rBV	134603	279597	4.38%	0.492%
32	14.986	2020	2023	2031	rVV7	17407	27760	0.44%	0.049%
33	15.057	2031	2035	2039	rVB7	4396	6735	0.11%	0.012%
34	15.504	2104	2111	2116	rBV7	4065	7974	0.12%	0.014%
35	15.610	2120	2129	2143	rBV	2902710	4231828	66.34%	7.439%
36	15.733	2144	2150	2163	rVV	988691	1300930	20.39%	2.287%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017156.D
 Acq On : 13 Sep 2023 19:09
 Operator : MA/JU
 Sample : 04324-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	15.845	2166	2169	2174	rVB4	14575	18978	0.30%	0.033%
38	16.392	2259	2262	2267	rVB7	5204	7443	0.12%	0.013%
39	16.886	2342	2346	2349	rBV4	13595	17410	0.27%	0.031%
40	17.051	2372	2374	2380	rVB7	6601	7648	0.12%	0.013%
41	17.104	2380	2383	2390	rBV8	3921	10418	0.16%	0.018%
42	17.175	2390	2395	2396	rBV5	4153	6755	0.11%	0.012%
43	17.380	2423	2430	2439	rBV	1826358	2559691	40.12%	4.500%
44	17.480	2441	2447	2461	rVV	3801025	5002948	78.42%	8.795%
45	17.769	2493	2496	2500	rBV6	6601	11569	0.18%	0.020%
46	17.963	2526	2529	2533	rBV6	5061	7162	0.11%	0.013%
47	18.222	2569	2573	2580	rBV	89017	126338	1.98%	0.222%
48	19.292	2751	2755	2758	rBV	45969	56522	0.89%	0.099%
49	19.357	2762	2766	2775	rVB2	53341	89493	1.40%	0.157%
50	19.457	2779	2783	2791	rBV3	69816	96806	1.52%	0.170%
51	19.721	2822	2828	2835	rBV	4901204	6379299	100.00%	11.214%
52	21.480	3122	3127	3135	rBV	2181657	2760046	43.27%	4.852%
53	23.839	3521	3528	3541	rVB	2943188	5874917	92.09%	10.328%
54	24.004	3549	3556	3568	rVB	1250246	2651783	41.57%	4.662%




Sum of corrected areas: 56886035

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017156.D
Acq On : 13 Sep 2023 19:09
Operator : MA/JU
Sample : 04324-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHW8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

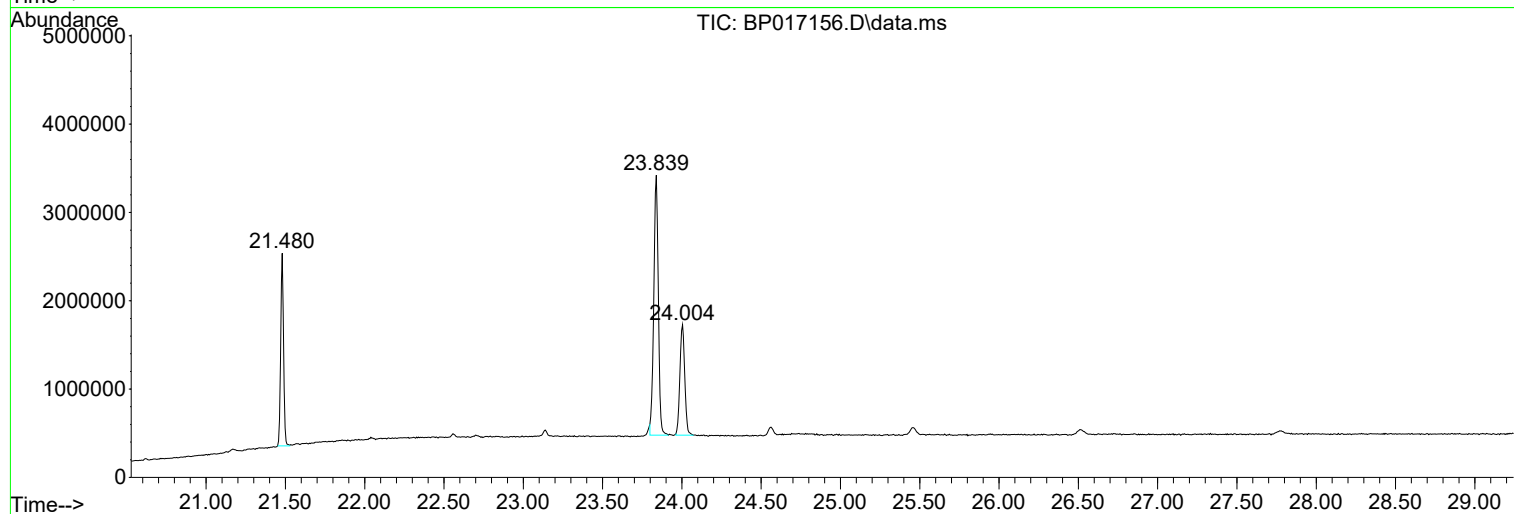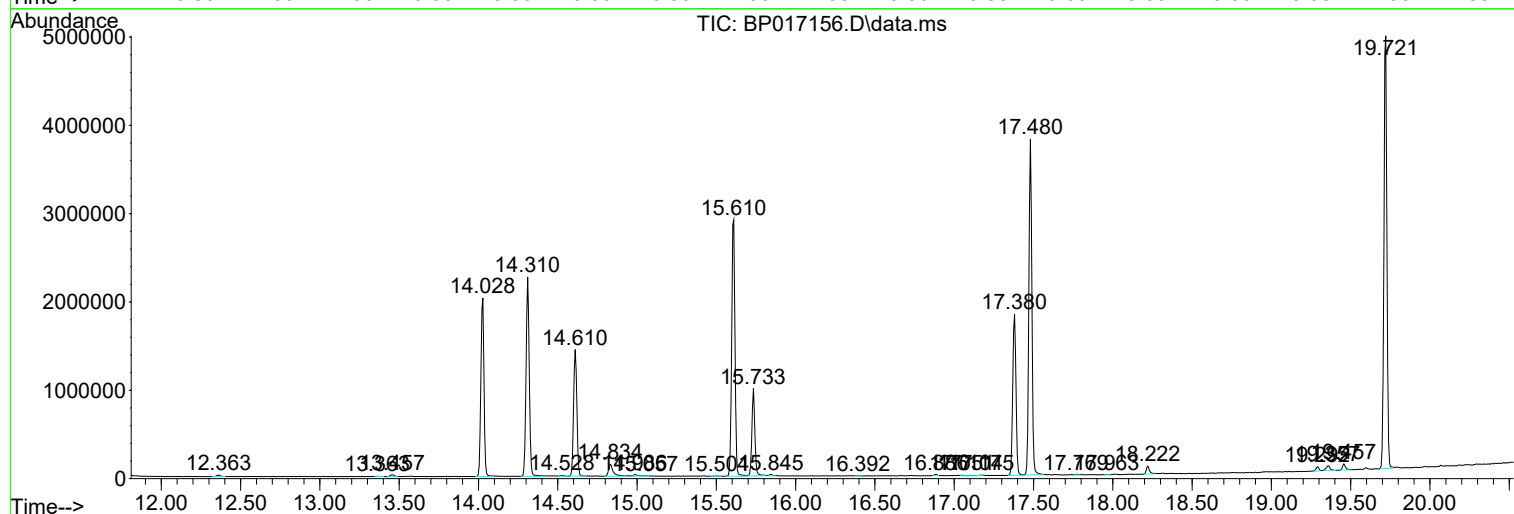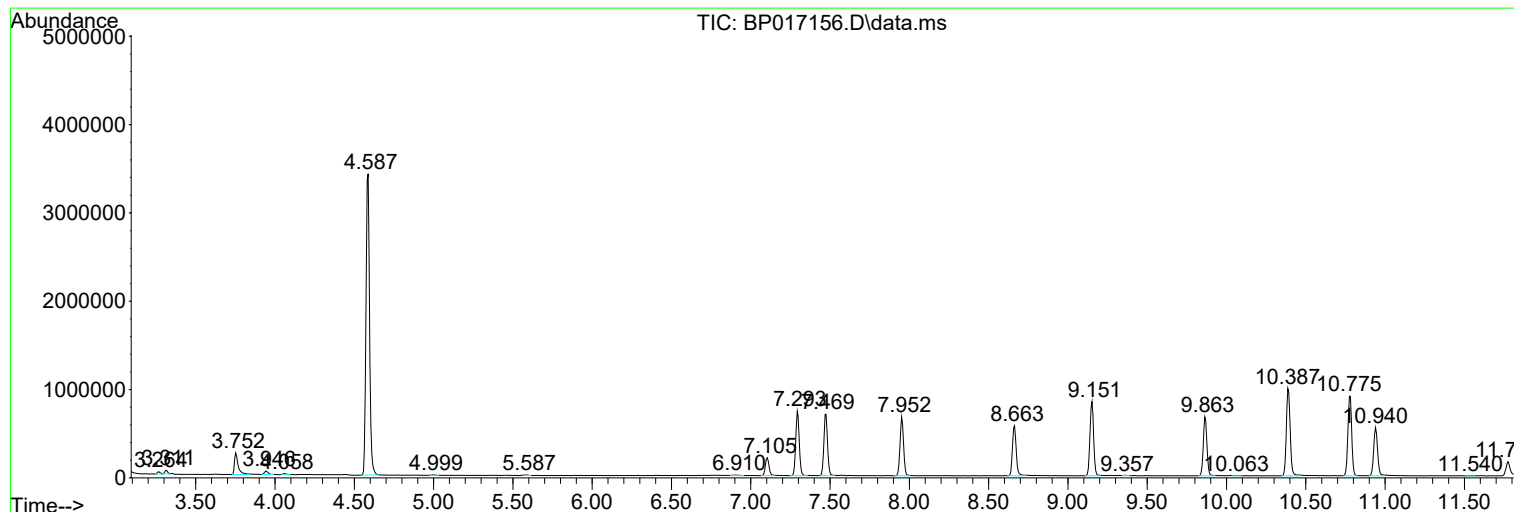

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017156.D
Acq On : 13 Sep 2023 19:09
Operator : MA/JU
Sample : 04324-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHW8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.587	102.87 ng/ul	5310550	1,4-Dichlorobenzene-d4	7.952

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	64
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

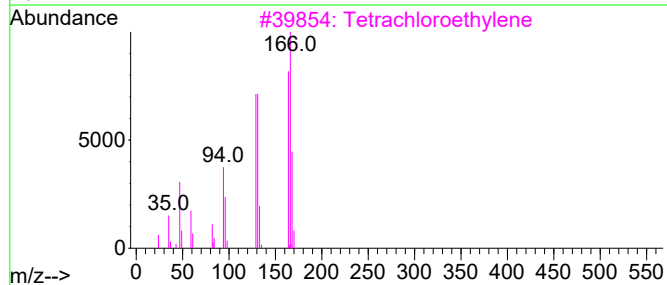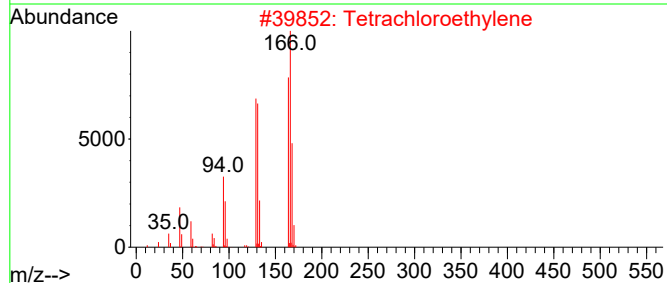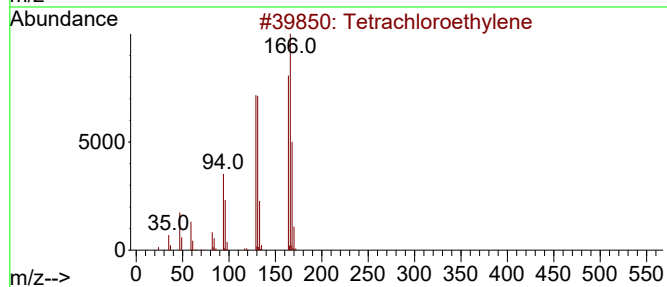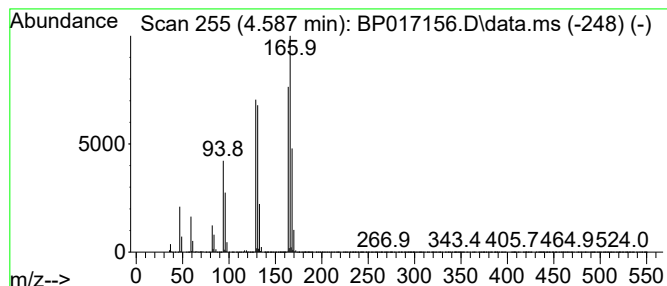

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017156.D
Acq On : 13 Sep 2023 19:09
Operator : MA/JU
Sample : 04324-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHW8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.587	102.9	ng/ul	5310550	1	7.952	1032440	20.0