

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017157.D
 Acq On : 13 Sep 2023 19:44
 Operator : MA/JU
 Sample : 04324-18
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017157.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	35	rBV	53665	82042	0.69%	0.116%
2	3.311	35	38	42	rVV	52430	68844	0.58%	0.098%
3	3.346	42	44	51	rVB	21571	28336	0.24%	0.040%
4	3.752	109	113	127	rBV	287025	474606	3.98%	0.674%
5	3.946	141	146	154	rVB	44292	75300	0.63%	0.107%
6	4.058	162	165	172	rVB2	11550	17622	0.15%	0.025%
7	4.440	228	230	235	rVB6	9700	14881	0.12%	0.021%
8	4.581	248	254	272	rVB	7342171	11932647	100.00%	16.941%
9	4.999	320	325	329	rBV3	8429	12925	0.11%	0.018%
10	7.099	676	682	694	rBV	256515	416196	3.49%	0.591%
11	7.293	708	715	725	rBV	876953	1327716	11.13%	1.885%
12	7.469	737	745	754	rBV	843226	1343041	11.26%	1.907%
13	7.952	820	827	835	rBV	698922	1083263	9.08%	1.538%
14	8.658	940	947	958	rBV	675045	1126932	9.44%	1.600%
15	9.152	1021	1031	1042	rBV	993359	1596846	13.38%	2.267%
16	9.863	1144	1152	1161	rBV	786764	1257210	10.54%	1.785%
17	10.387	1231	1241	1254	rBV	1173756	1925928	16.14%	2.734%
18	10.775	1300	1307	1316	rBV	966165	1581743	13.26%	2.246%
19	10.940	1327	1335	1346	rBV	611556	1026224	8.60%	1.457%
20	11.775	1471	1477	1487	rBV	51073	115315	0.97%	0.164%
21	12.357	1570	1576	1582	rBV	20657	34362	0.29%	0.049%
22	13.457	1758	1763	1769	rBV2	20157	36901	0.31%	0.052%
23	14.028	1852	1860	1873	rBV	2238597	3125445	26.19%	4.437%
24	14.310	1901	1908	1919	rBV	2567178	3651266	30.60%	5.184%
25	14.610	1951	1959	1967	rBV	1489948	2104403	17.64%	2.988%
26	14.834	1989	1997	2012	rBV	170906	352496	2.95%	0.500%
27	15.610	2121	2129	2140	rBV	3348542	4849926	40.64%	6.885%
28	15.734	2144	2150	2164	rVV	1171561	1501113	12.58%	2.131%
29	15.845	2165	2169	2175	rVB2	16172	25931	0.22%	0.037%
30	16.881	2342	2345	2354	rVB8	13172	18779	0.16%	0.027%
31	17.381	2423	2430	2440	rBV	1924282	2656395	22.26%	3.771%
32	17.481	2440	2447	2462	rVV2	4274824	5844245	48.98%	8.297%
33	18.222	2568	2573	2582	rBV3	62555	108887	0.91%	0.155%
34	19.292	2751	2755	2760	rBV2	51218	65917	0.55%	0.094%
35	19.357	2762	2766	2774	rVB	51362	84472	0.71%	0.120%
36	19.457	2780	2783	2787	rBV4	40185	47177	0.40%	0.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017157.D
Acq On : 13 Sep 2023 19:44
Operator : MA/JU
Sample : 04324-18
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJG0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION

37	19.722	2822	2828	2834	rBV	5905907	7365080	61.72%	10.456%
38	21.480	3122	3127	3134	rBV	2358560	2941376	24.65%	4.176%
39	23.839	3521	3528	3544	rVB2	3575332	7187828	60.24%	10.204%
40	24.004	3549	3556	3569	rVB	1396174	2928344	24.54%	4.157%




Sum of corrected areas: 70437960

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017157.D
Acq On : 13 Sep 2023 19:44
Operator : MA/JU
Sample : 04324-18
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

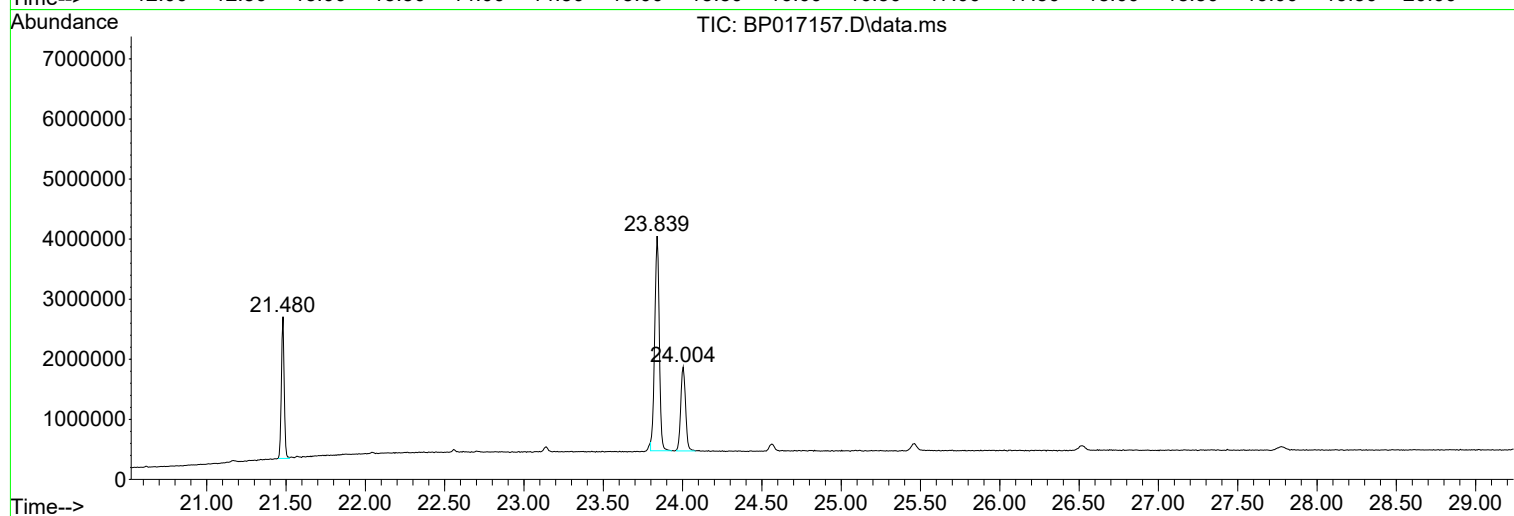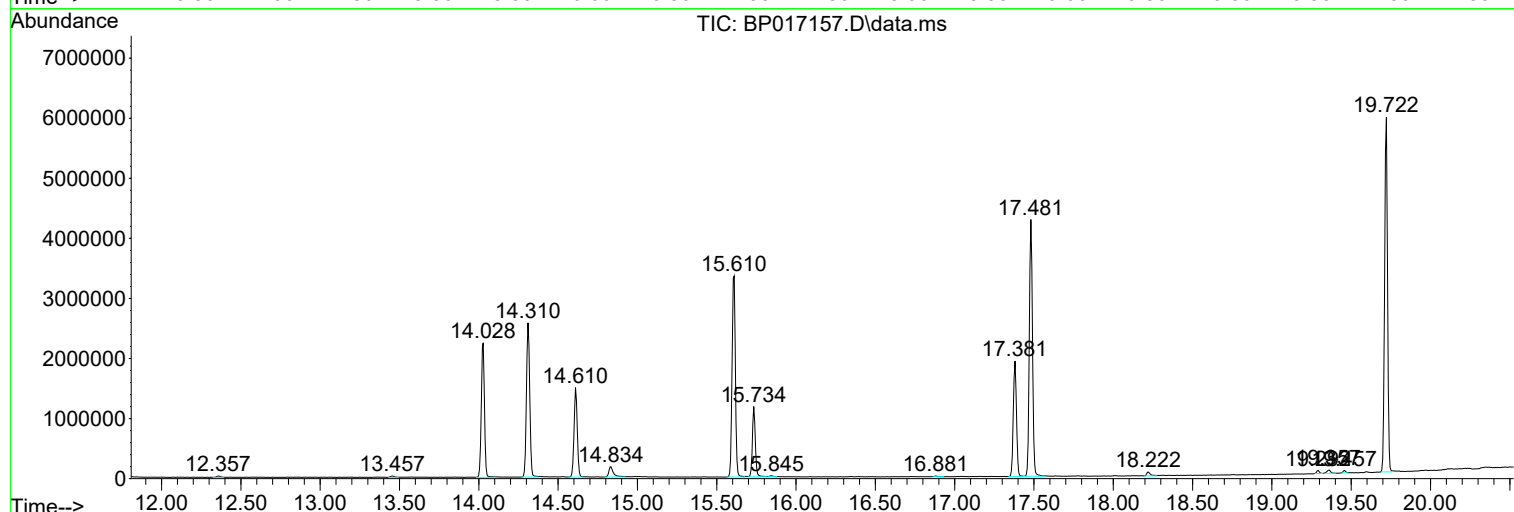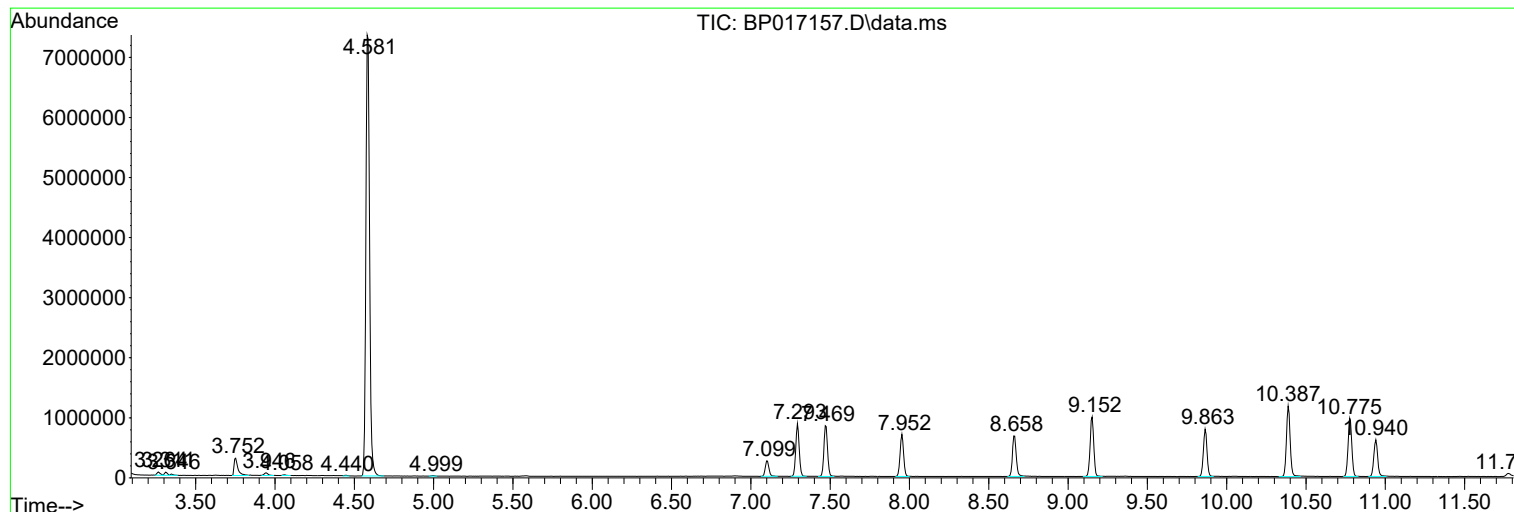

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017157.D
Acq On : 13 Sep 2023 19:44
Operator : MA/JU
Sample : 04324-18
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJG0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.581	220.31 ng/ul	11932600	1,4-Dichlorobenzene-d4	7.952

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	35

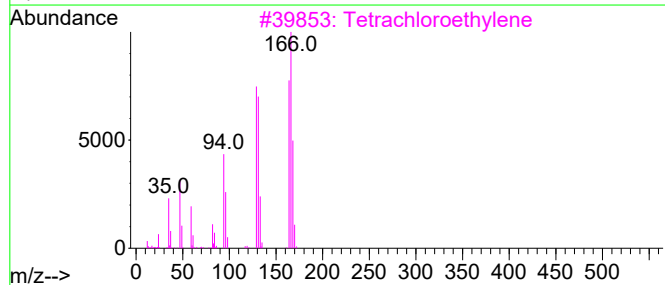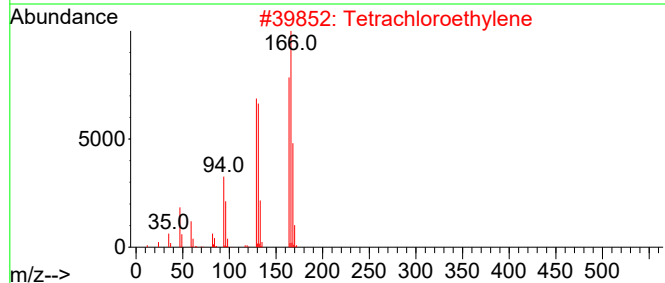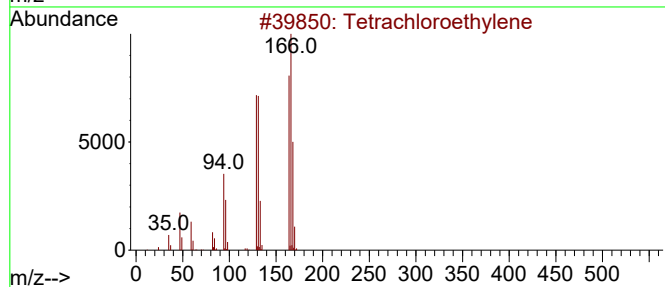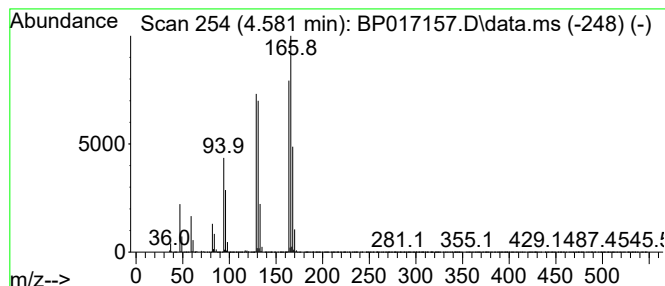

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017157.D
Acq On : 13 Sep 2023 19:44
Operator : MA/JU
Sample : 04324-18
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.581	220.3	ng/ul	11932600	1	7.952	1083260	20.0