

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017161.D
 Acq On : 13 Sep 2023 22:02
 Operator : MA/JU
 Sample : PB155240BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK240

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017161.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	34	38	44	rBV	70564	87802	1.34%	0.136%
2	3.746	108	112	126	rBV	611412	936992	14.35%	1.452%
3	4.058	161	165	170	rBV2	13359	18354	0.28%	0.028%
4	6.411	559	565	570	rBV8	3293	8030	0.12%	0.012%
5	7.099	675	682	693	rBV	1052727	1657305	25.38%	2.569%
6	7.293	709	715	726	rVB	895341	1347988	20.64%	2.089%
7	7.469	738	745	755	rBV	1090369	1675249	25.66%	2.596%
8	7.952	820	827	834	rBV	956657	1455061	22.28%	2.255%
9	8.658	940	947	960	rBV	1266391	2052527	31.43%	3.181%
10	9.152	1022	1031	1040	rBV	1003027	1611874	24.68%	2.498%
11	9.863	1143	1152	1161	rBV	849549	1341120	20.54%	2.079%
12	10.387	1232	1241	1258	rBV	1287424	2110731	32.32%	3.271%
13	10.775	1300	1307	1316	rBV	1304970	2129334	32.61%	3.300%
14	10.940	1326	1335	1352	rBV	893185	1517990	23.25%	2.353%
15	12.357	1571	1576	1582	rVB2	20203	33331	0.51%	0.052%
16	13.457	1756	1763	1768	rBV	29006	48807	0.75%	0.076%
17	13.569	1776	1782	1787	rBV8	6294	11151	0.17%	0.017%
18	14.028	1852	1860	1871	rBV	2396857	3340658	51.16%	5.178%
19	14.310	1901	1908	1917	rBV	2719853	3822615	58.54%	5.925%
20	14.610	1953	1959	1974	rBV	2044128	2928480	44.85%	4.539%
21	14.828	1988	1996	2013	rBV	943971	1559794	23.89%	2.418%
22	15.010	2025	2027	2032	rVB6	6083	8248	0.13%	0.013%
23	15.416	2090	2096	2100	rBV9	3879	7963	0.12%	0.012%
24	15.604	2122	2128	2138	rBV	3568079	4958711	75.94%	7.686%
25	15.734	2144	2150	2165	rBV	1071880	1407301	21.55%	2.181%
26	15.845	2165	2169	2174	rVB2	16650	23366	0.36%	0.036%
27	17.045	2370	2373	2378	rVB7	4899	6638	0.10%	0.010%
28	17.169	2389	2394	2398	rBV7	5586	10506	0.16%	0.016%
29	17.381	2423	2430	2440	rBV	2693143	3661897	56.08%	5.676%
30	17.481	2440	2447	2463	rVV	4022711	5547393	84.96%	8.598%
31	19.292	2751	2755	2760	rBV3	42455	56931	0.87%	0.088%
32	19.357	2763	2766	2771	rVB2	36638	49792	0.76%	0.077%
33	19.457	2781	2783	2788	rBV6	10846	10305	0.16%	0.016%
34	19.716	2822	2827	2839	rBV	5036066	6529773	100.00%	10.121%
35	21.480	3122	3127	3138	rBV	2934836	3719185	56.96%	5.764%
36	23.839	3521	3528	3542	rVB2	2711448	5505307	84.31%	8.533%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017161.D
Acq On : 13 Sep 2023 22:02
Operator : MA/JU
Sample : PB155240BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK240

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION

37 24.004 3549 3556 3567 rVB 1602810 3321674 50.87% 5.148%




Sum of corrected areas: 64520183

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017161.D
Acq On : 13 Sep 2023 22:02
Operator : MA/JU
Sample : PB155240BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK240

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

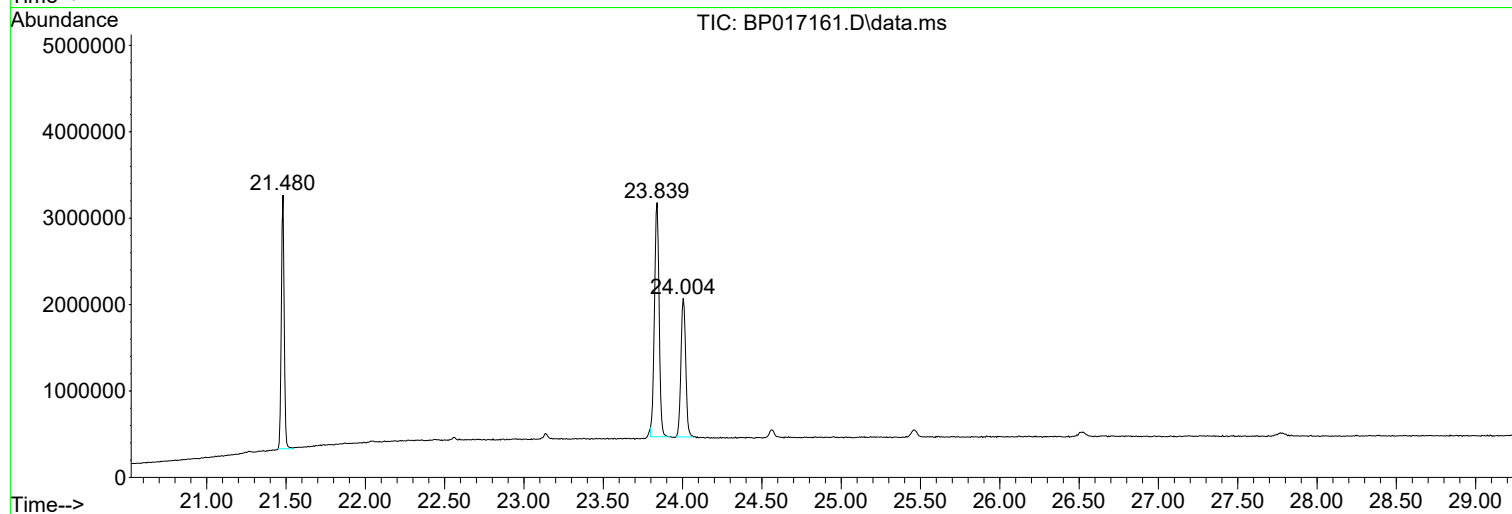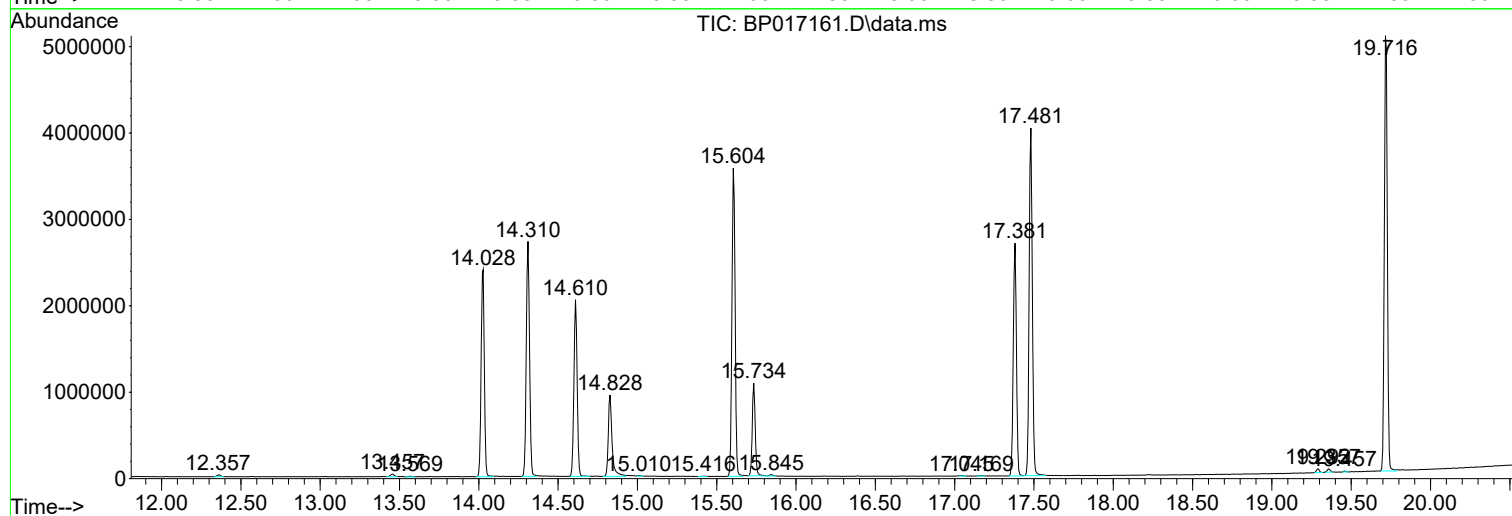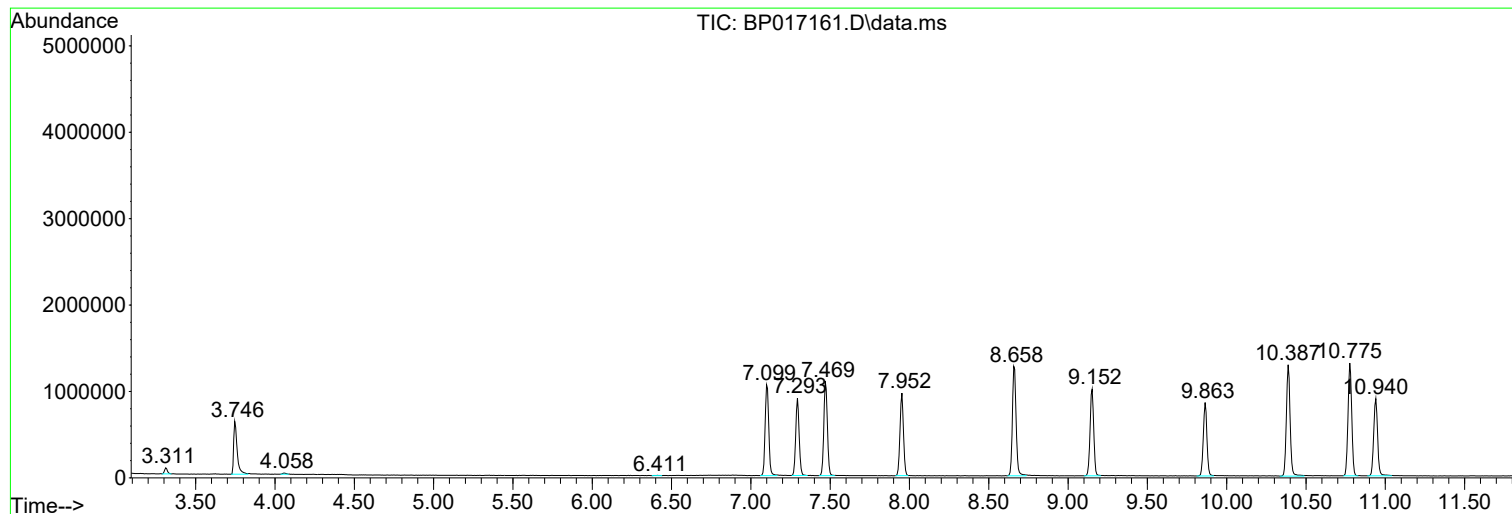

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017161.D
Acq On : 13 Sep 2023 22:02
Operator : MA/JU
Sample : PB155240BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK240

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017161.D
Acq On : 13 Sep 2023 22:02
Operator : MA/JU
Sample : PB155240BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK240

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------