

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017168.D
 Acq On : 14 Sep 2023 09:59
 Operator : MA/JU
 Sample : PB155343BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK343

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	33	37	42	rVB	58947	77072	1.20%	0.125%
2	3.740	107	111	129	rBV	497423	833008	12.92%	1.352%
3	4.046	160	163	169	rVB4	12550	19859	0.31%	0.032%
4	6.881	644	645	653	rVB6	5534	9171	0.14%	0.015%
5	7.087	674	680	689	rBV	916942	1474796	22.87%	2.393%
6	7.281	706	713	724	rVB	792659	1206850	18.72%	1.959%
7	7.457	736	743	751	rBV	960326	1491048	23.12%	2.420%
8	7.940	818	825	838	rVB	771800	1185477	18.39%	1.924%
9	8.652	937	946	961	rBV	1181083	1886350	29.26%	3.061%
10	9.140	1019	1029	1036	rBV	911320	1447556	22.45%	2.349%
11	9.857	1142	1151	1164	rBV	747511	1228766	19.06%	1.994%
12	10.381	1232	1240	1252	rBV	1164654	1908237	29.60%	3.097%
13	10.769	1298	1306	1313	rBV	1104917	1767959	27.42%	2.869%
14	10.934	1326	1334	1342	rBV	800607	1348469	20.91%	2.188%
15	12.357	1571	1576	1583	rVB	20036	34713	0.54%	0.056%
16	13.404	1745	1754	1755	rBV9	9835	17590	0.27%	0.029%
17	13.451	1758	1762	1768	rVV6	14307	30687	0.48%	0.050%
18	13.569	1780	1782	1786	rVB5	5851	6672	0.10%	0.011%
19	14.028	1852	1860	1867	rBV	2305605	3120125	48.39%	5.063%
20	14.310	1901	1908	1918	rBV	2522540	3594037	55.74%	5.833%
21	14.610	1952	1959	1967	rBV	1728605	2522571	39.12%	4.094%
22	14.834	1991	1997	2018	rBV	876381	1488844	23.09%	2.416%
23	15.198	2054	2059	2060	rBV5	5841	9015	0.14%	0.015%
24	15.363	2077	2087	2088	rBV3	32601	90921	1.41%	0.148%
25	15.610	2122	2129	2143	rBV	3339298	4651058	72.13%	7.548%
26	15.739	2145	2151	2165	rVV	871962	1221640	18.95%	1.983%
27	15.845	2165	2169	2183	rVB4	33039	93135	1.44%	0.151%
28	16.069	2202	2207	2213	rVV6	11810	24043	0.37%	0.039%
29	16.510	2277	2282	2288	rVB3	11014	18930	0.29%	0.031%
30	16.663	2301	2308	2316	rVB	80206	147831	2.29%	0.240%
31	17.057	2369	2375	2380	rBV6	21423	42886	0.67%	0.070%
32	17.386	2424	2431	2437	rBV	2282594	3210890	49.80%	5.211%
33	17.486	2441	2448	2464	rVV	3755837	5325582	82.60%	8.643%
34	17.622	2467	2471	2476	rVB6	11080	16158	0.25%	0.026%
35	17.745	2487	2492	2496	rBV	85481	111458	1.73%	0.181%
36	18.010	2532	2537	2543	rBV10	12300	24951	0.39%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017168.D
 Acq On : 14 Sep 2023 09:59
 Operator : MA/JU
 Sample : PB155343BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK343

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	18.092	2548	2551	2558	rBV4	14539	30019	0.47%	0.049%
38	18.227	2571	2574	2585	rVB4	13465	37342	0.58%	0.061%
39	18.563	2629	2631	2637	rBV7	12216	22243	0.34%	0.036%
40	18.663	2644	2648	2656	rVB	84646	107599	1.67%	0.175%
41	18.769	2663	2666	2672	rVB6	16033	25997	0.40%	0.042%
42	19.298	2752	2756	2762	rBV2	46005	58146	0.90%	0.094%
43	19.369	2764	2768	2775	rVV2	45916	84126	1.30%	0.137%
44	19.439	2776	2780	2783	rBV	82685	97775	1.52%	0.159%
45	19.727	2823	2829	2834	rBV	5059929	6447807	100.00%	10.464%
46	20.116	2891	2895	2900	rVB	96984	110184	1.71%	0.179%
47	20.727	2996	2999	3004	rVB	113234	132299	2.05%	0.215%
48	21.292	3092	3095	3099	rVB2	118152	136306	2.11%	0.221%
49	21.486	3123	3128	3138	rBV	2533791	3537994	54.87%	5.742%
50	21.851	3187	3190	3194	rBV	99497	116771	1.81%	0.190%
51	23.857	3524	3531	3539	rBV2	2917716	5547941	86.04%	9.003%
52	24.021	3552	3559	3571	rVB	1600511	3439131	53.34%	5.581%




Sum of corrected areas: 61620035

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017168.D
Acq On : 14 Sep 2023 09:59
Operator : MA/JU
Sample : PB155343BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK343

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

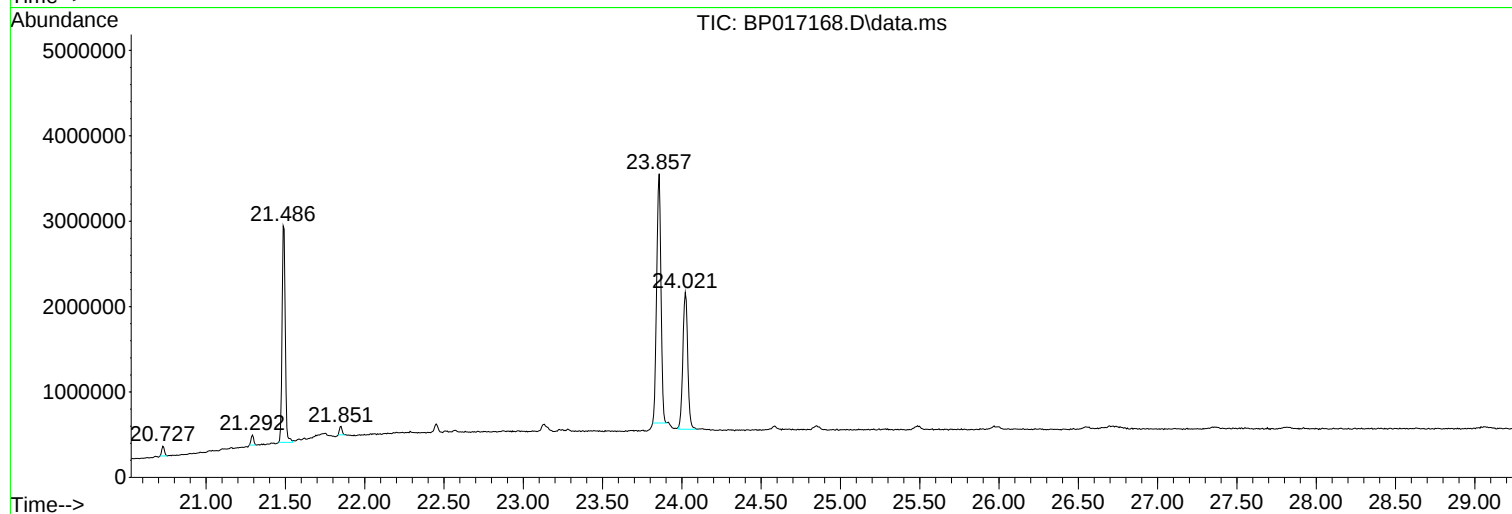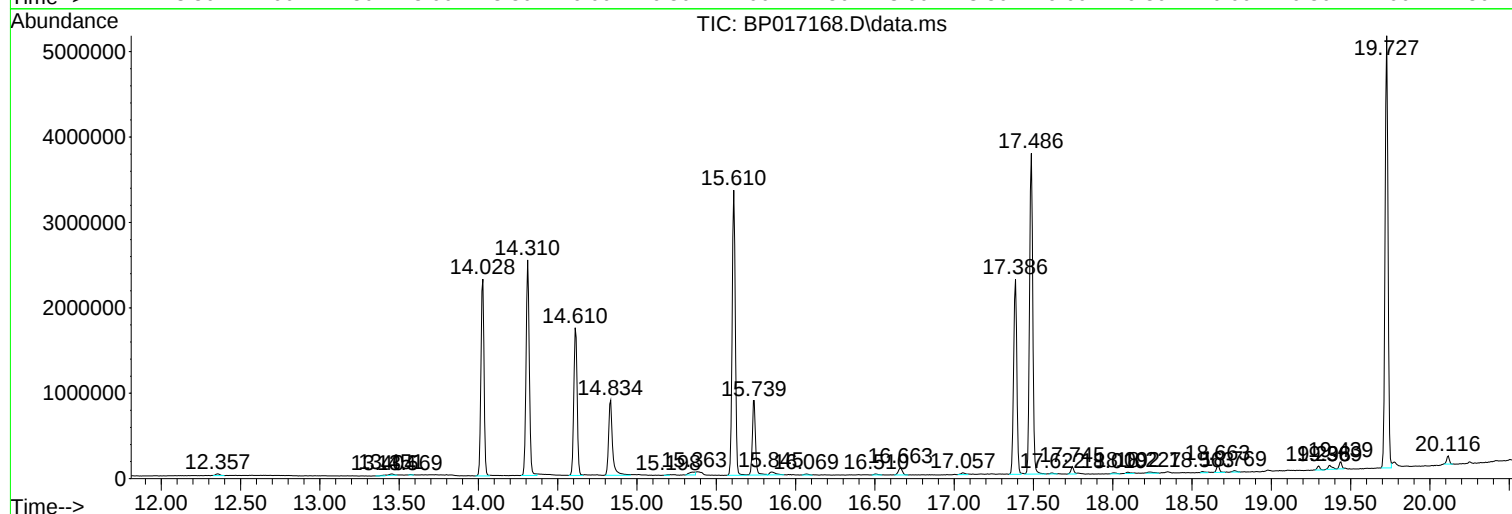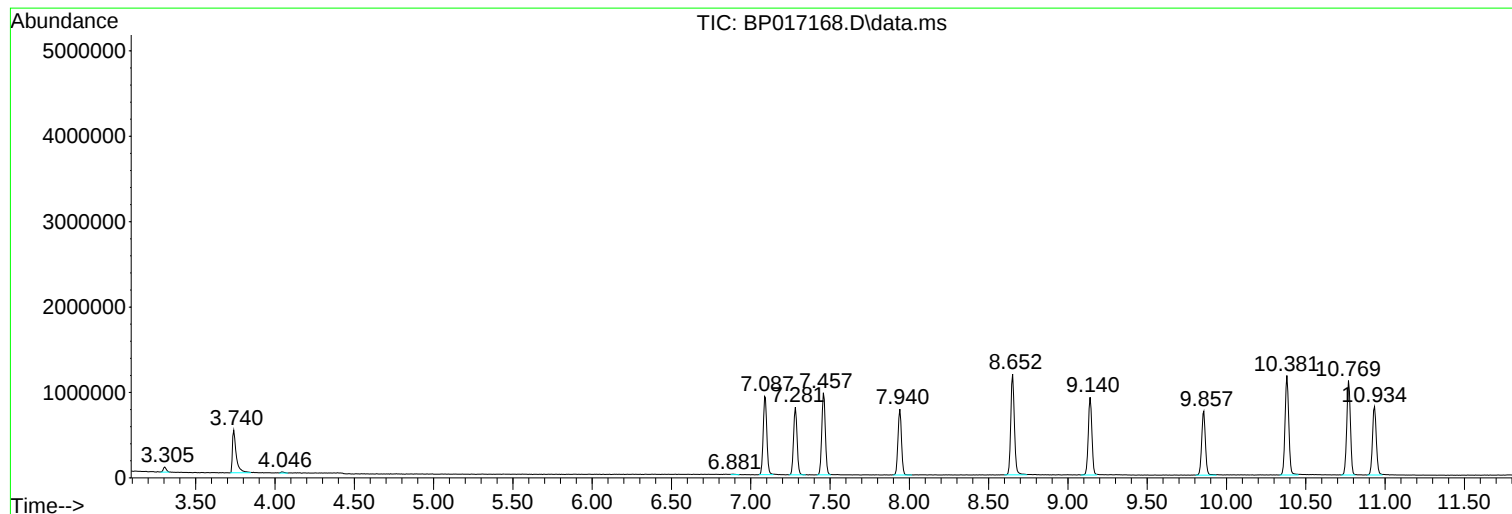

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017168.D
Acq On : 14 Sep 2023 09:59
Operator : MA/JU
Sample : PB155343BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK343

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017168.D
Acq On : 14 Sep 2023 09:59
Operator : MA/JU
Sample : PB155343BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK343

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc