

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017170.D
 Acq On : 14 Sep 2023 11:07
 Operator : MA/JU
 Sample : 04274-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 RT2683

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	25	30	56	rVB	3456050	4901167	100.00%	26.217%
2	3.534	74	76	81	rBV6	4473	5087	0.10%	0.027%
3	3.611	86	89	93	rBV2	10688	15629	0.32%	0.084%
4	3.940	140	145	151	rBV	43303	64168	1.31%	0.343%
5	4.058	161	165	174	rVB	42482	58761	1.20%	0.314%
6	4.199	186	189	196	rVB6	15086	27096	0.55%	0.145%
7	4.581	249	254	263	rVB	67287	92664	1.89%	0.496%
8	4.993	320	324	330	rBV2	8632	14305	0.29%	0.077%
9	5.222	358	363	367	rBV	15404	21425	0.44%	0.115%
10	5.581	416	424	427	rBV6	6531	13129	0.27%	0.070%
11	6.910	643	650	657	rVB6	9225	28405	0.58%	0.152%
12	7.134	685	688	695	rVB8	3314	6545	0.13%	0.035%
13	7.499	748	750	754	rVB5	6362	7612	0.16%	0.041%
14	7.552	754	759	769	rBV2	18959	47279	0.96%	0.253%
15	7.828	801	806	811	rBV3	21529	34832	0.71%	0.186%
16	7.952	820	827	838	rBV	703201	1122211	22.90%	6.003%
17	8.299	881	886	893	rVB3	12541	20052	0.41%	0.107%
18	9.199	1035	1039	1042	rBV5	3073	5149	0.11%	0.028%
19	9.352	1063	1065	1070	rVB6	4320	6038	0.12%	0.032%
20	10.628	1273	1282	1292	rBV	212302	363747	7.42%	1.946%
21	10.775	1299	1307	1316	rBV	908157	1485151	30.30%	7.944%
22	11.151	1364	1371	1379	rBV2	61860	109802	2.24%	0.587%
23	11.469	1421	1425	1429	rBV7	2631	5121	0.10%	0.027%
24	11.828	1478	1486	1487	rBV8	2723	5653	0.12%	0.030%
25	12.357	1570	1576	1583	rBV2	39462	69477	1.42%	0.372%
26	12.881	1660	1665	1668	rBV7	4310	6513	0.13%	0.035%
27	13.457	1757	1763	1769	rBV2	18759	33231	0.68%	0.178%
28	13.798	1817	1821	1825	rBV7	4331	5034	0.10%	0.027%
29	14.610	1950	1959	1970	rBV	1248843	1834668	37.43%	9.814%
30	14.998	2019	2025	2032	rBV	3956	8872	0.18%	0.047%
31	15.410	2090	2095	2096	rBV5	5637	7876	0.16%	0.042%
32	15.863	2168	2172	2180	rVV3	14927	26229	0.54%	0.140%
33	16.269	2239	2241	2244	rVB4	6128	5853	0.12%	0.031%
34	16.469	2270	2275	2276	rBV5	3452	5100	0.10%	0.027%
35	16.592	2292	2296	2302	rVB5	13747	19253	0.39%	0.103%
36	16.728	2318	2319	2324	rBV5	5382	6018	0.12%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017170.D
 Acq On : 14 Sep 2023 11:07
 Operator : MA/JU
 Sample : 04274-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 RT2683

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	17.181	2390	2396	2401	rBV10	6015	12973	0.26%	0.069%
38	17.239	2402	2406	2410	rBV7	15962	22931	0.47%	0.123%
39	17.275	2410	2412	2420	rVB8	6195	8357	0.17%	0.045%
40	17.381	2424	2430	2439	rBV	1611381	2292775	46.78%	12.264%
41	17.963	2525	2529	2533	rBV6	12218	23418	0.48%	0.125%
42	18.222	2569	2573	2584	rBV	138765	221416	4.52%	1.184%
43	18.416	2603	2606	2610	rVB6	16385	20110	0.41%	0.108%
44	19.363	2763	2767	2772	rVB	77649	96637	1.97%	0.517%
45	19.457	2780	2783	2787	rBV5	62745	82465	1.68%	0.441%
46	21.480	3122	3127	3134	rBV	2047130	2658745	54.25%	14.222%
47	24.010	3550	3557	3567	rVB	1378744	2765546	56.43%	14.793%




Sum of corrected areas: 18694525

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017170.D
Acq On : 14 Sep 2023 11:07
Operator : MA/JU
Sample : 04274-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RT2683

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

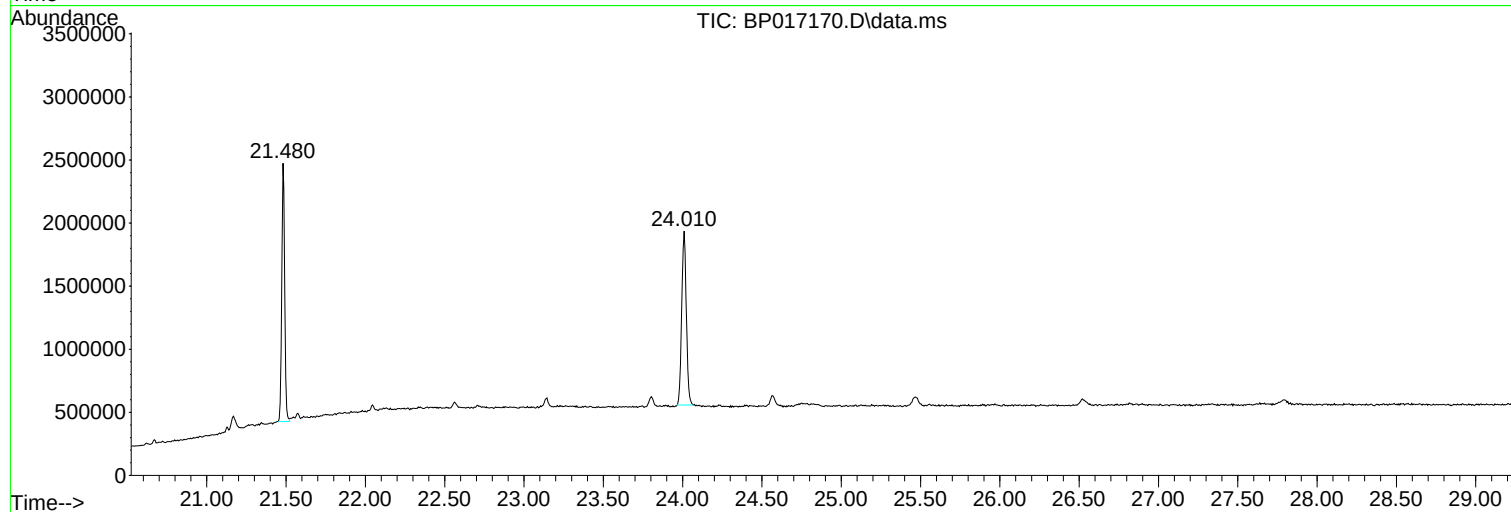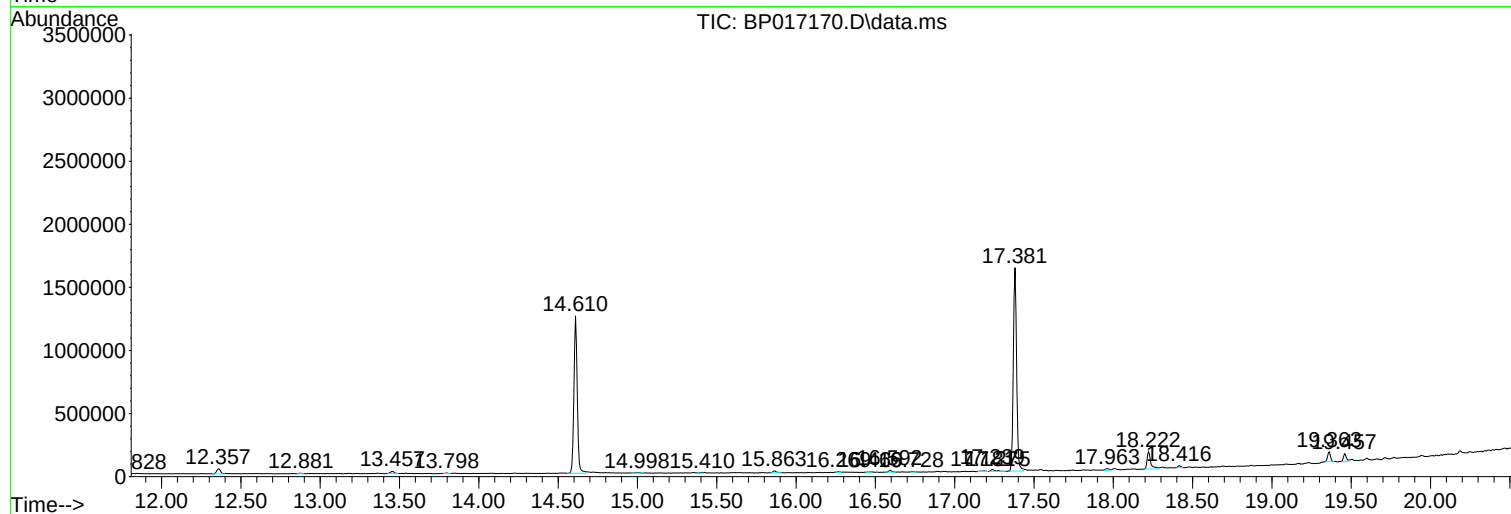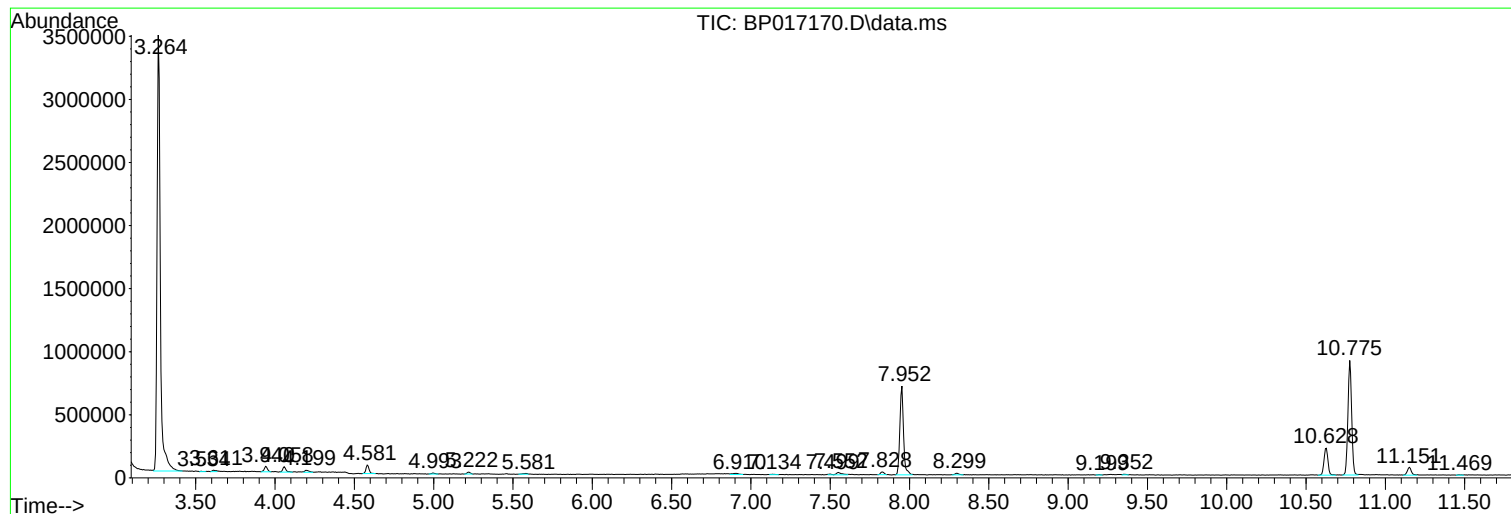

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017170.D
Acq On : 14 Sep 2023 11:07
Operator : MA/JU
Sample : 04274-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RT2683

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017170.D
Acq On : 14 Sep 2023 11:07
Operator : MA/JU
Sample : 04274-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RT2683

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc