

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017171.D
 Acq On : 14 Sep 2023 11:42
 Operator : MA/JU
 Sample : 04324-20
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017171.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	27	30	35	rVV5	14529	18136	0.32%	0.034%
2	3.310	35	38	44	rVB	56700	67018	1.19%	0.125%
3	3.752	109	113	127	rBV	306530	478554	8.53%	0.891%
4	3.940	141	145	153	rVB	50063	73153	1.30%	0.136%
5	4.057	162	165	169	rVB	15999	18494	0.33%	0.034%
6	4.210	188	191	195	rBV5	4469	7047	0.13%	0.013%
7	4.581	248	254	268	rBV	723482	1043610	18.61%	1.942%
8	4.999	321	325	331	rVB5	8252	14505	0.26%	0.027%
9	5.587	421	425	429	rVB3	6876	8655	0.15%	0.016%
10	6.904	647	649	658	rVB10	6679	13524	0.24%	0.025%
11	7.104	677	683	691	rBV	225527	358634	6.39%	0.667%
12	7.293	708	715	726	rBV	928810	1400965	24.98%	2.607%
13	7.469	738	745	757	rBV	852112	1346392	24.00%	2.506%
14	7.951	820	827	838	rBV	759619	1183417	21.10%	2.202%
15	8.657	939	947	960	rBV	629152	1051744	18.75%	1.957%
16	9.151	1021	1031	1044	rBV	1038585	1676708	29.89%	3.120%
17	9.863	1145	1152	1163	rBV	814425	1305108	23.27%	2.429%
18	10.387	1233	1241	1254	rBV	1165545	1939466	34.58%	3.609%
19	10.775	1299	1307	1315	rBV	988891	1648070	29.38%	3.067%
20	10.939	1327	1335	1350	rBV	1138296	1917110	34.18%	3.568%
21	12.357	1571	1576	1583	rBV	20636	36084	0.64%	0.067%
22	13.451	1757	1762	1772	rVB8	6477	14227	0.25%	0.026%
23	13.569	1776	1782	1786	rVV8	5228	6963	0.12%	0.013%
24	13.851	1825	1830	1835	rVB9	4405	6329	0.11%	0.012%
25	14.028	1853	1860	1867	rBV	2204875	3000041	53.49%	5.583%
26	14.310	1900	1908	1923	rBV	2561977	3630577	64.73%	6.756%
27	14.610	1952	1959	1968	rBV	1425390	2050200	36.55%	3.815%
28	14.833	1991	1997	2008	rBV	90261	194507	3.47%	0.362%
29	15.610	2122	2129	2143	rBV	3221889	4595429	81.93%	8.552%
30	15.733	2144	2150	2164	rVV	848976	1188615	21.19%	2.212%
31	15.845	2165	2169	2178	rVB4	16490	31569	0.56%	0.059%
32	16.398	2258	2263	2267	rBV7	4105	6185	0.11%	0.012%
33	17.045	2369	2373	2376	rBV5	4293	6682	0.12%	0.012%
34	17.380	2424	2430	2440	rBV	1687887	2330759	41.55%	4.338%
35	17.480	2441	2447	2467	rVV	3498715	4832055	86.15%	8.992%
36	18.221	2569	2573	2580	rBV3	38727	57620	1.03%	0.107%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017171.D
Acq On : 14 Sep 2023 11:42
Operator : MA/JU
Sample : 04324-20
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJA8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION

37	19.292	2752	2755	2759	rVB2	38668	43452	0.77%	0.081%
38	19.363	2763	2767	2772	rVB	34994	50273	0.90%	0.094%
39	19.457	2781	2783	2788	rVB5	19997	23393	0.42%	0.044%
40	19.721	2822	2828	2835	rBV	4318491	5507494	98.19%	10.249%
41	21.480	3123	3127	3133	rBV	1845859	2333550	41.60%	4.343%
42	23.845	3522	3529	3543	rVB	2749169	5609067	100.00%	10.438%
43	24.009	3551	3557	3570	rVB	1249335	2609663	46.53%	4.857%




Sum of corrected areas: 53735044

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017171.D
Acq On : 14 Sep 2023 11:42
Operator : MA/JU
Sample : 04324-20
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

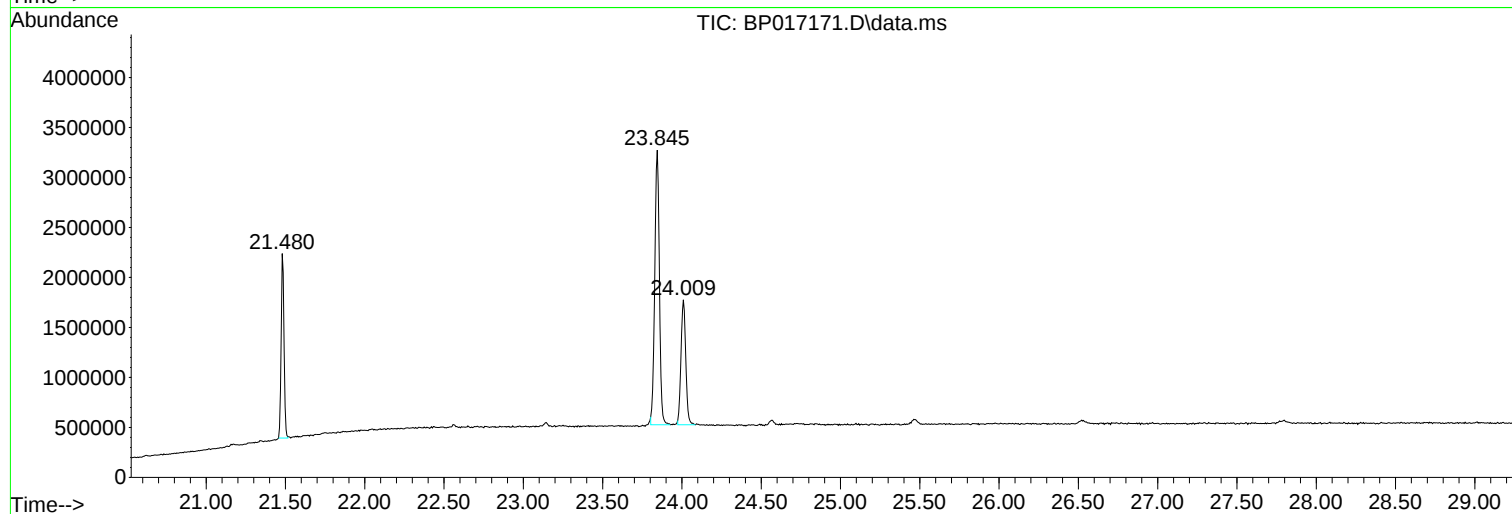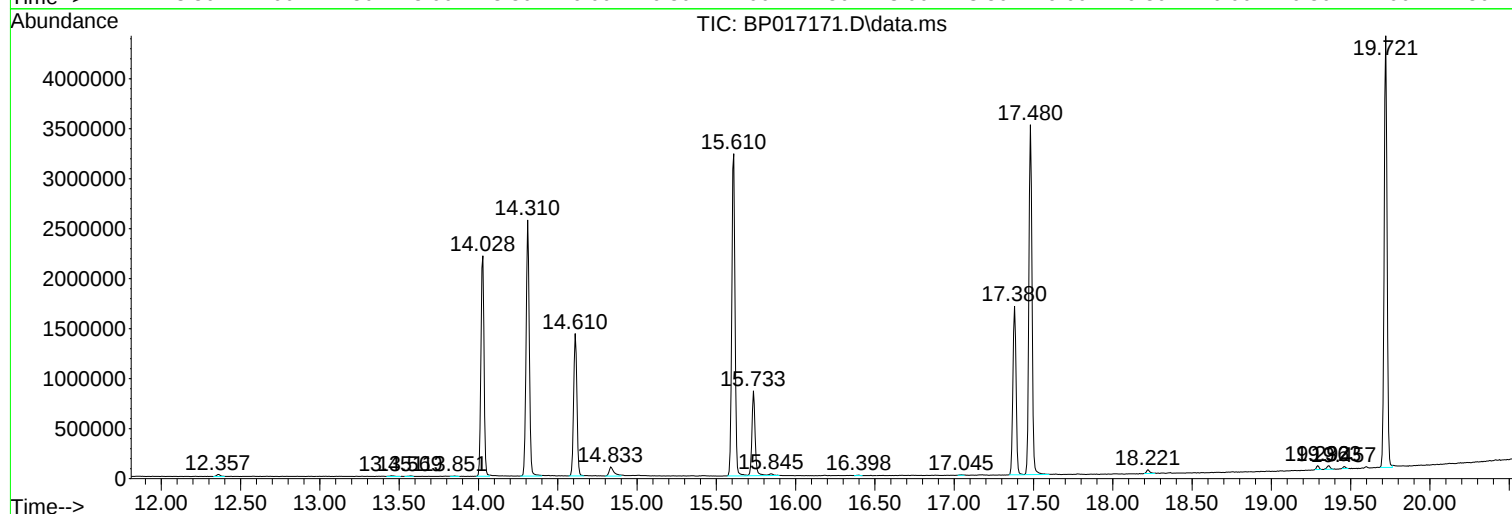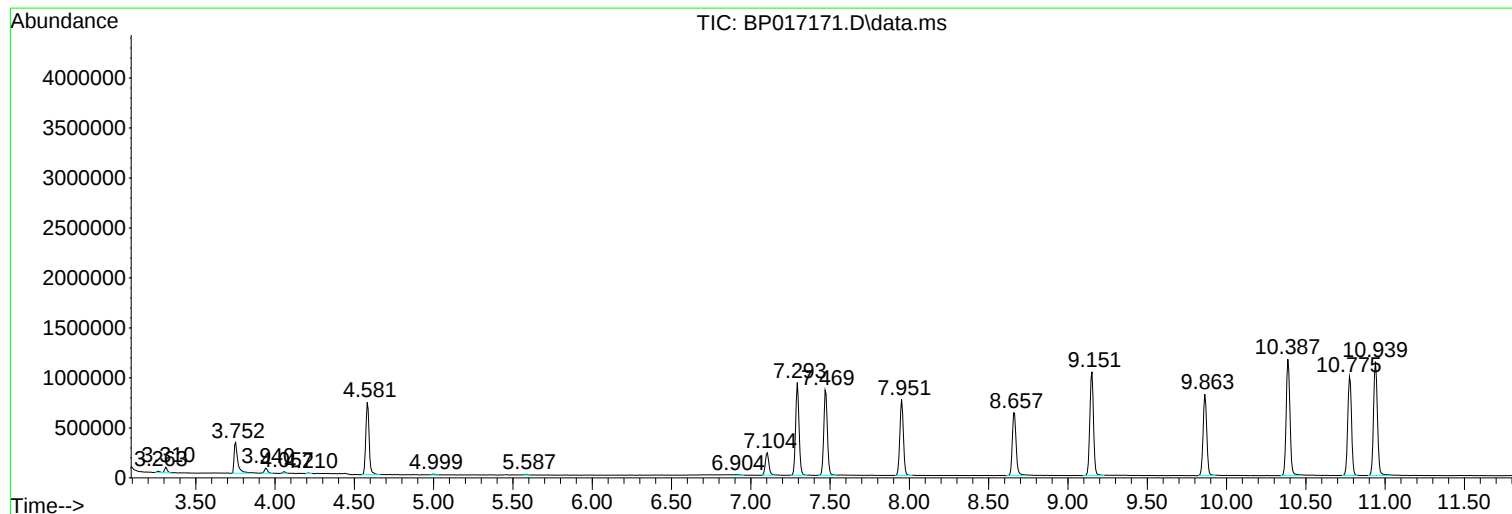

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017171.D
Acq On : 14 Sep 2023 11:42
Operator : MA/JU
Sample : 04324-20
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJA8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.581	17.64 ng/ul	1043610	1,4-Dichlorobenzene-d4	7.951

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	35

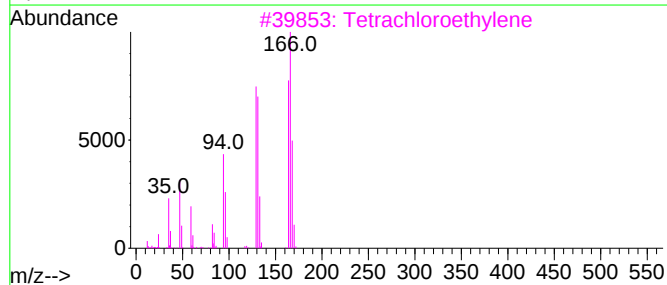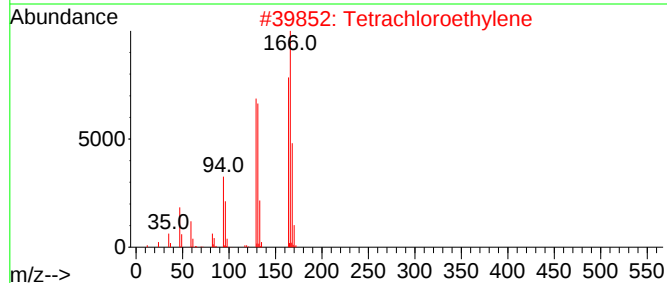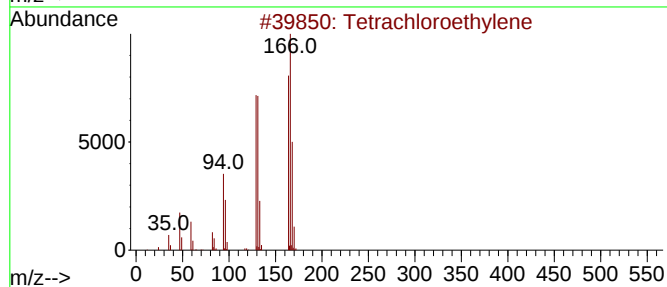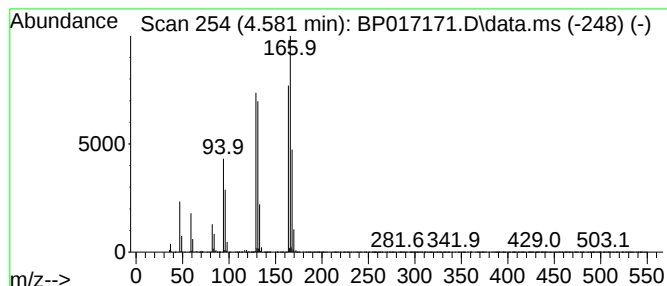

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017171.D
Acq On : 14 Sep 2023 11:42
Operator : MA/JU
Sample : 04324-20
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.581	17.6	ng/ul	1043610	1	7.951	1183420	20.0