

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017175.D
 Acq On : 14 Sep 2023 13:59
 Operator : MA/JU
 Sample : PB155433BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK433

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	34	38	45	rVB	66053	84333	1.81%	0.166%
2	3.746	109	112	135	rBV	554739	833420	17.89%	1.640%
3	4.058	162	165	169	rVB2	14174	16270	0.35%	0.032%
4	7.105	674	683	694	rBV	924610	1493872	32.06%	2.940%
5	7.293	707	715	726	rVB	790155	1202439	25.81%	2.367%
6	7.469	738	745	759	rBV	971984	1510667	32.42%	2.973%
7	7.952	820	827	835	rVB	788945	1200603	25.77%	2.363%
8	8.664	940	948	965	rBV	1091967	1833084	39.34%	3.608%
9	9.152	1022	1031	1041	rBV	874596	1423927	30.56%	2.803%
10	9.863	1144	1152	1166	rBV	744765	1189815	25.54%	2.342%
11	10.387	1232	1241	1259	rBV	1090666	1835530	39.39%	3.613%
12	10.775	1299	1307	1316	rBV	1036109	1729668	37.12%	3.404%
13	10.940	1326	1335	1352	rBV	757239	1281305	27.50%	2.522%
14	12.363	1570	1577	1581	rBV	17564	30467	0.65%	0.060%
15	13.457	1756	1763	1769	rBV4	15868	27789	0.60%	0.055%
16	13.569	1777	1782	1783	rBV5	3166	4682	0.10%	0.009%
17	14.028	1852	1860	1870	rBV	1901419	2674173	57.39%	5.264%
18	14.310	1901	1908	1921	rBV	2227254	3156070	67.73%	6.212%
19	14.610	1952	1959	1968	rBV	1544256	2223614	47.72%	4.377%
20	14.828	1990	1996	2016	rBV	637231	1138981	24.44%	2.242%
21	15.281	2070	2073	2076	rBV5	4104	5029	0.11%	0.010%
22	15.416	2094	2096	2102	rVB7	3722	5196	0.11%	0.010%
23	15.604	2120	2128	2142	rBV	2724377	4001894	85.89%	7.877%
24	15.734	2144	2150	2163	rVV	739585	1001209	21.49%	1.971%
25	15.845	2166	2169	2179	rVB6	16238	27731	0.60%	0.055%
26	16.187	2221	2227	2229	rBV7	3029	4667	0.10%	0.009%
27	16.551	2286	2289	2296	rVB9	2610	5212	0.11%	0.010%
28	17.045	2369	2373	2379	rVB8	4423	6410	0.14%	0.013%
29	17.169	2389	2394	2397	rBV6	5659	9058	0.19%	0.018%
30	17.381	2423	2430	2441	rBV	1898288	2575748	55.28%	5.070%
31	17.481	2441	2447	2466	rVB	3046342	4287047	92.01%	8.438%
32	19.292	2752	2755	2760	rBV3	30480	38285	0.82%	0.075%
33	19.363	2764	2767	2774	rVB2	32805	45349	0.97%	0.089%
34	19.722	2822	2828	2835	rBV	3675102	4659481	100.00%	9.171%
35	21.486	3123	3128	3136	rBV	1784348	2353841	50.52%	4.633%
36	23.845	3522	3529	3542	rVB	2171933	4428412	95.04%	8.716%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017175.D
Acq On : 14 Sep 2023 13:59
Operator : MA/JU
Sample : PB155433BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK433

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION

37	24.010	3551	3557	3569	rVB	1214500	2460461	52.81%	4.843%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 50805739

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017175.D
Acq On : 14 Sep 2023 13:59
Operator : MA/JU
Sample : PB155433BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK433

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

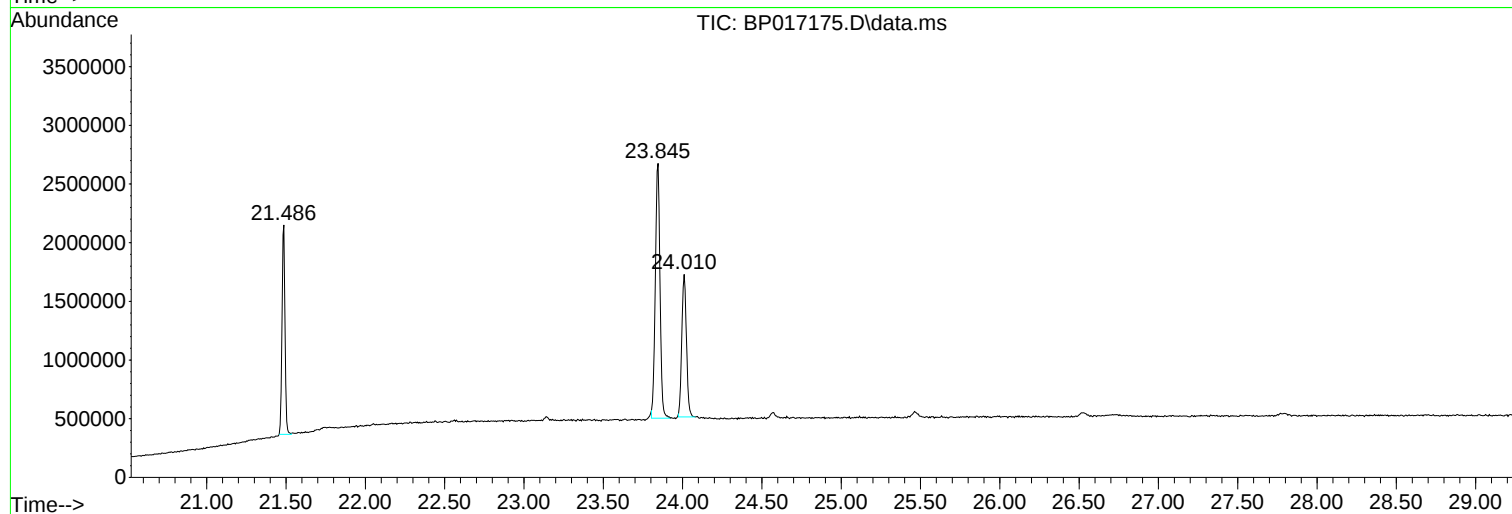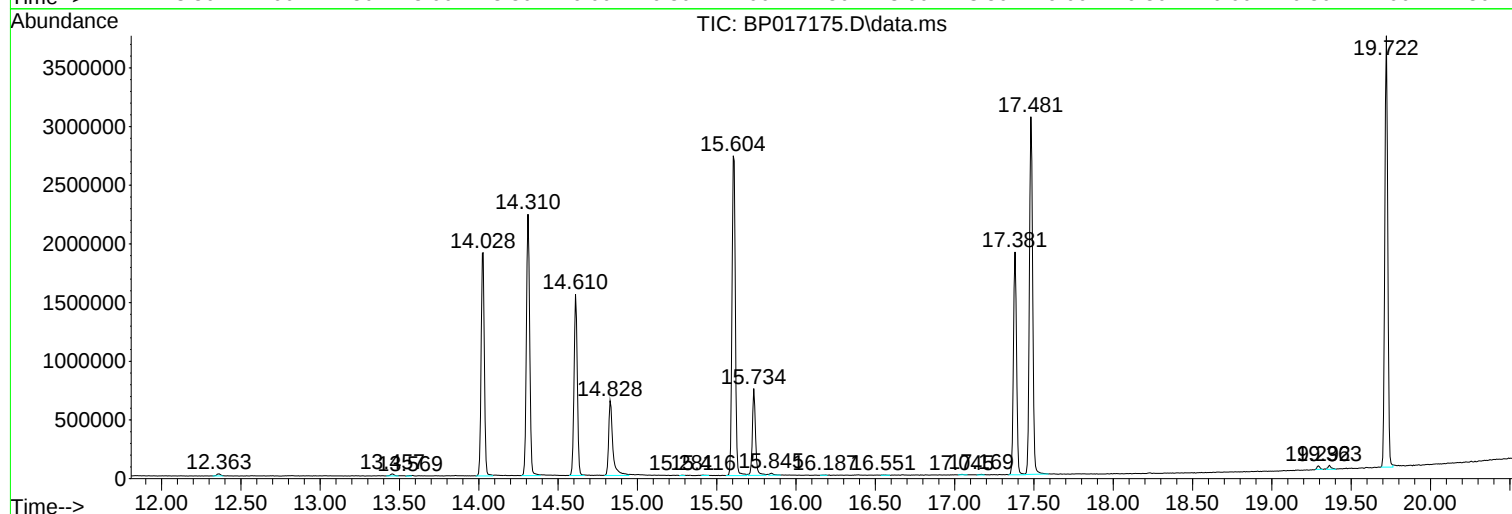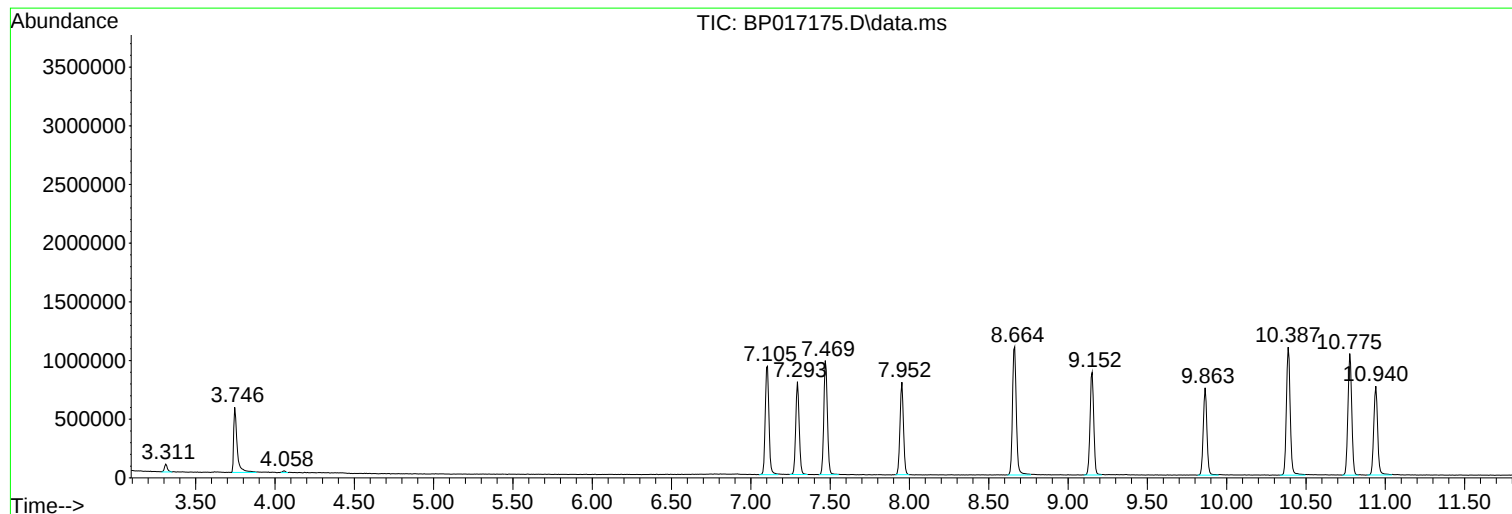

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017175.D
Acq On : 14 Sep 2023 13:59
Operator : MA/JU
Sample : PB155433BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK433

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017175.D
Acq On : 14 Sep 2023 13:59
Operator : MA/JU
Sample : PB155433BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK433

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------