

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017177.D
 Acq On : 14 Sep 2023 15:13
 Operator : MA/JU
 Sample : 04227-19
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	25	30	34	rBV	148130	189770	3.97%	0.436%
2	3.311	34	38	46	rVB	47762	68631	1.44%	0.158%
3	3.752	109	113	124	rBV	142538	227476	4.76%	0.523%
4	3.940	139	145	152	rBV	28181	43762	0.92%	0.101%
5	4.052	162	164	168	rVB2	13444	15333	0.32%	0.035%
6	4.581	248	254	268	rVB	483409	717855	15.02%	1.650%
7	4.993	319	324	327	rBV3	8607	14262	0.30%	0.033%
8	5.028	327	330	337	rVB	10671	18312	0.38%	0.042%
9	6.911	649	650	654	rVB4	5586	5705	0.12%	0.013%
10	7.099	676	682	689	rBV	187399	290223	6.07%	0.667%
11	7.287	706	714	724	rBV	680704	1063622	22.25%	2.445%
12	7.469	738	745	754	rBV	676045	1053881	22.04%	2.422%
13	7.946	820	826	836	rVB	653451	1028617	21.52%	2.364%
14	8.658	941	947	958	rBV	498486	812621	17.00%	1.868%
15	8.734	958	960	969	rVB9	5737	11635	0.24%	0.027%
16	9.146	1023	1030	1038	rBV	767772	1228195	25.69%	2.823%
17	9.357	1061	1066	1071	rVB2	19009	30762	0.64%	0.071%
18	9.863	1144	1152	1161	rBV	584141	966722	20.22%	2.222%
19	10.387	1233	1241	1254	rBV	843883	1424713	29.80%	3.274%
20	10.775	1299	1307	1316	rBV	859343	1423394	29.77%	3.271%
21	10.940	1324	1335	1347	rBV	649309	1141489	23.88%	2.623%
22	11.851	1485	1490	1496	rVB	22459	35940	0.75%	0.083%
23	12.357	1572	1576	1584	rVB2	16247	26759	0.56%	0.061%
24	13.457	1757	1763	1769	rBV3	13174	22387	0.47%	0.051%
25	13.575	1778	1783	1786	rBV7	3678	5128	0.11%	0.012%
26	13.851	1826	1830	1835	rVB3	11966	15467	0.32%	0.036%
27	14.028	1853	1860	1873	rBV	1535430	2199434	46.01%	5.055%
28	14.310	1902	1908	1919	rBV	1869877	2658406	55.61%	6.110%
29	14.404	1922	1924	1928	rVV5	6185	8609	0.18%	0.020%
30	14.463	1932	1934	1940	rVB7	4767	7859	0.16%	0.018%
31	14.610	1953	1959	1968	rBV	1275695	1779557	37.22%	4.090%
32	14.751	1980	1983	1987	rVB6	3518	5692	0.12%	0.013%
33	14.840	1991	1998	2014	rBV	82615	195411	4.09%	0.449%
34	14.987	2020	2023	2025	rBV3	6374	7249	0.15%	0.017%
35	15.416	2090	2096	2101	rVB9	5952	10771	0.23%	0.025%
36	15.610	2121	2129	2143	rBV	2418585	3442616	72.01%	7.912%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017177.D
 Acq On : 14 Sep 2023 15:13
 Operator : MA/JU
 Sample : 04227-19
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	15.734	2144	2150	2163	rVV	658561	943041	19.73%	2.167%
38	15.845	2166	2169	2175	rVB5	11770	20676	0.43%	0.048%
39	16.187	2223	2227	2230	rBV6	3184	4808	0.10%	0.011%
40	16.245	2234	2237	2242	rBV7	2543	5210	0.11%	0.012%
41	17.010	2362	2367	2370	rBV7	7409	15182	0.32%	0.035%
42	17.169	2390	2394	2400	rVB9	4605	8784	0.18%	0.020%
43	17.381	2424	2430	2440	rBV	1526967	2165851	45.30%	4.978%
44	17.481	2441	2447	2464	rVV	2655729	3781439	79.10%	8.691%
45	18.010	2535	2537	2540	rBV4	4069	4914	0.10%	0.011%
46	18.228	2570	2574	2578	rBV7	15018	23012	0.48%	0.053%
47	19.292	2752	2755	2760	rVB2	30477	40107	0.84%	0.092%
48	19.363	2764	2767	2771	rVB	29052	43747	0.92%	0.101%
49	19.722	2822	2828	2835	rBV	3419325	4516078	94.46%	10.379%
50	21.486	3123	3128	3134	rBV	1865197	2382017	49.83%	5.475%
51	23.851	3523	3530	3543	rVB	2296921	4780733	100.00%	10.988%
52	24.016	3551	3558	3570	rVB	1230941	2576771	53.90%	5.922%




Sum of corrected areas: 43510635

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017177.D
Acq On : 14 Sep 2023 15:13
Operator : MA/JU
Sample : 04227-19
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

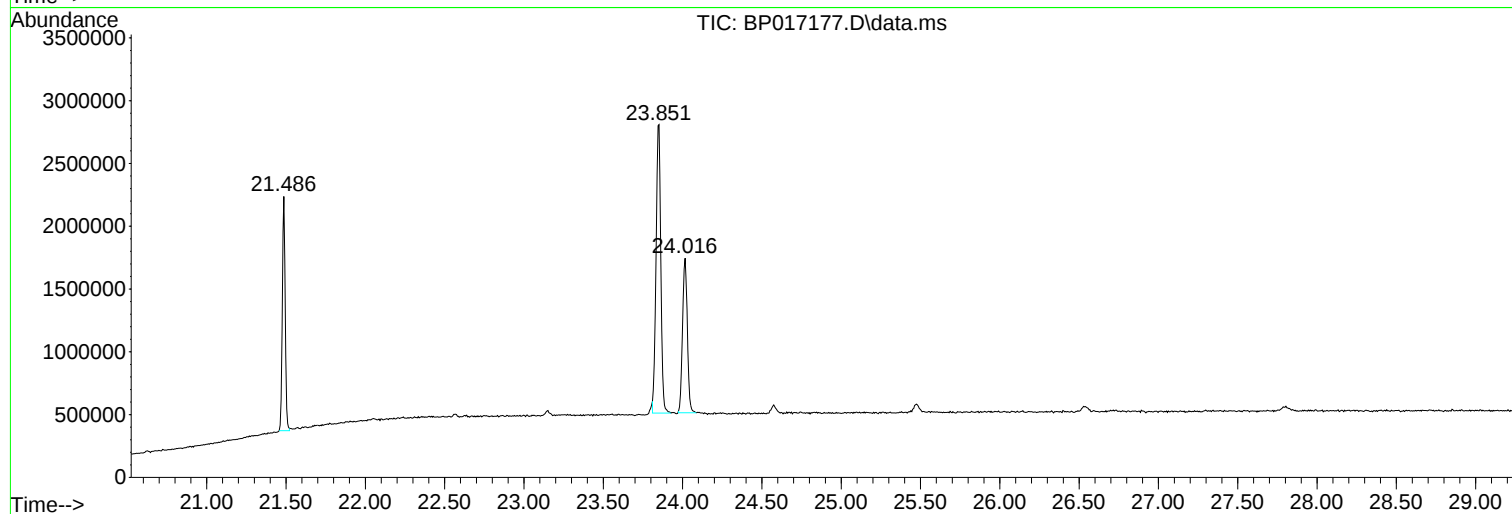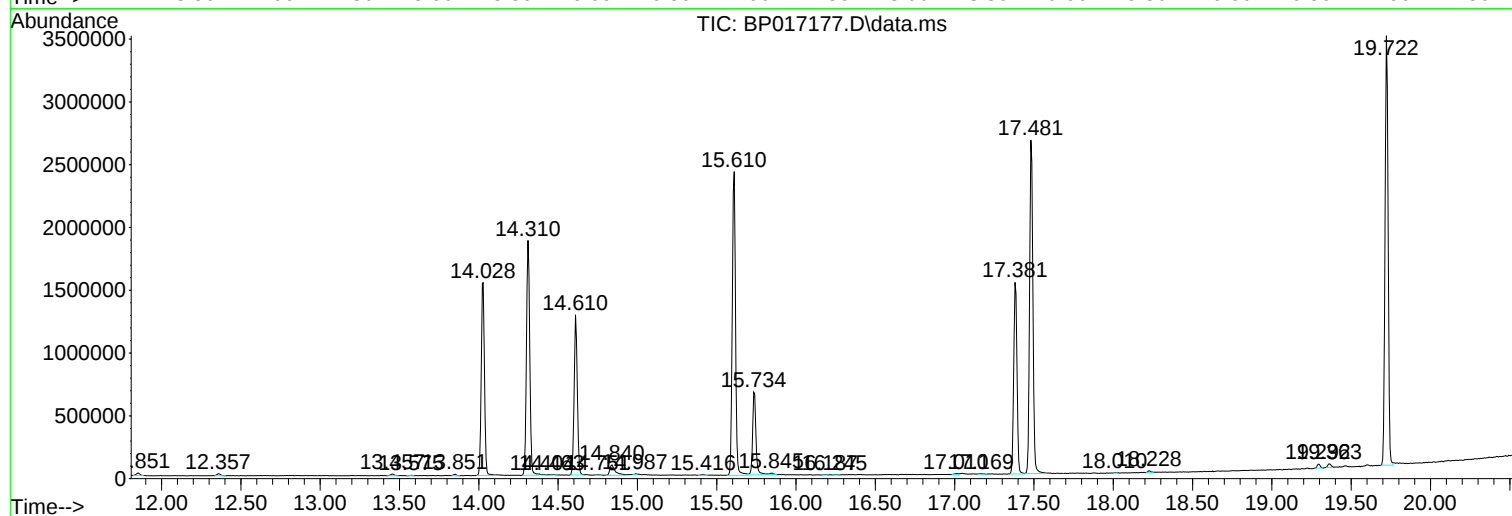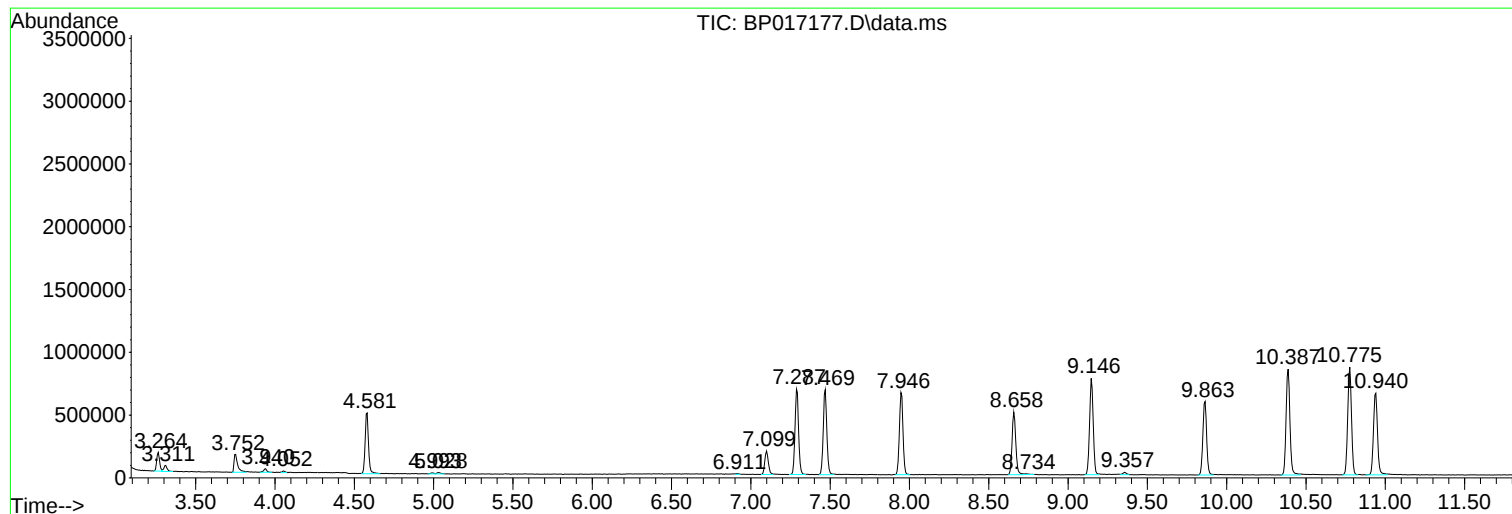

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017177.D
Acq On : 14 Sep 2023 15:13
Operator : MA/JU
Sample : 04227-19
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ99










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.581	13.96 ng/ul	717855	1,4-Dichlorobenzene-d4	7.946

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

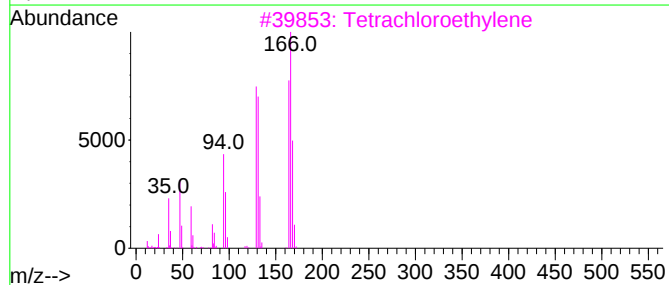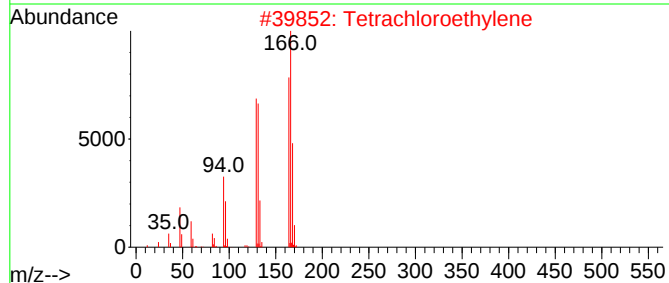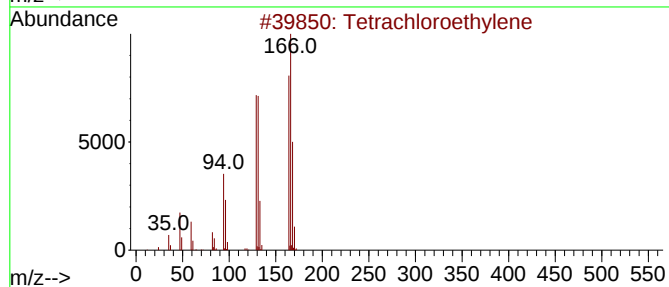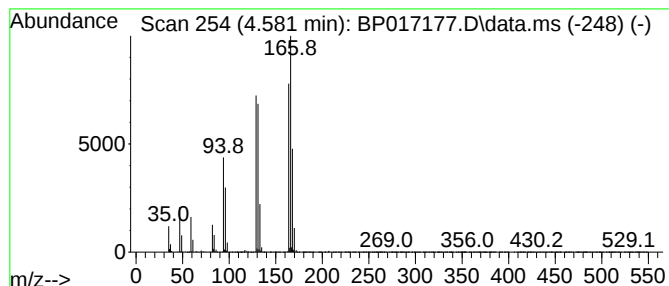

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017177.D
Acq On : 14 Sep 2023 15:13
Operator : MA/JU
Sample : 04227-19
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.581	14.0	ng/u1	717855	1	7.946	1028620	20.0