

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017180.D
 Acq On : 14 Sep 2023 16:56
 Operator : MA/JU
 Sample : 04324-07
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	34	rBV	43280	55249	1.06%	0.107%
2	3.311	34	38	42	rVV	46137	52613	1.01%	0.102%
3	3.752	110	113	123	rBV	177998	264222	5.08%	0.513%
4	3.940	141	145	151	rVB	39428	62124	1.19%	0.121%
5	4.058	162	165	171	rVB2	13763	17397	0.33%	0.034%
6	4.581	248	254	271	rVB	3392432	4805680	92.39%	9.329%
7	4.993	321	324	330	rVB3	6973	11158	0.21%	0.022%
8	5.452	397	402	407	rVB7	4398	6894	0.13%	0.013%
9	5.575	420	423	429	rBV5	6603	11084	0.21%	0.022%
10	6.222	529	533	536	rBV6	3144	5491	0.11%	0.011%
11	7.099	675	682	692	rBV	207742	328824	6.32%	0.638%
12	7.293	704	715	726	rBV	777671	1190372	22.88%	2.311%
13	7.469	737	745	756	rBV	767900	1181657	22.72%	2.294%
14	7.952	819	827	839	rVB	767327	1199089	23.05%	2.328%
15	8.658	940	947	962	rBV	565039	920669	17.70%	1.787%
16	9.146	1023	1030	1038	rBV	852108	1374233	26.42%	2.668%
17	9.863	1144	1152	1163	rBV	680287	1097839	21.11%	2.131%
18	10.387	1233	1241	1259	rBV	982384	1637084	31.47%	3.178%
19	10.775	1300	1307	1316	rBV	1008097	1657865	31.87%	3.218%
20	10.940	1326	1335	1352	rBV	457778	807992	15.53%	1.568%
21	11.769	1470	1476	1493	rBV	126086	274696	5.28%	0.533%
22	12.357	1570	1576	1581	rBV2	16329	27852	0.54%	0.054%
23	13.451	1756	1762	1768	rBV5	15525	29141	0.56%	0.057%
24	14.022	1853	1859	1871	rBV	1843463	2439985	46.91%	4.736%
25	14.310	1900	1908	1925	rBV	2078135	2921405	56.16%	5.671%
26	14.528	1939	1945	1951	rVB6	9110	14037	0.27%	0.027%
27	14.610	1951	1959	1967	rBV	1461572	2059255	39.59%	3.997%
28	14.834	1992	1997	2014	rBV	85959	196340	3.77%	0.381%
29	15.110	2040	2044	2049	rVB8	3385	7065	0.14%	0.014%
30	15.604	2121	2128	2144	rBV	2662742	3731110	71.73%	7.243%
31	15.734	2144	2150	2163	rVV	766252	1026810	19.74%	1.993%
32	15.845	2165	2169	2173	rVB4	12481	18252	0.35%	0.035%
33	16.881	2341	2345	2351	rBV2	22220	27253	0.52%	0.053%
34	17.016	2361	2368	2372	rBV10	9112	26177	0.50%	0.051%
35	17.186	2395	2397	2402	rVB4	10569	13151	0.25%	0.026%
36	17.381	2423	2430	2440	rBV	1711005	2395603	46.05%	4.650%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017180.D
 Acq On : 14 Sep 2023 16:56
 Operator : MA/JU
 Sample : 04324-07
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHF8

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	17.481	2441	2447	2465	rVB	2934660	4073685	78.32%	7.908%
38	18.222	2569	2573	2579	rBV4	36006	57452	1.10%	0.112%
39	19.292	2751	2755	2759	rBV3	41666	55393	1.06%	0.108%
40	19.357	2763	2766	2770	rVB	36963	51399	0.99%	0.100%
41	19.457	2780	2783	2788	rBV4	35846	47876	0.92%	0.093%
42	19.722	2822	2828	2835	rBV	3809831	4891278	94.03%	9.495%
43	21.480	3122	3127	3135	rBV	1957674	2531001	48.66%	4.913%
44	23.839	3521	3528	3545	rVB2	2574267	5201630	100.00%	10.097%
45	24.004	3550	3556	3566	rVB	1326169	2709722	52.09%	5.260%




Sum of corrected areas: 51515104

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017180.D
Acq On : 14 Sep 2023 16:56
Operator : MA/JU
Sample : 04324-07
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

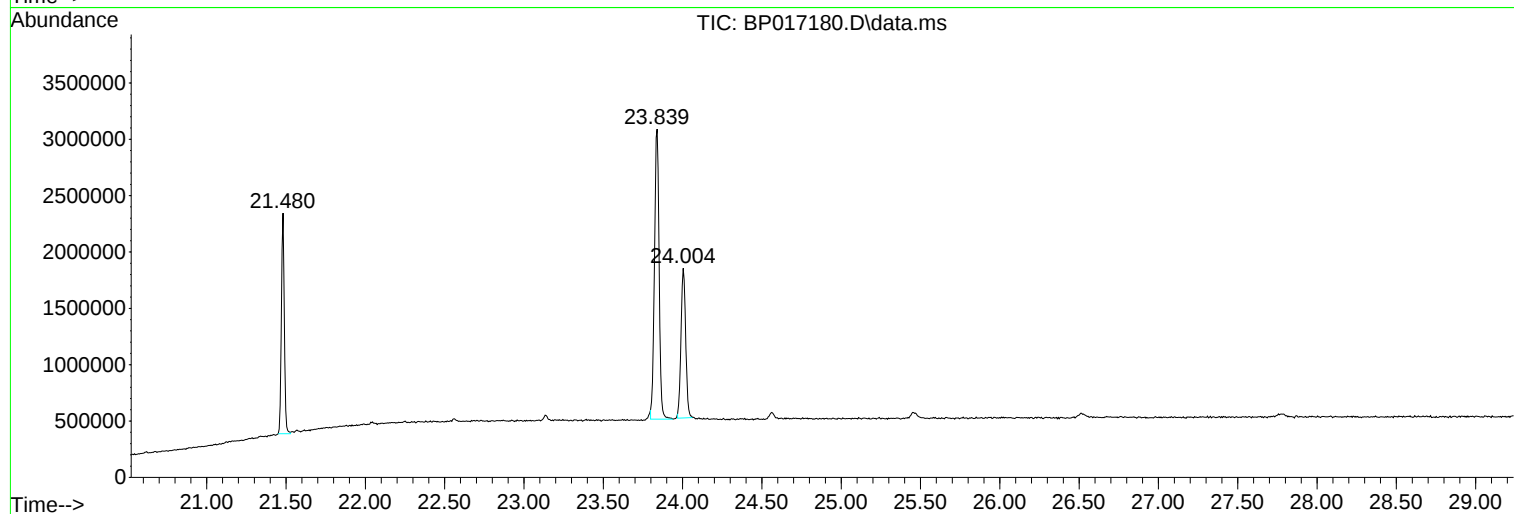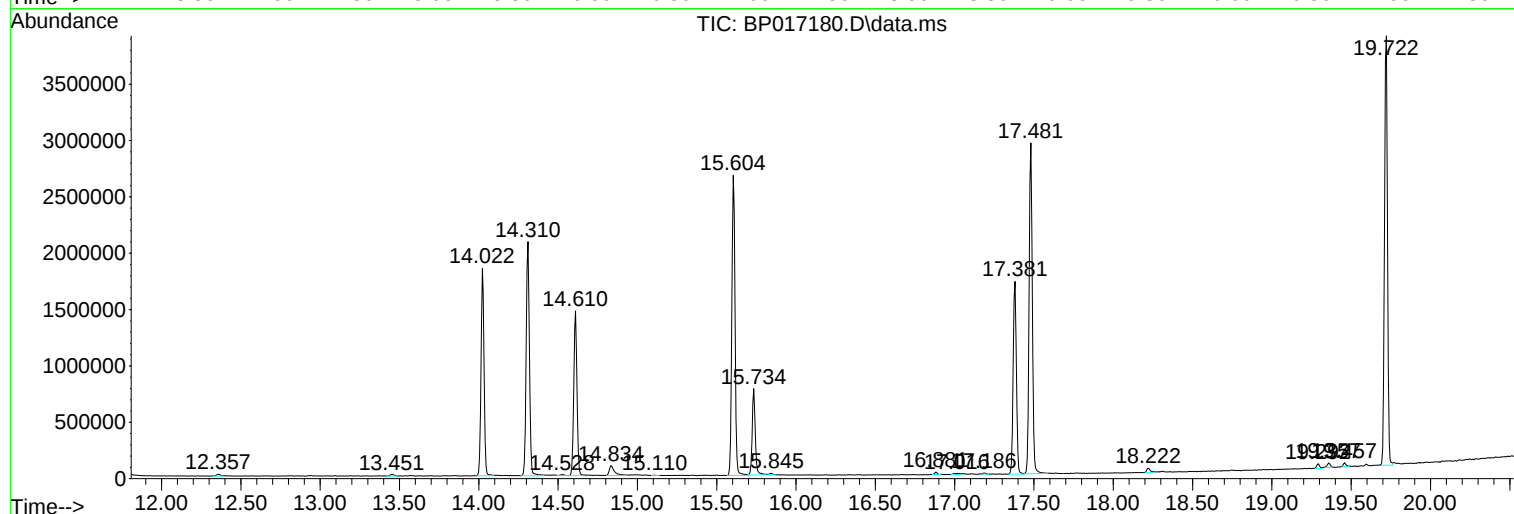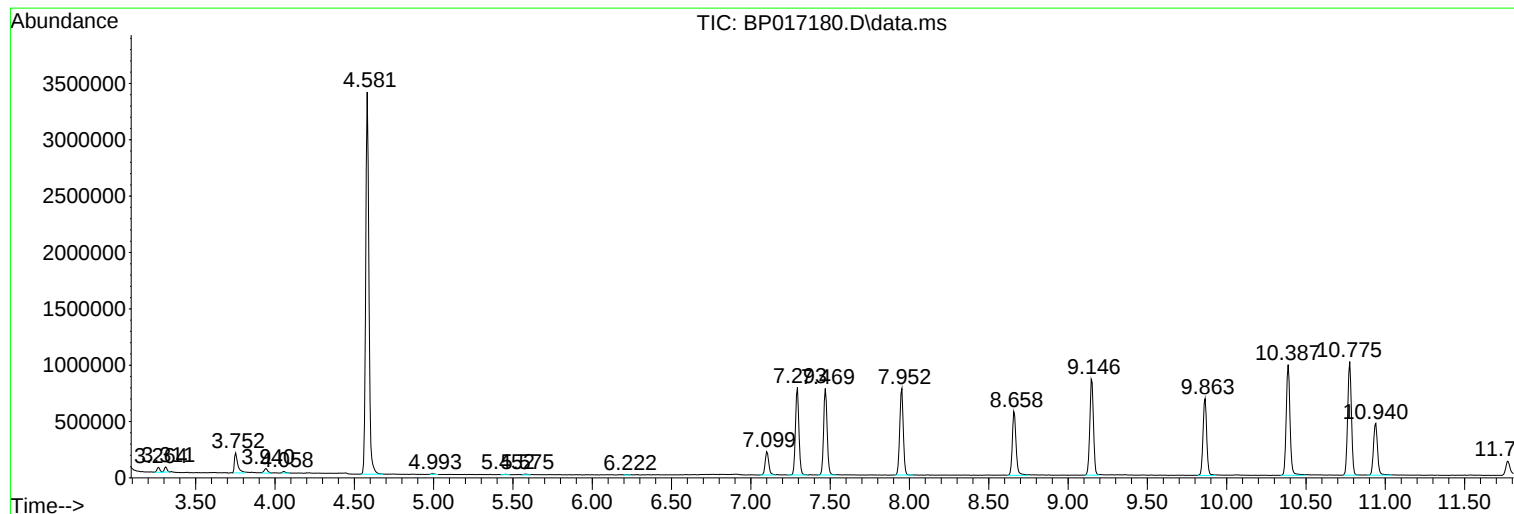

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017180.D
Acq On : 14 Sep 2023 16:56
Operator : MA/JU
Sample : 04324-07
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHF8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.581	80.16 ng/ul	4805680	1,4-Dichlorobenzene-d4	7.952

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	72
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

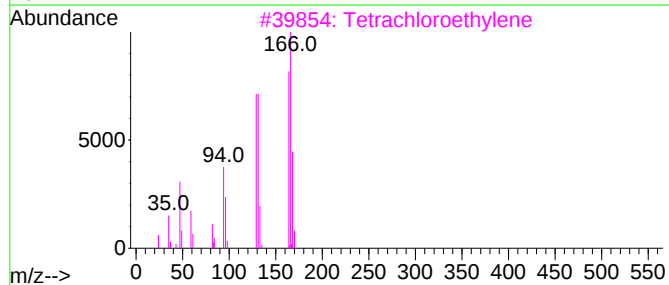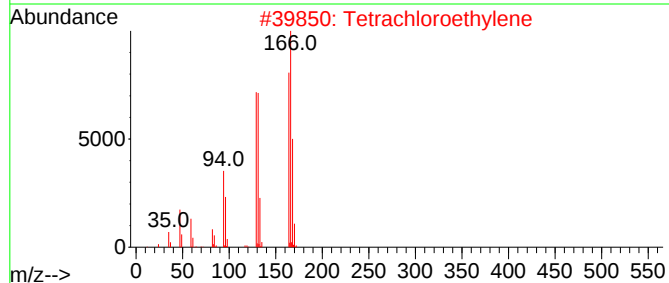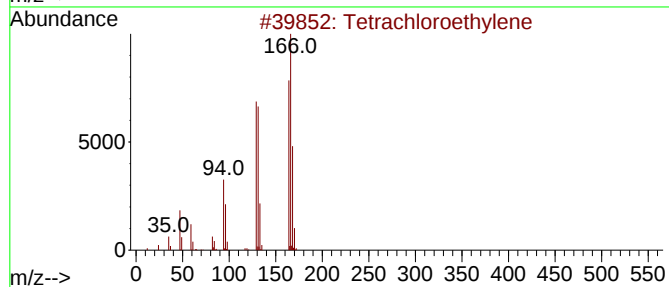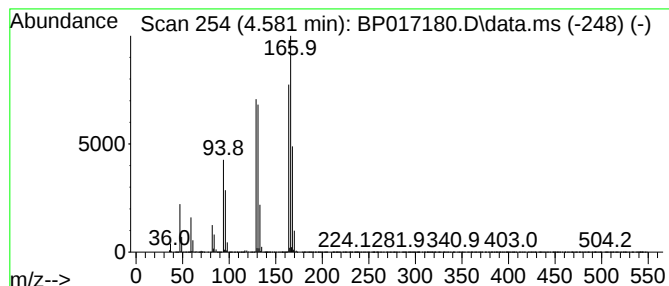

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017180.D
Acq On : 14 Sep 2023 16:56
Operator : MA/JU
Sample : 04324-07
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.581	80.2	ng/u1	4805680	1	7.952	1199090	20.0