

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017181.D
 Acq On : 14 Sep 2023 17:31
 Operator : MA/JU
 Sample : 04324-08
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017181.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	35	rBV	43209	53773	1.11%	0.119%
2	3.311	35	38	42	rVB	38642	43551	0.90%	0.097%
3	3.752	110	113	124	rBV	173560	257831	5.34%	0.572%
4	3.940	141	145	151	rVB	32698	50188	1.04%	0.111%
5	4.058	162	165	169	rVB	11413	12043	0.25%	0.027%
6	4.581	248	254	270	rVB	3208125	4542377	94.13%	10.072%
7	4.993	321	324	327	rBV2	5242	6500	0.13%	0.014%
8	5.581	420	424	428	rBV5	5269	7743	0.16%	0.017%
9	7.099	676	682	692	rBV	156284	253253	5.25%	0.562%
10	7.293	706	715	725	rBV	637175	986645	20.45%	2.188%
11	7.469	738	745	757	rBV	612624	946722	19.62%	2.099%
12	7.952	820	827	838	rVB	631108	987298	20.46%	2.189%
13	8.657	941	947	958	rBV	441462	717316	14.86%	1.591%
14	9.146	1023	1030	1042	rBV	693073	1135323	23.53%	2.517%
15	9.863	1144	1152	1161	rBV	556727	891567	18.48%	1.977%
16	10.387	1232	1241	1256	rBV	801799	1332780	27.62%	2.955%
17	10.775	1299	1307	1320	rBV	839881	1370600	28.40%	3.039%
18	10.940	1328	1335	1350	rBV	416369	727828	15.08%	1.614%
19	11.775	1470	1477	1488	rBV2	75283	170807	3.54%	0.379%
20	12.357	1570	1576	1583	rBV3	13116	23743	0.49%	0.053%
21	13.457	1756	1763	1769	rBV3	16914	30271	0.63%	0.067%
22	14.022	1850	1859	1871	rBV	1573392	2155150	44.66%	4.779%
23	14.310	1900	1908	1925	rBV	1645000	2421031	50.17%	5.368%
24	14.469	1933	1935	1939	rVB5	4303	4986	0.10%	0.011%
25	14.522	1940	1944	1951	rVB6	8222	13784	0.29%	0.031%
26	14.610	1951	1959	1978	rBV	1145177	1686530	34.95%	3.740%
27	14.834	1992	1997	2008	rBV	71717	156790	3.25%	0.348%
28	15.051	2031	2034	2036	rVB4	3907	4863	0.10%	0.011%
29	15.351	2080	2085	2090	rBV7	4453	10671	0.22%	0.024%
30	15.504	2108	2111	2114	rVB5	4578	5652	0.12%	0.013%
31	15.604	2119	2128	2144	rBV	2339348	3236037	67.06%	7.176%
32	15.734	2144	2150	2158	rBV	694292	928241	19.24%	2.058%
33	15.845	2165	2169	2174	rVB4	9729	13640	0.28%	0.030%
34	16.386	2258	2261	2266	rVB7	3783	7531	0.16%	0.017%
35	16.881	2341	2345	2352	rVB3	20924	29775	0.62%	0.066%
36	17.016	2366	2368	2371	rBV4	5070	6275	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017181.D
 Acq On : 14 Sep 2023 17:31
 Operator : MA/JU
 Sample : 04324-08
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	17.186	2394	2397	2403	rVB7	7111	12713	0.26%	0.028%
38	17.380	2423	2430	2439	rBV	1337717	1969296	40.81%	4.367%
39	17.480	2440	2447	2456	rBV	2638919	3802625	78.80%	8.432%
40	17.633	2471	2473	2476	rBV3	4898	5464	0.11%	0.012%
41	18.216	2569	2572	2581	rBV5	33207	49704	1.03%	0.110%
42	19.292	2751	2755	2759	rVB	33879	44967	0.93%	0.100%
43	19.357	2763	2766	2770	rVB	31658	43051	0.89%	0.095%
44	19.451	2780	2782	2789	rBV6	27286	35764	0.74%	0.079%
45	19.716	2822	2827	2840	rBV	3724106	4705315	97.51%	10.434%
46	21.480	3122	3127	3134	rBV	1606799	2092585	43.36%	4.640%
47	23.839	3521	3528	3537	rVB	2430651	4825634	100.00%	10.700%
48	24.004	3550	3556	3566	rVB	1118011	2281512	47.28%	5.059%




Sum of corrected areas: 45097745

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017181.D
Acq On : 14 Sep 2023 17:31
Operator : MA/JU
Sample : 04324-08
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

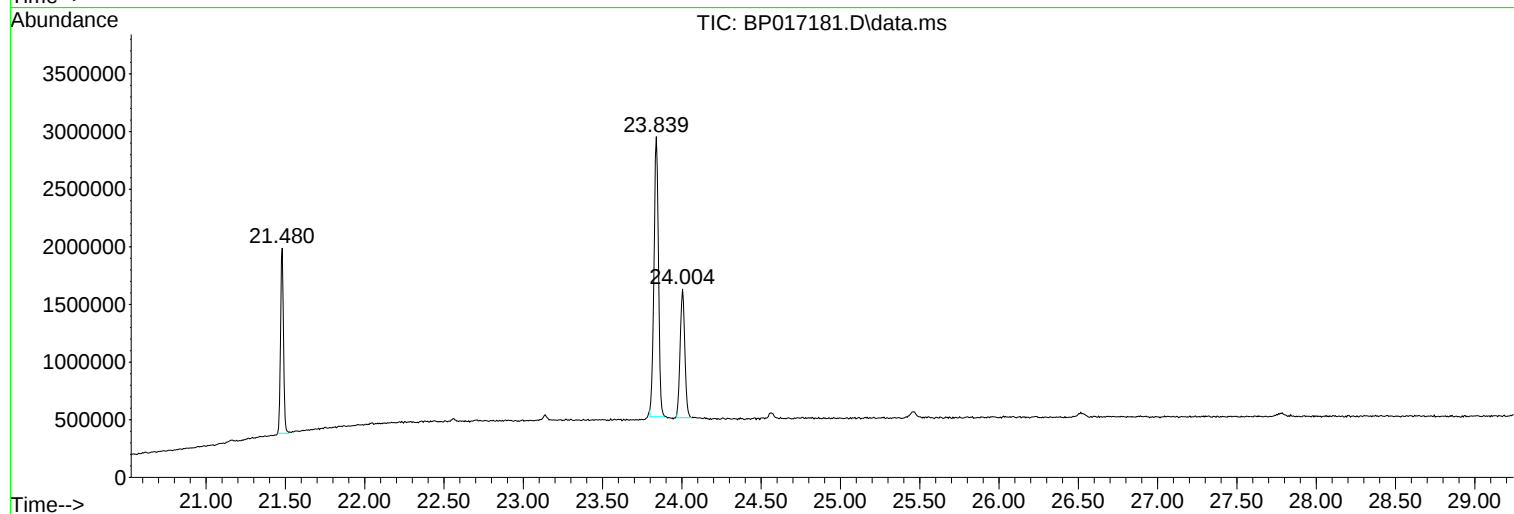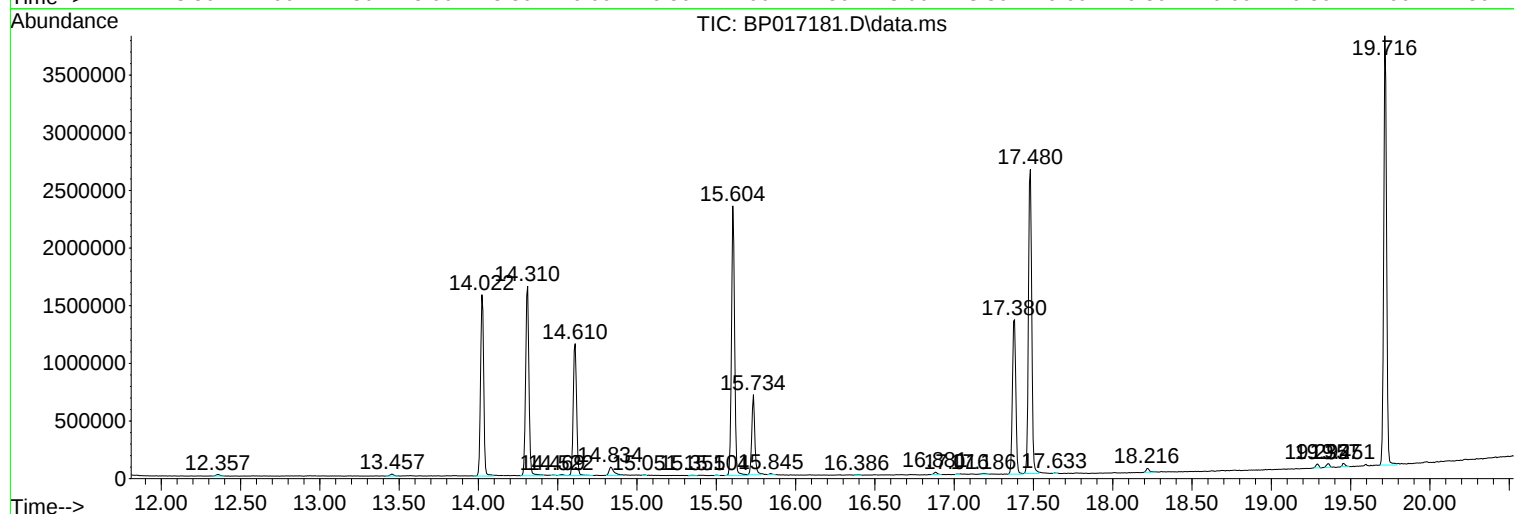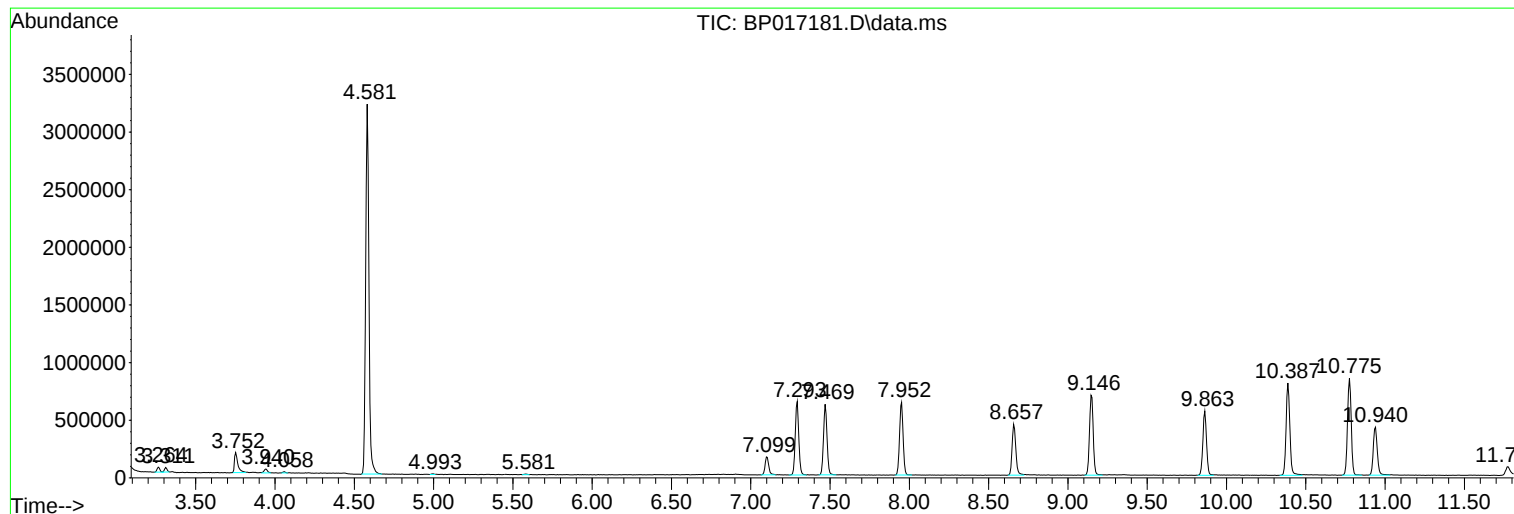

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017181.D
Acq On : 14 Sep 2023 17:31
Operator : MA/JU
Sample : 04324-08
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHG0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.581	92.02 ng/ul	4542380	1,4-Dichlorobenzene-d4	7.952

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

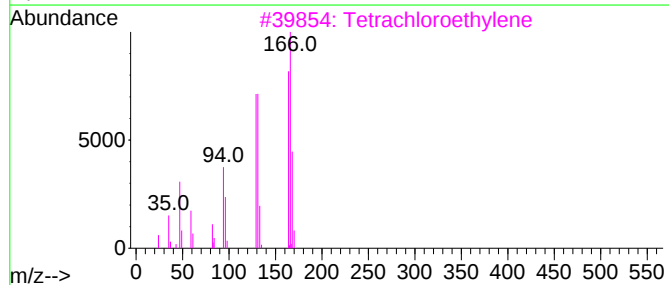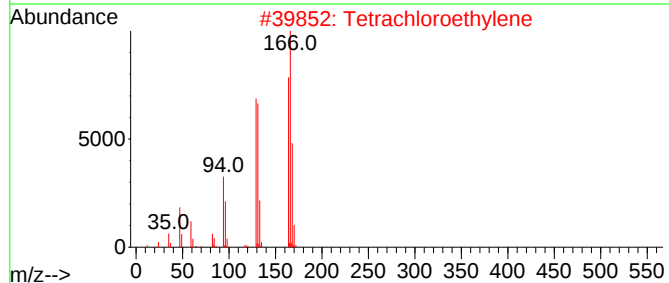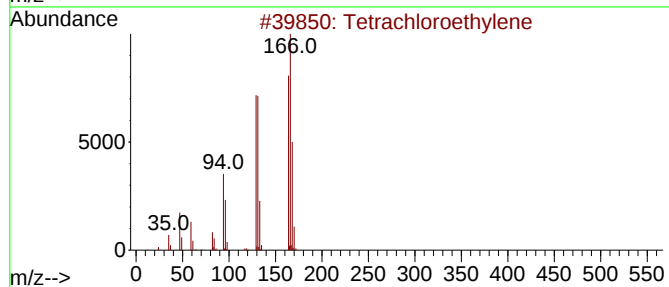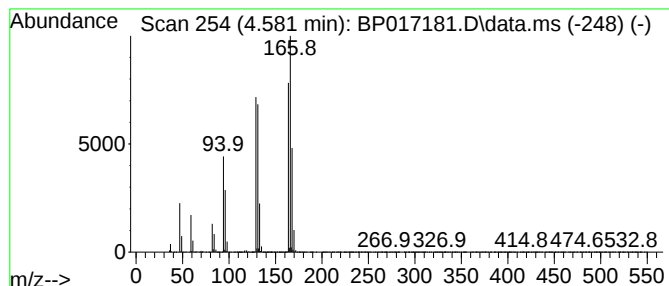

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017181.D
Acq On : 14 Sep 2023 17:31
Operator : MA/JU
Sample : 04324-08
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.581	92.0	ng/ul	4542380	1	7.952	987298	20.0