

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017185.D
 Acq On : 14 Sep 2023 19:49
 Operator : MA/JU
 Sample : PB155424BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK424

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	5	8	10	rBV2	15998	14289	0.46%	0.095%
2	3.158	10	12	14	rVV	28672	25394	0.82%	0.170%
3	3.187	14	17	22	rVV	529921	560809	18.10%	3.747%
4	3.234	22	25	29	rVB3	14396	16478	0.53%	0.110%
5	3.340	40	43	49	rVB3	15959	20091	0.65%	0.134%
6	3.546	75	78	86	rVB2	19121	27481	0.89%	0.184%
7	4.052	161	164	170	rVB3	17470	23911	0.77%	0.160%
8	4.205	186	190	195	rBV	26932	36495	1.18%	0.244%
9	4.263	196	200	204	rVB	30469	39725	1.28%	0.265%
10	4.358	211	216	219	rBV	54952	68591	2.21%	0.458%
11	4.399	219	223	228	rVB	55618	66011	2.13%	0.441%
12	5.028	327	330	334	rBV4	4297	4921	0.16%	0.033%
13	5.987	491	493	497	rVB4	4018	5111	0.16%	0.034%
14	6.534	581	586	590	rBV3	14554	22755	0.73%	0.152%
15	6.681	606	611	616	rBV	19311	29818	0.96%	0.199%
16	7.110	681	684	688	rVB6	2201	3276	0.11%	0.022%
17	7.228	702	704	710	rVB5	2499	3580	0.12%	0.024%
18	7.622	768	771	774	rBV5	2252	3808	0.12%	0.025%
19	7.946	819	826	837	rBV	905627	1401258	45.22%	9.363%
20	8.140	854	859	862	rBV6	2541	4438	0.14%	0.030%
21	10.328	1229	1231	1234	rVB3	3346	3234	0.10%	0.022%
22	10.775	1299	1307	1316	rBV	1113857	1857828	59.96%	12.414%
23	11.210	1377	1381	1384	rBV6	2760	4327	0.14%	0.029%
24	11.845	1485	1489	1493	rVB7	2883	4576	0.15%	0.031%
25	12.810	1652	1653	1661	rVB7	2393	4829	0.16%	0.032%
26	13.451	1758	1762	1764	rBV5	2595	3202	0.10%	0.021%
27	13.769	1812	1816	1818	rBV4	2492	3138	0.10%	0.021%
28	13.845	1825	1829	1839	rVB4	2874	6153	0.20%	0.041%
29	14.610	1951	1959	1967	rBV	1635129	2372664	76.57%	15.854%
30	15.404	2092	2094	2096	rBV3	2963	3422	0.11%	0.023%
31	16.180	2223	2226	2230	rBV6	2555	3913	0.13%	0.026%
32	16.804	2330	2332	2334	rBV3	2931	3461	0.11%	0.023%
33	17.169	2390	2394	2396	rBV4	3498	4579	0.15%	0.031%
34	17.380	2423	2430	2443	rBV	2105994	3098683	100.00%	20.705%
35	17.945	2524	2526	2528	rBV3	3974	3591	0.12%	0.024%
36	21.480	3122	3127	3137	rBV	2167995	2812764	90.77%	18.794%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017185.D
Acq On : 14 Sep 2023 19:49
Operator : MA/JU
Sample : PB155424BL
Misc : GCMS CONFIRMATION
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK424

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION

37 24.004 3549 3556 3572 rVB 1125123 2397385 77.37% 16.019%




Sum of corrected areas: 14965989

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017185.D
Acq On : 14 Sep 2023 19:49
Operator : MA/JU
Sample : PB155424BL
Misc : GCMS CONFIRMATION
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK424

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

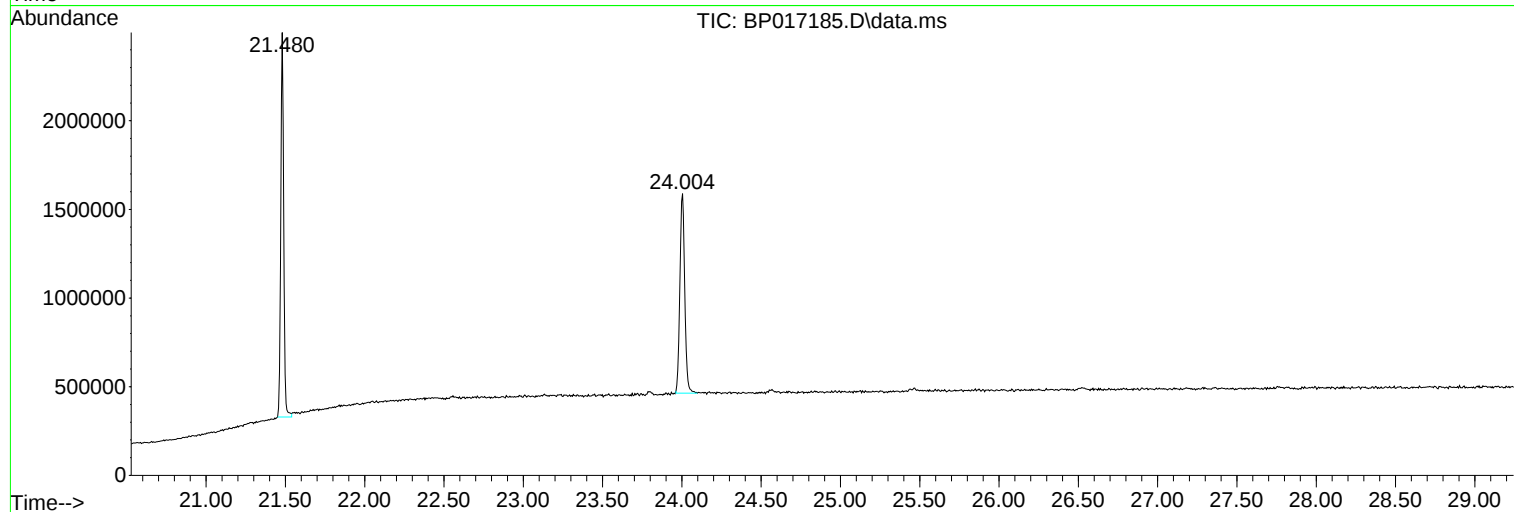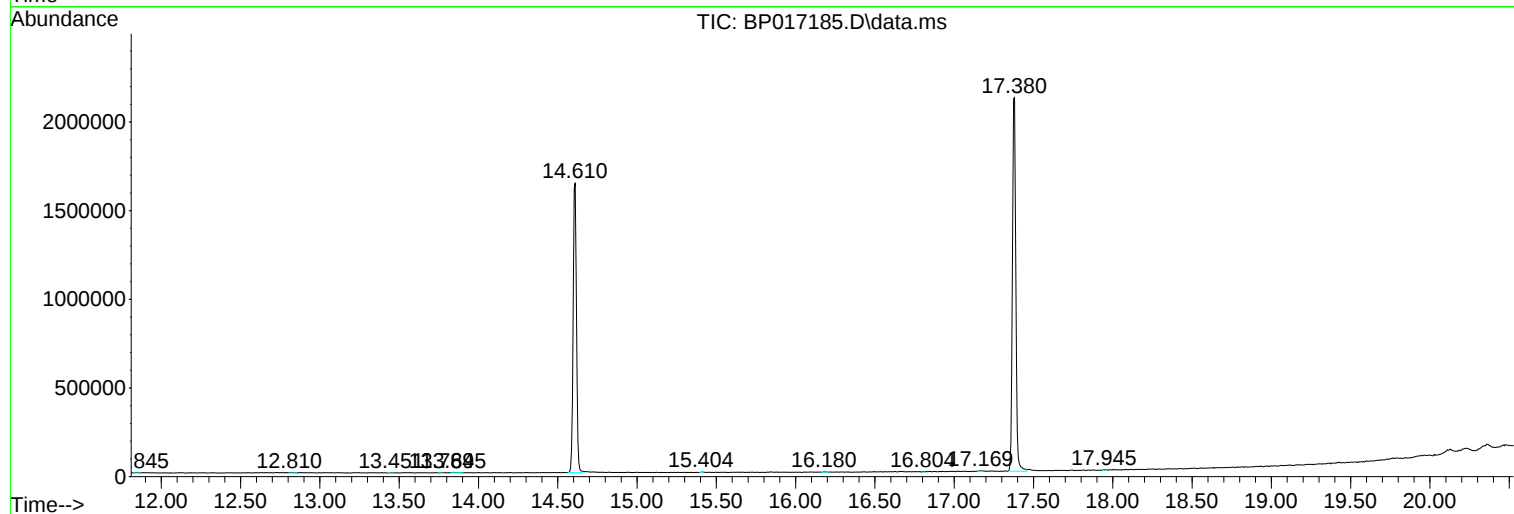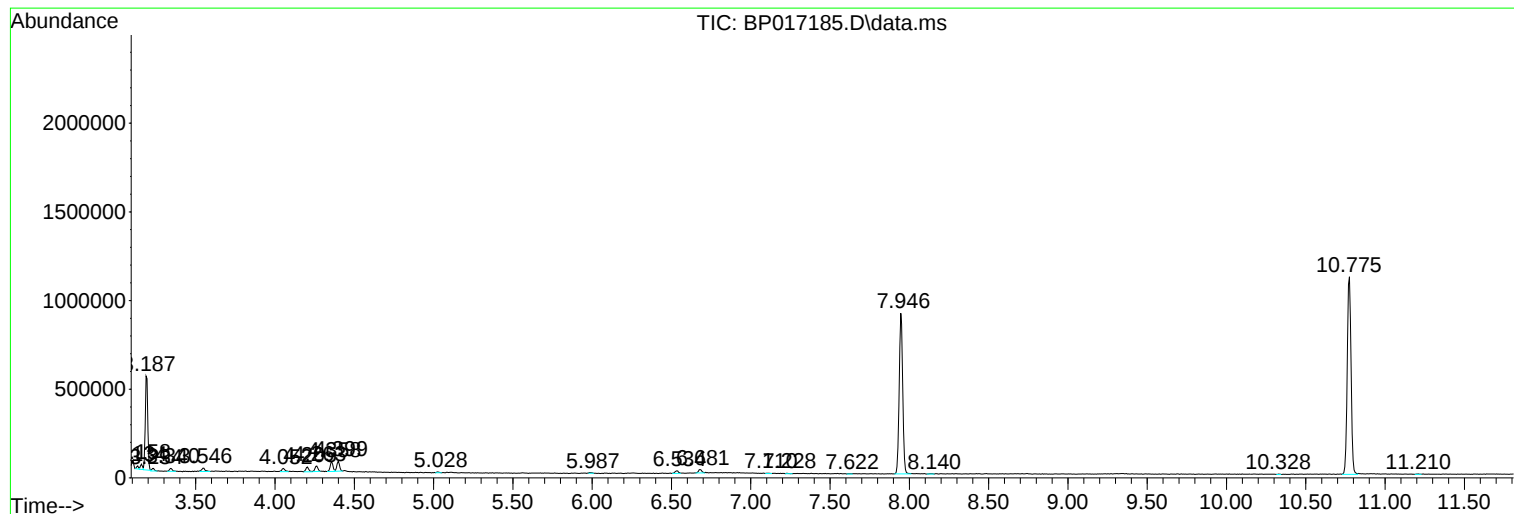

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017185.D
Acq On : 14 Sep 2023 19:49
Operator : MA/JU
Sample : PB155424BL
Misc : GCMS CONFIRMATION
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK424










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.187	8.00 ng/ul	560809	1,4-Dichlorobenzene-d4	7.946

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane	100	C7H16	000142-82-5	95
2			Heptane	100	C7H16	000142-82-5	94
3			Heptane	100	C7H16	000142-82-5	91
4			Heptane	100	C7H16	000142-82-5	87
5			Decane, 4-methyl-	156	C11H24	002847-72-5	42

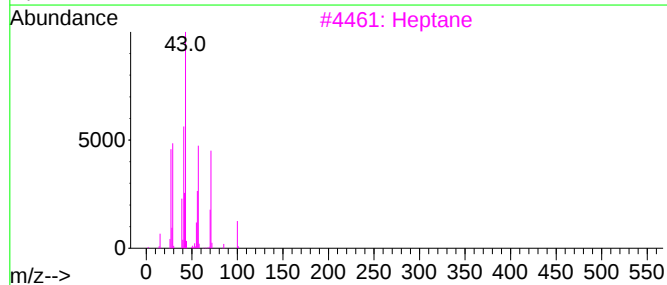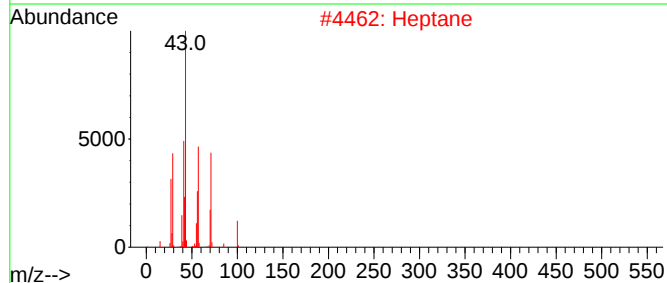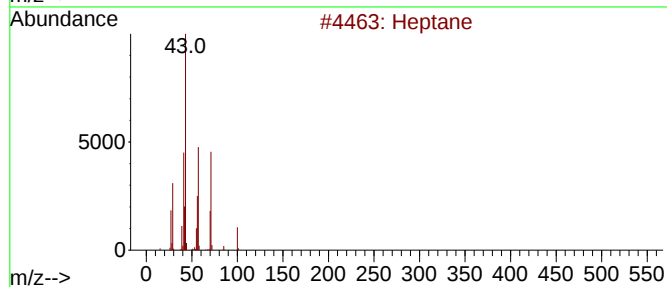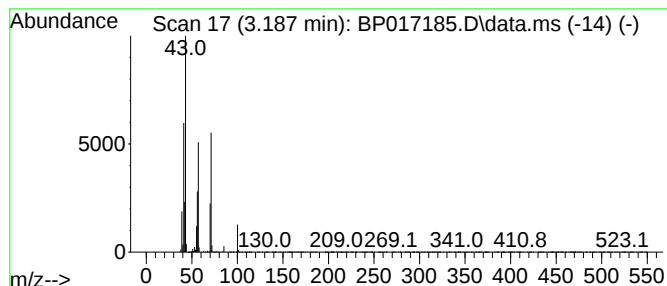

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017185.D
Acq On : 14 Sep 2023 19:49
Operator : MA/JU
Sample : PB155424BL
Misc : GCMS CONFIRMATION
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK424

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.187	8.0	ng/ul	560809	1	7.946	1401260	20.0