
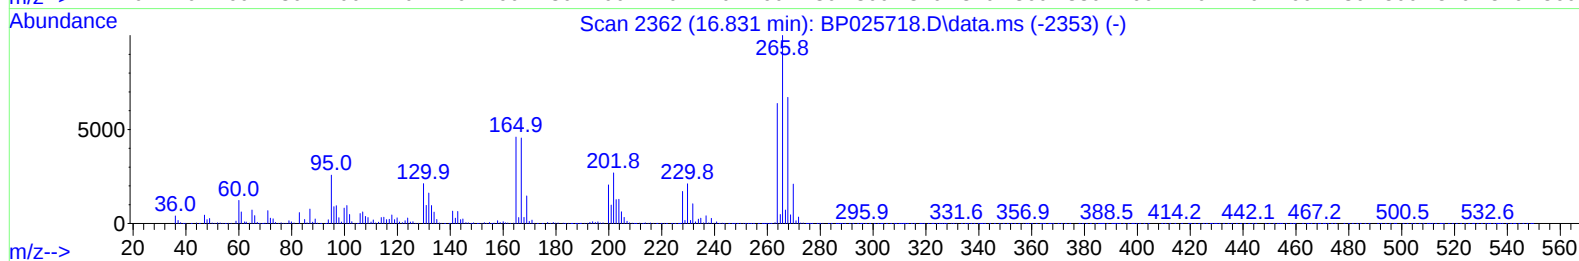
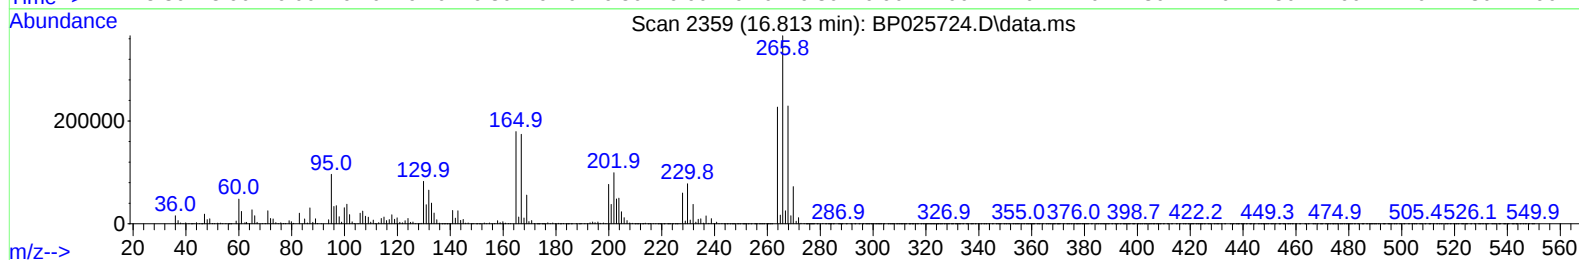


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091225\
Data File : BP025724.D
Acq On : 11 Sep 2025 08:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 12:58:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 09:20:45 2025
Response via : Initial Calibration

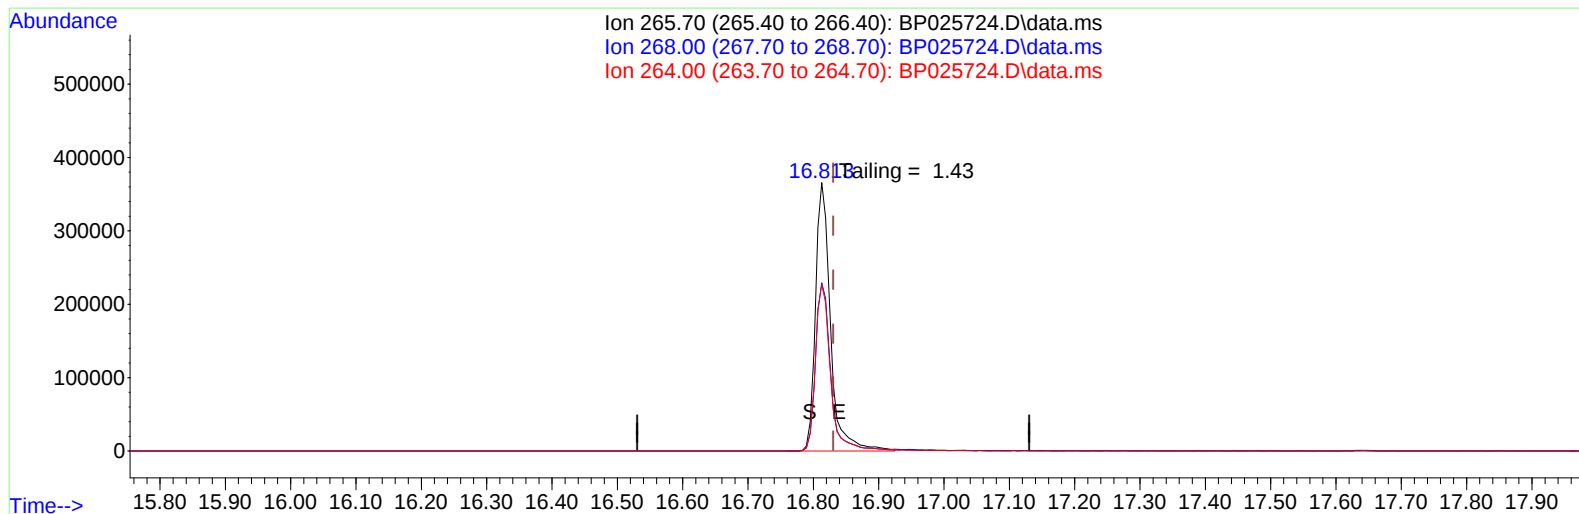

TIC: BP025724.D\data.ms

(70) Pentachlorophenol (C)




16.813min (-0.018) 7217.81 ng

response 589827

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	62.64
264.00	63.80	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091225\
Data File : BP025724.D
Acq On : 11 Sep 2025 08:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 12:58:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 09:20:45 2025
Response via : Initial Calibration

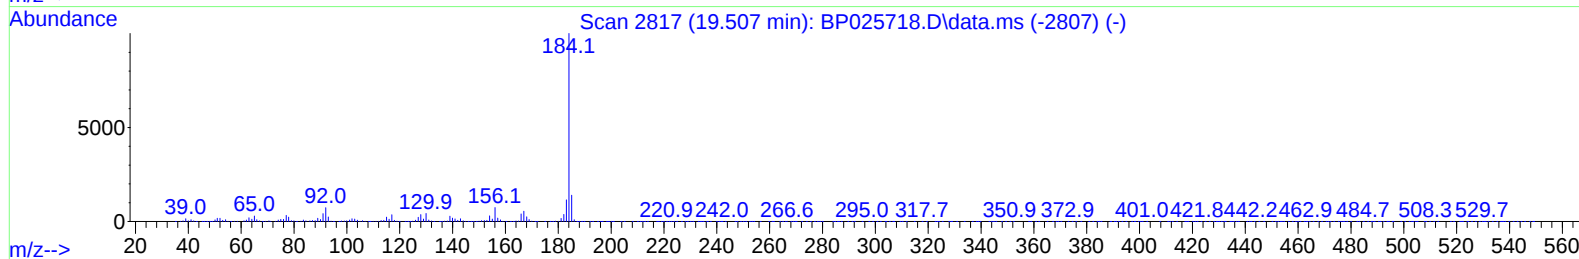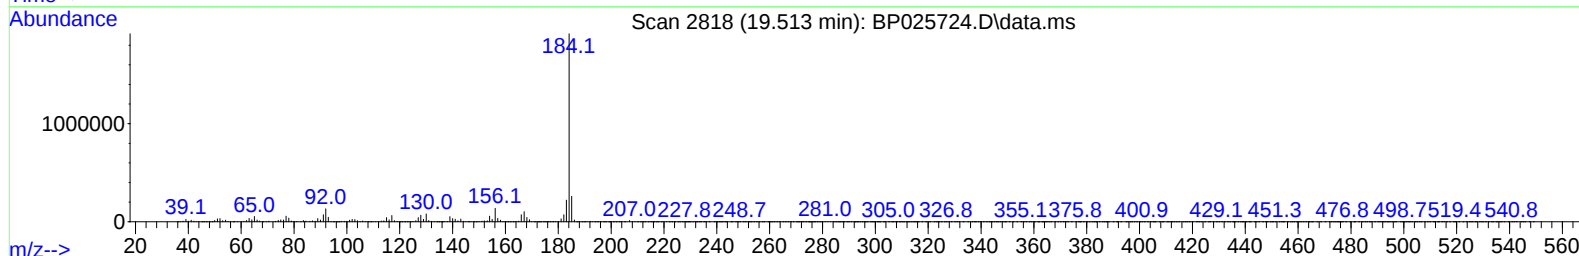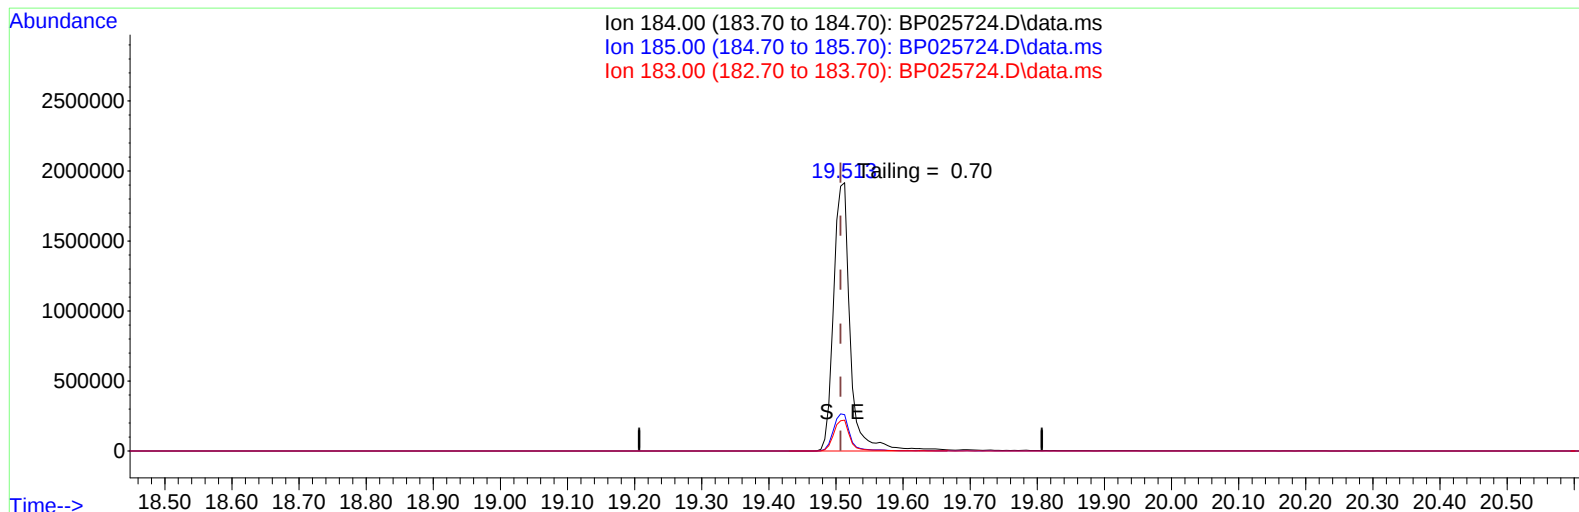

TIC: BP025724.D\data.ms

(77) Benzidine

19.513min (+ 0.006) 4369.52 ng

response 3272403

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.55
183.00	11.50	11.52
0.00	0.00	0.00