
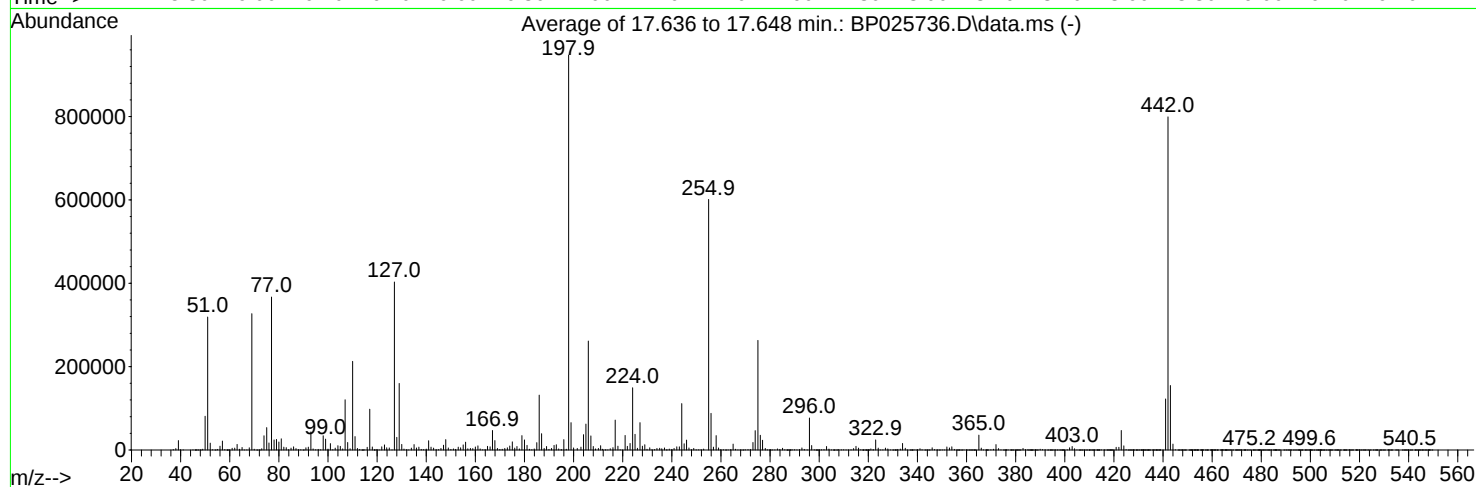


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091225\
Data File : BP025736.D
Acq On : 12 Sep 2025 09:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

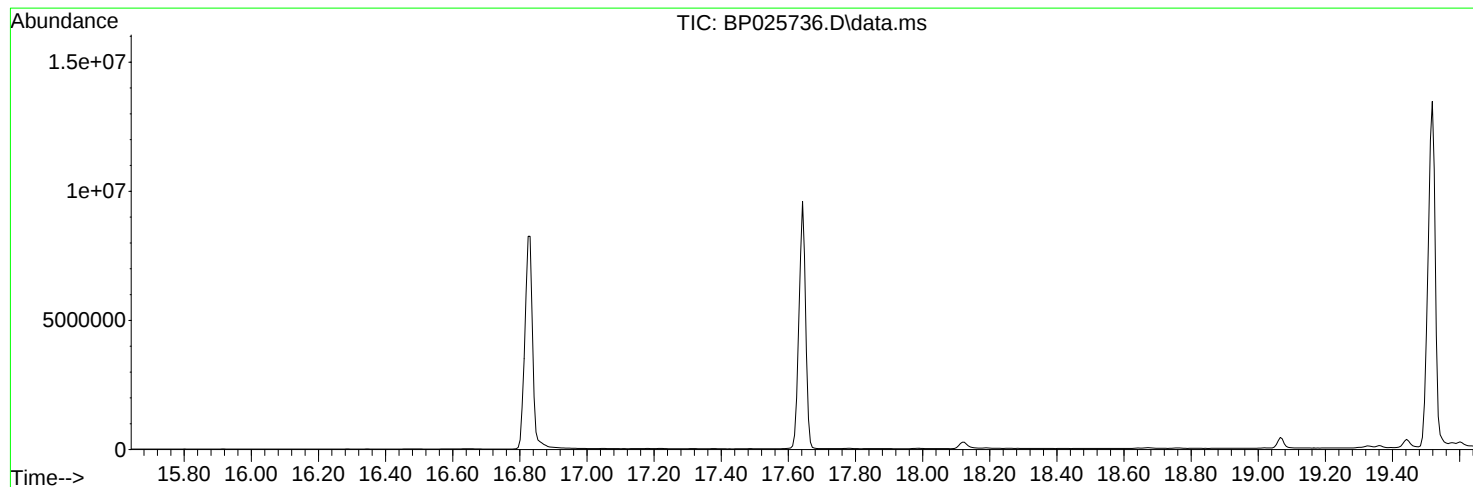




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2488

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	5570	PASS
69	69	100	100	100.0	327198	PASS
70	69	0.00	2	0.6	1811	PASS
197	198	0.00	2	0.2	1889	PASS
198	198	100	100	100.0	947266	PASS
199	198	5	9	7.0	65837	PASS
365	198	1	100	3.8	35856	PASS
441	443	0.01	150	79.1	122467	PASS
442	442	100	100	100.0	799360	PASS
443	442	15	24	19.4	154797	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091225\
Data File : BP025736.D
Acq On : 12 Sep 2025 09:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 12 11:24:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

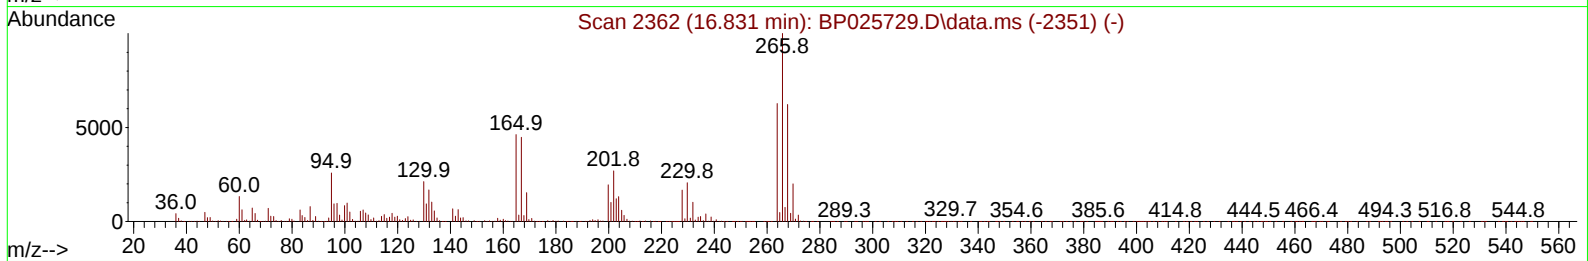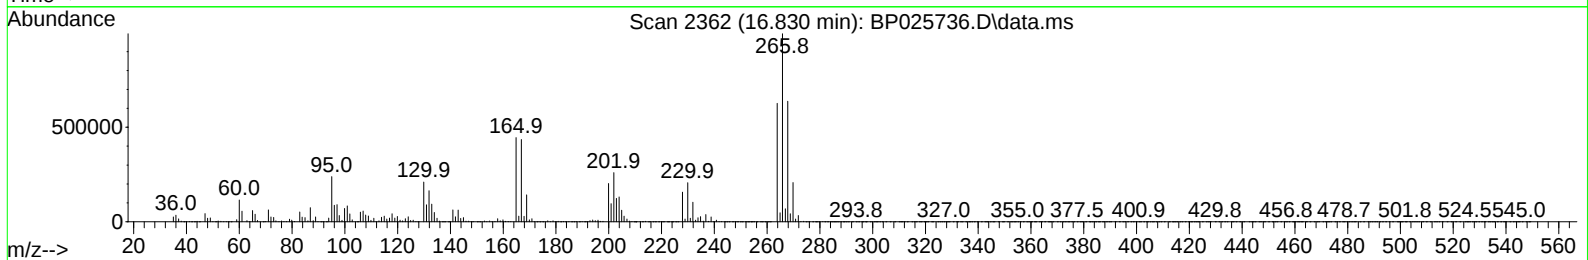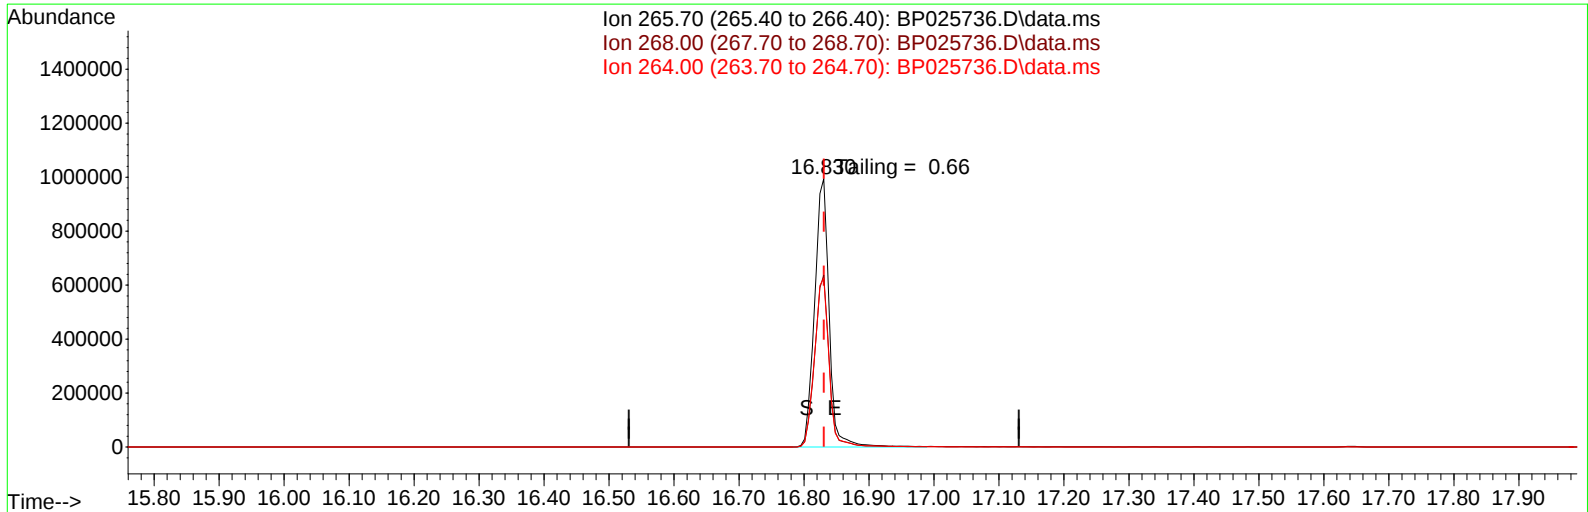

TIC: BP025736.D\data.ms

(70) Pentachlorophenol (C)

16.830min (-0.000) 27880.92 ng




response 1551454

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.05
264.00	62.70	62.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091225\
Data File : BP025736.D
Acq On : 12 Sep 2025 09:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 12 11:24:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

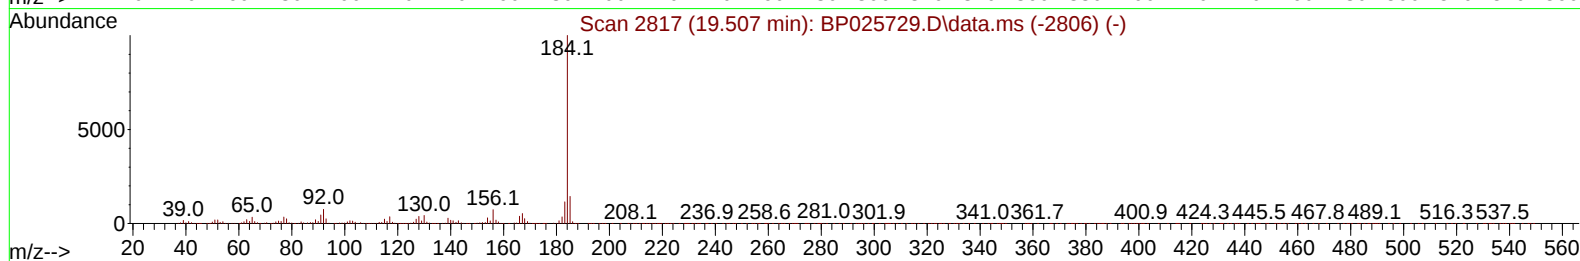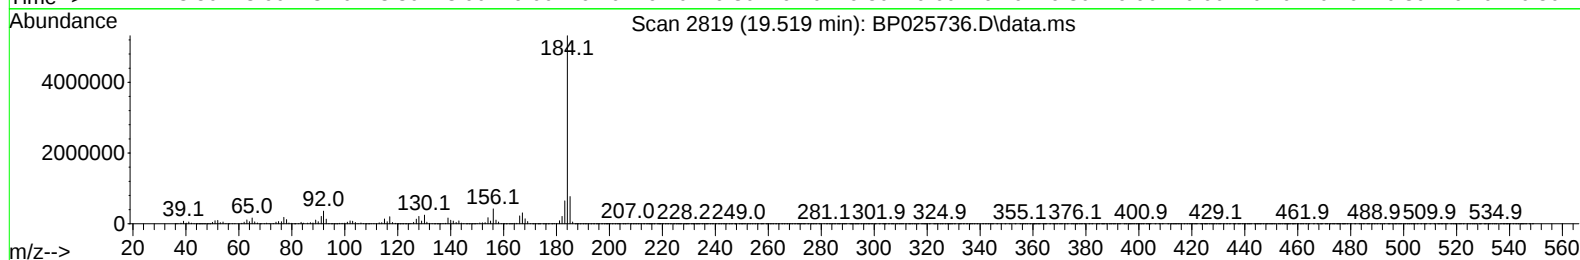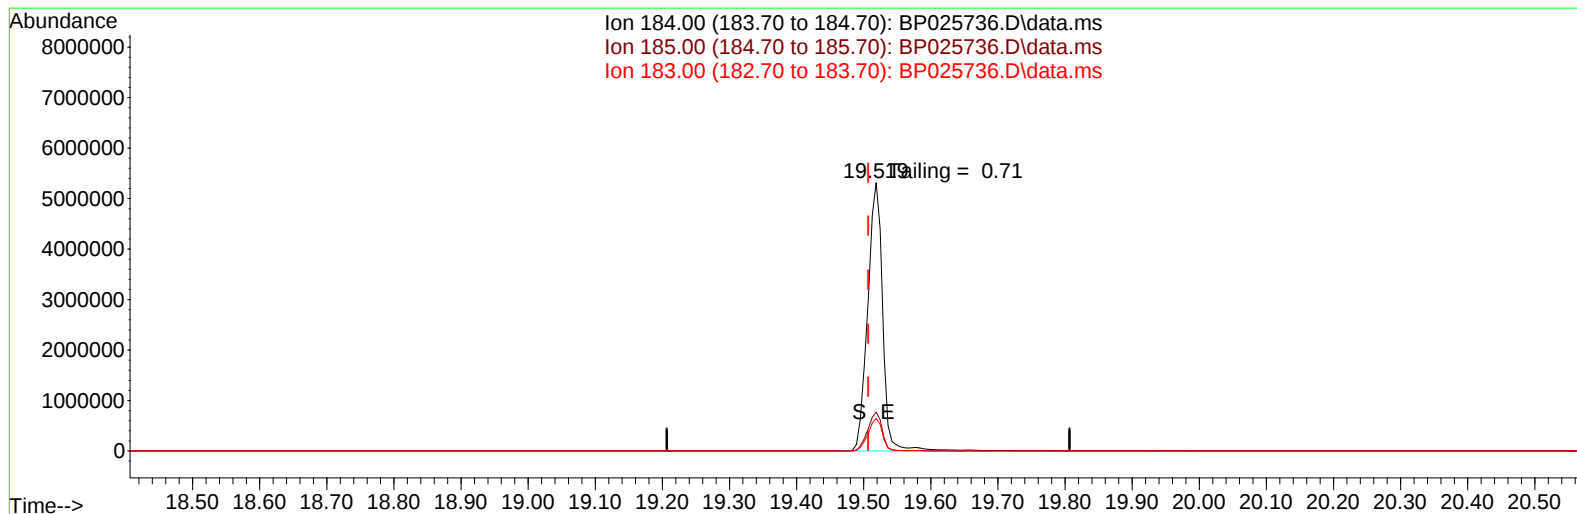

TIC: BP025736.D\data.ms

(77) Benzidine

19.519min (+ 0.012) 6627.59 ng

response 8052586

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.47
183.00	11.50	12.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/12/2025	BNA_P	<u>BP025736.D</u>
Compound Name	Response	Retention Time
DDT	4308532	20.801
DDD	67643	20.336
DDE	7246	19.819
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
74889	4383421	1.71

Instrument :
BNA_P
ClientSampleId :
DFTPP