
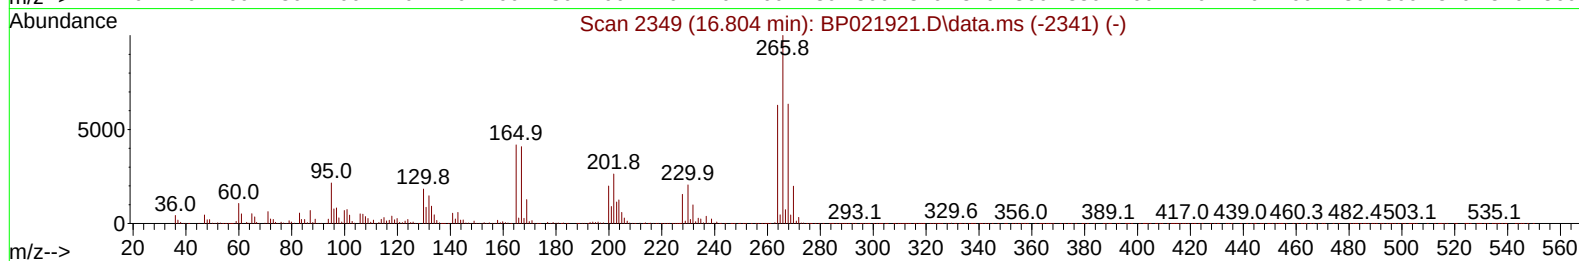
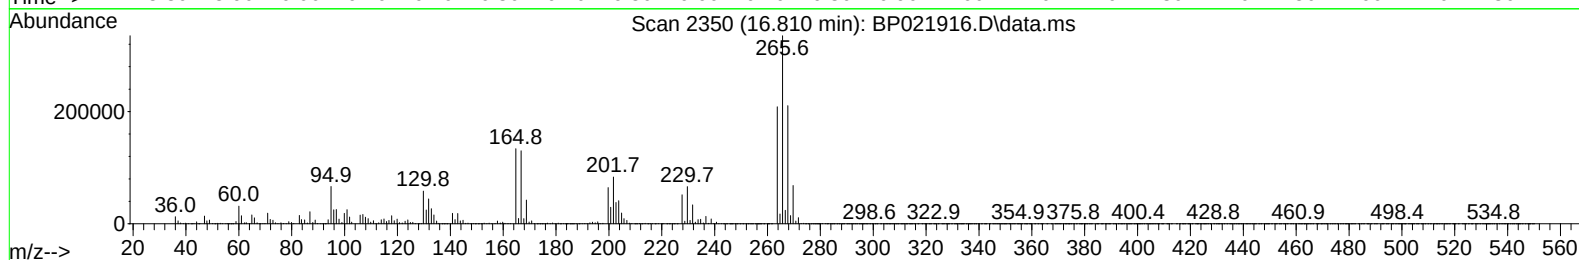


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091424\
Data File : BP021916.D
Acq On : 14 Sep 2024 11:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 05:22:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 05:10:07 2024
Response via : Initial Calibration

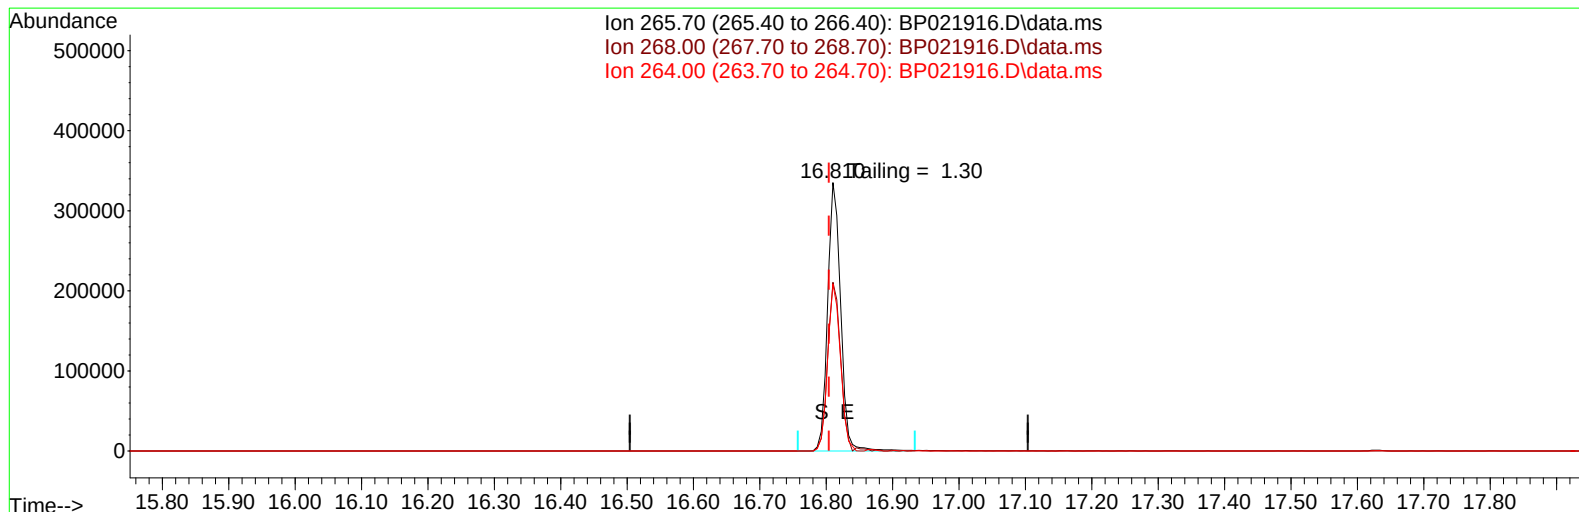

TIC: BP021916.D\data.ms

(70) Pentachlorophenol (C)




16.810min (+ 0.006) 1671591.33 ng

response 458665

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	67.15
264.00	62.90	67.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091424\
Data File : BP021916.D
Acq On : 14 Sep 2024 11:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 05:22:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 05:10:07 2024
Response via : Initial Calibration

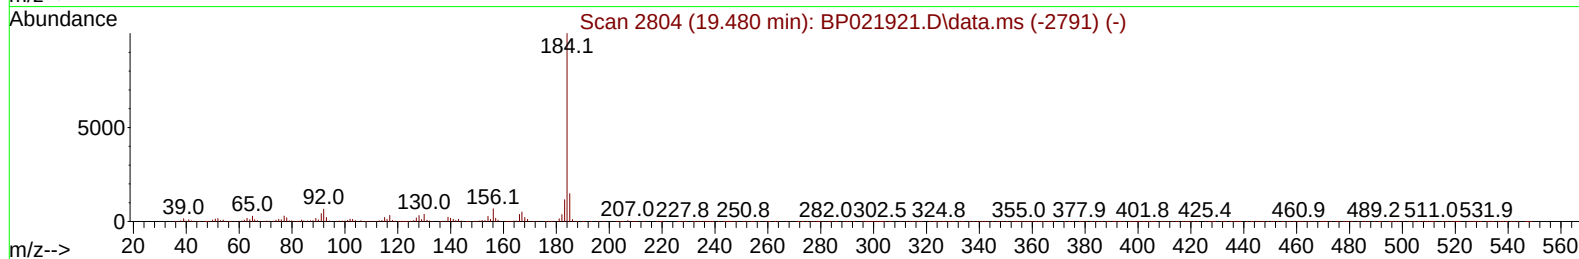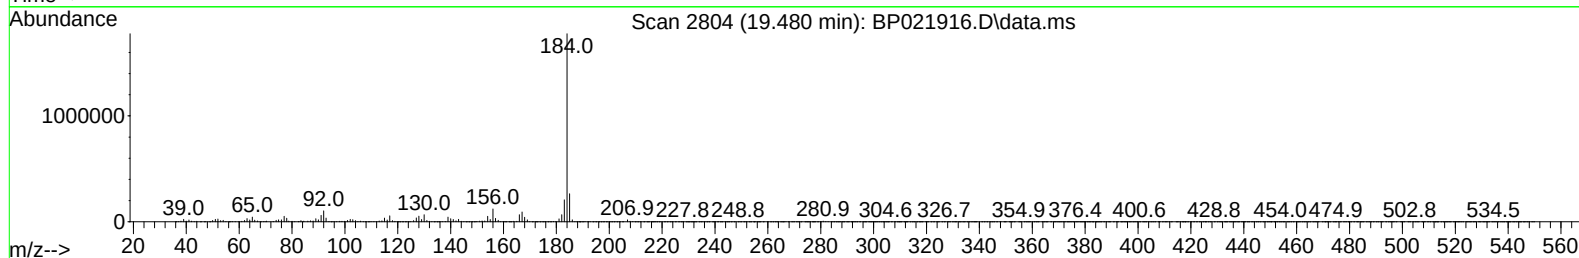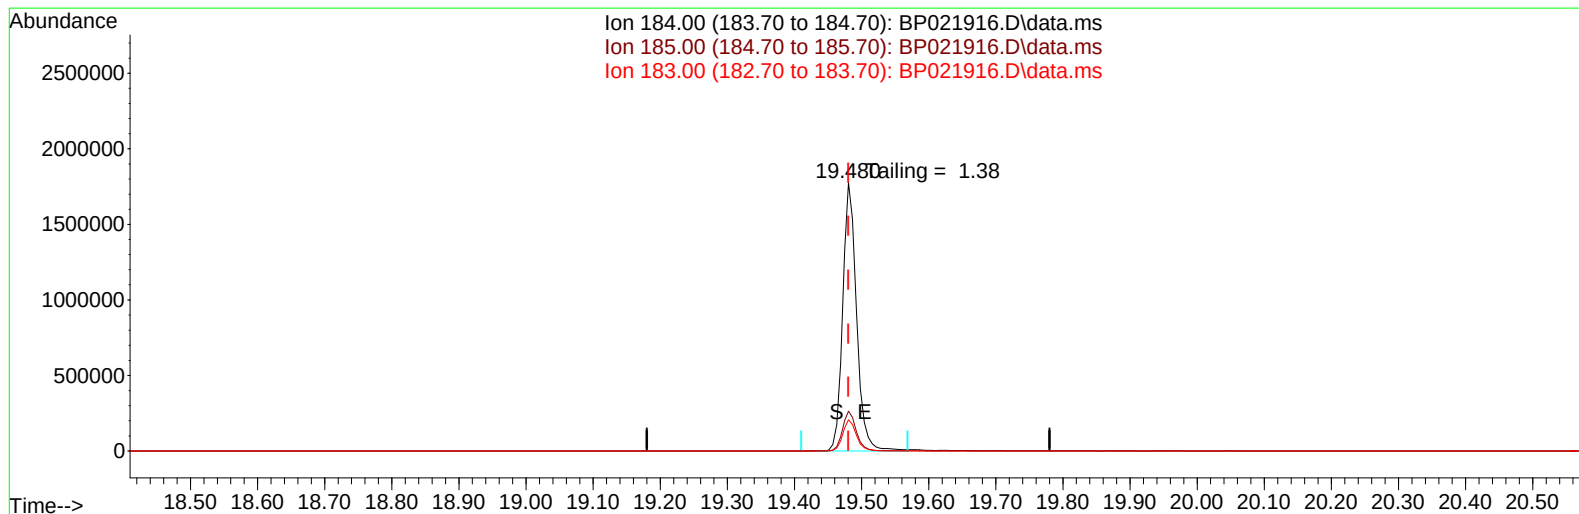

TIC: BP021916.D\data.ms

(77) Benzidine**19.480min (+ 0.000) 4374994.28 ng****response 2551109**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.86
183.00	11.60	11.64
0.00	0.00	0.00