


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091424\
Data File : BP021916.D
Acq On : 14 Sep 2024 11:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Sep 15 05:10:07 2024

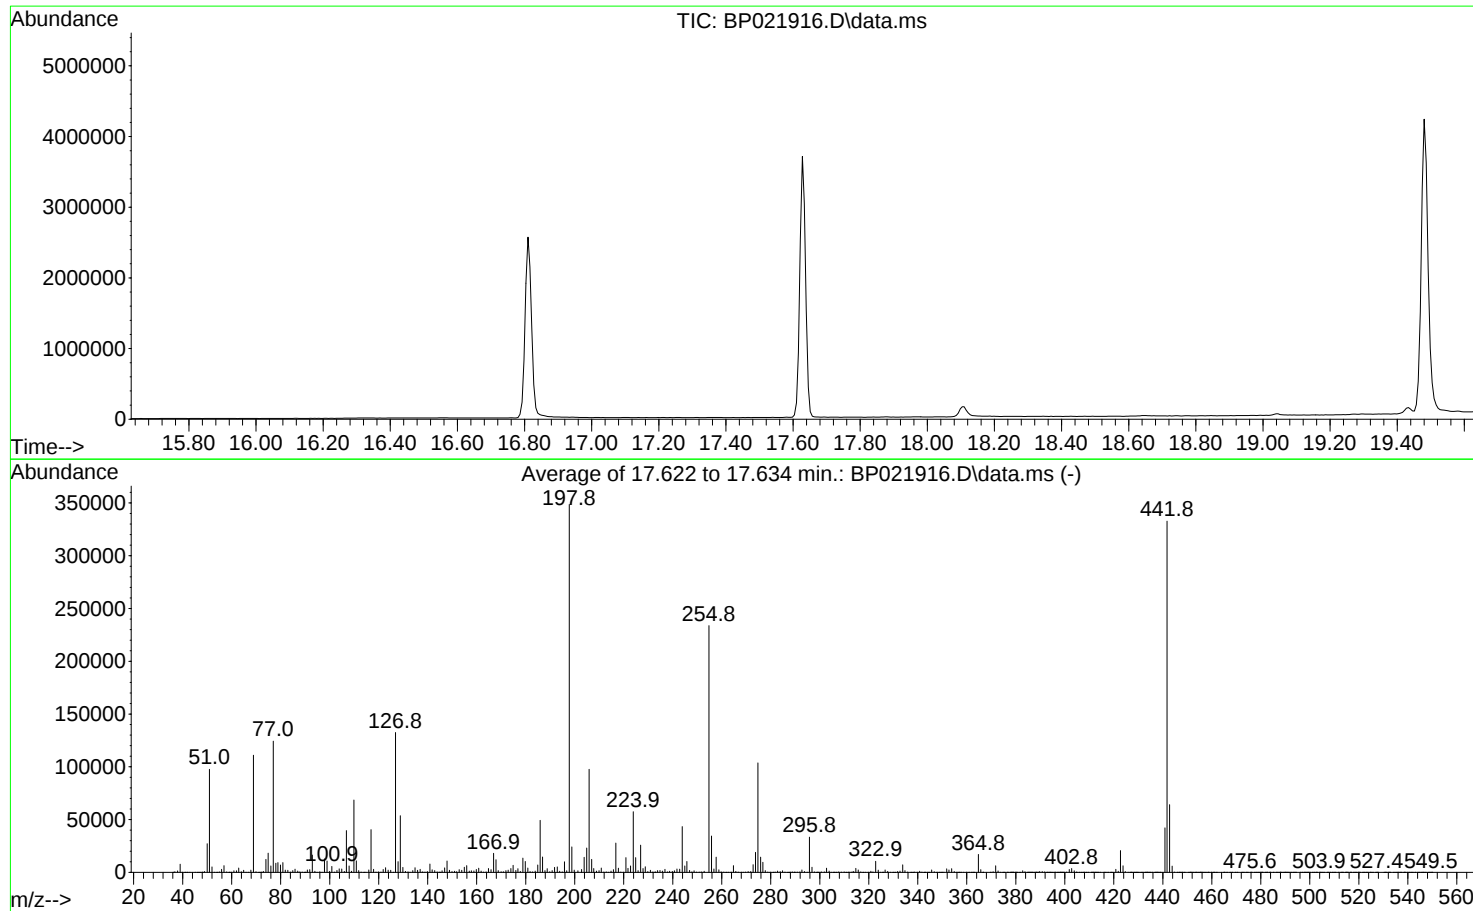




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	97676	PASS
68	69	0.00	2	2.0	2178	PASS
69	198	0.00	100	31.8	110952	PASS
70	69	0.00	2	0.5	579	PASS
127	198	10	80	38.0	132458	PASS
197	198	0.00	2	0.5	1584	PASS
198	198	100	100	100.0	348523	PASS
199	198	5	9	6.9	24034	PASS
275	198	10	60	29.7	103667	PASS
365	198	1	100	4.9	16941	PASS
441	198	0.01	100	12.1	42208	PASS
442	442	100	100	100.0	332810	PASS
443	442	15	24	19.3	64117	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091424\
Data File : BP021916.D
Acq On : 14 Sep 2024 11:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 15 05:22:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 05:10:07 2024
Response via : Initial Calibration

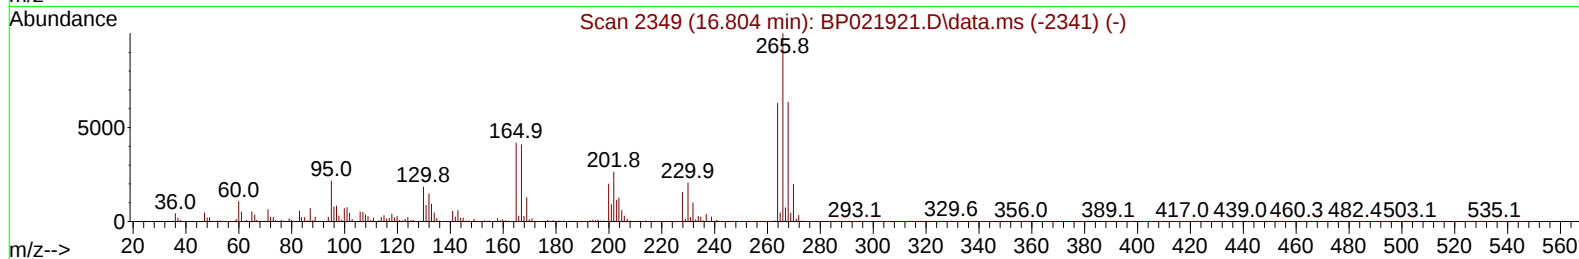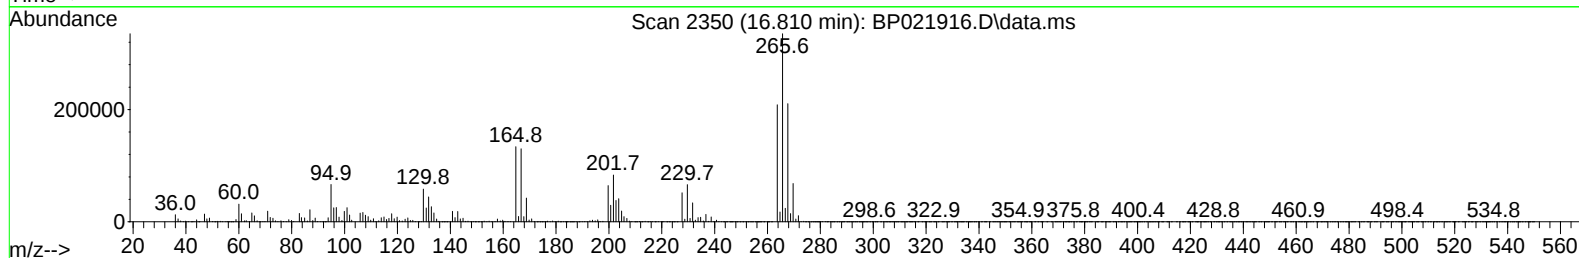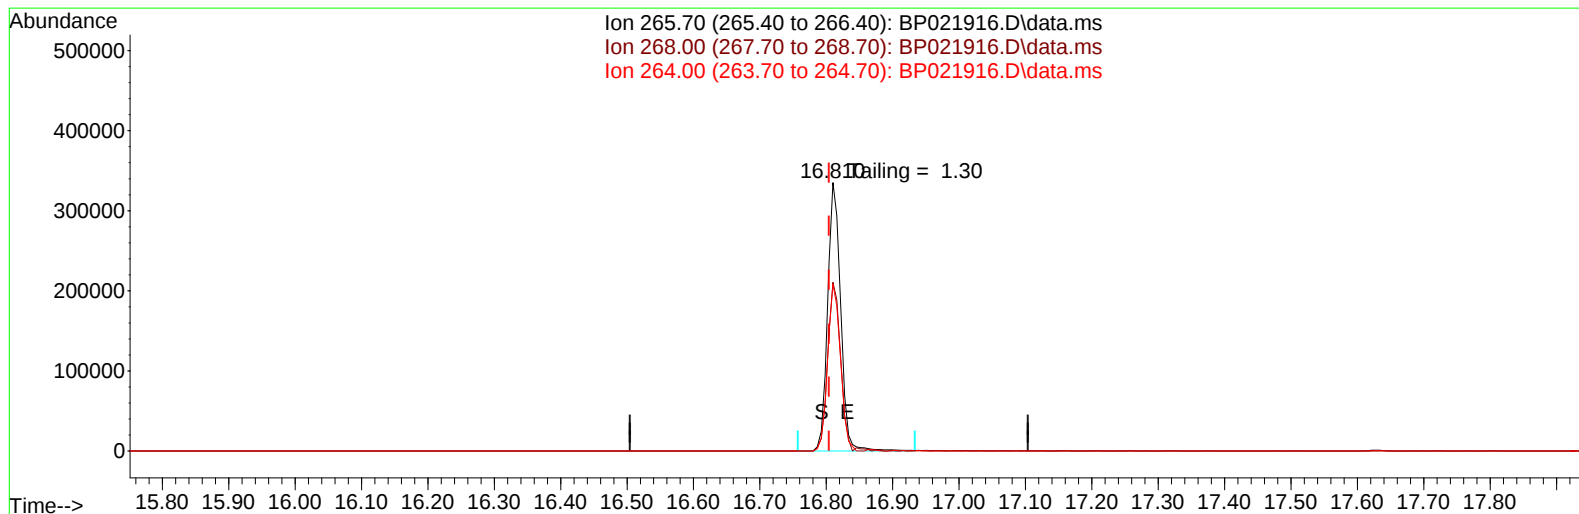

TIC: BP021916.D\data.ms

(70) Pentachlorophenol (C)

16.810min (+ 0.006) 1671591.33 ng




response 458665

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	67.15
264.00	62.90	67.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091424\
Data File : BP021916.D
Acq On : 14 Sep 2024 11:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 15 05:22:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 05:10:07 2024
Response via : Initial Calibration

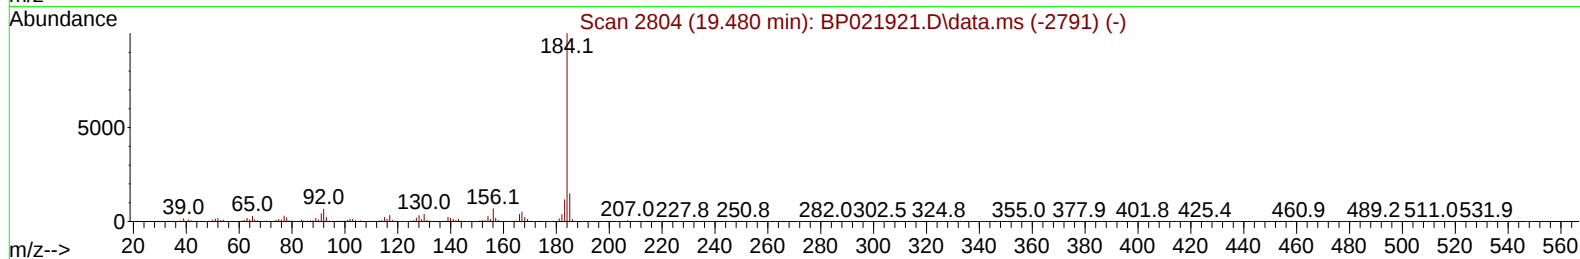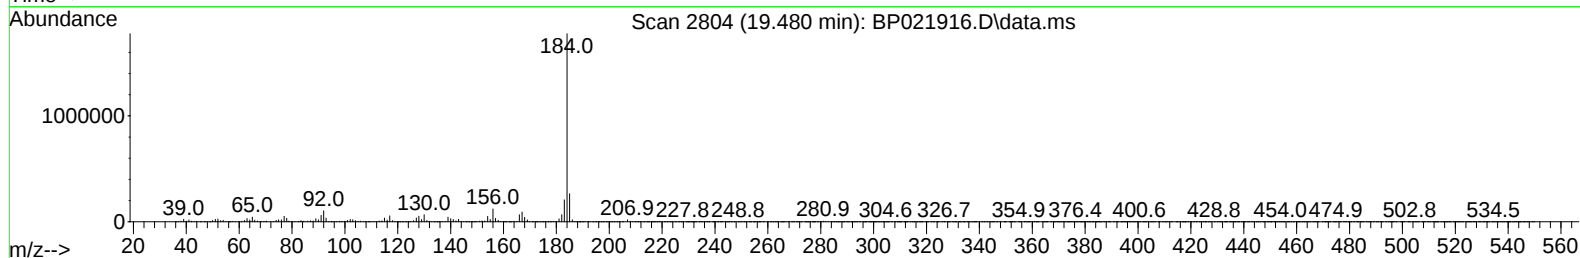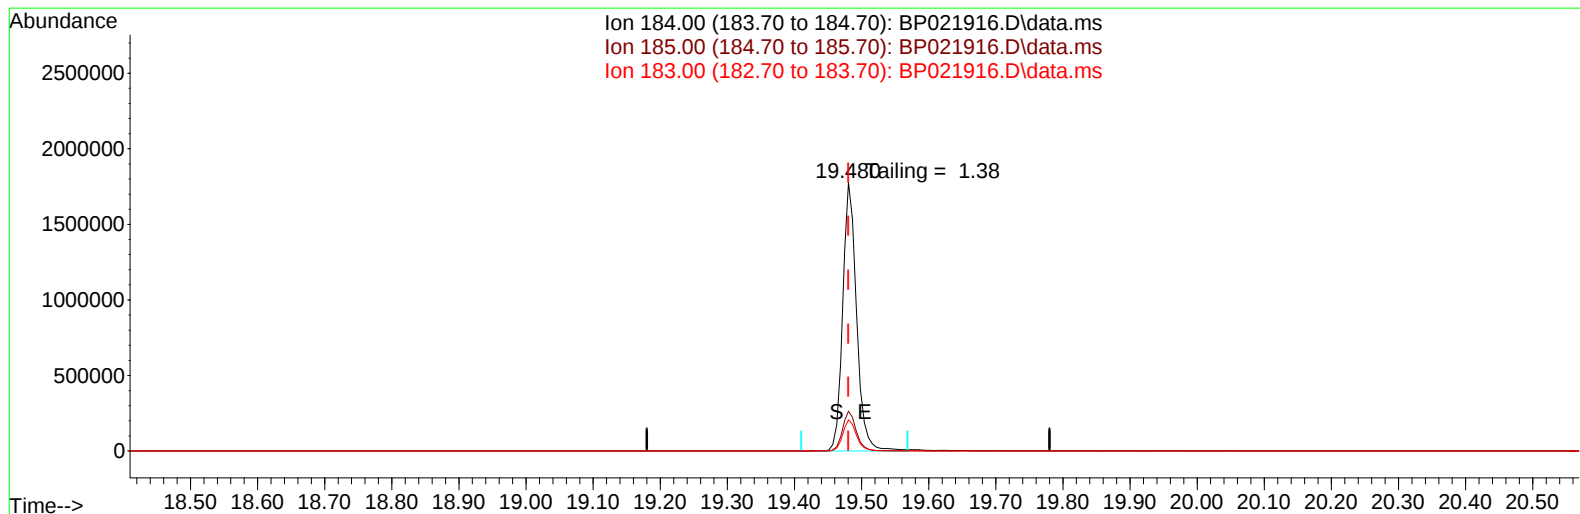

TIC: BP021916.D\data.ms

(77) Benzidine

19.480min (+ 0.000) 4374994.28 ng

response 2551109

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.86
183.00	11.60	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/16/2024	BNA_P	<u>BP021916.D</u>
Compound Name	Response	Retention Time
DDT	1401184	20.775
DDD	12912	20.369
DDE	0	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12912	1414096	0.91

Instrument :
BNA_P
ClientSampleId :
DFTPP