
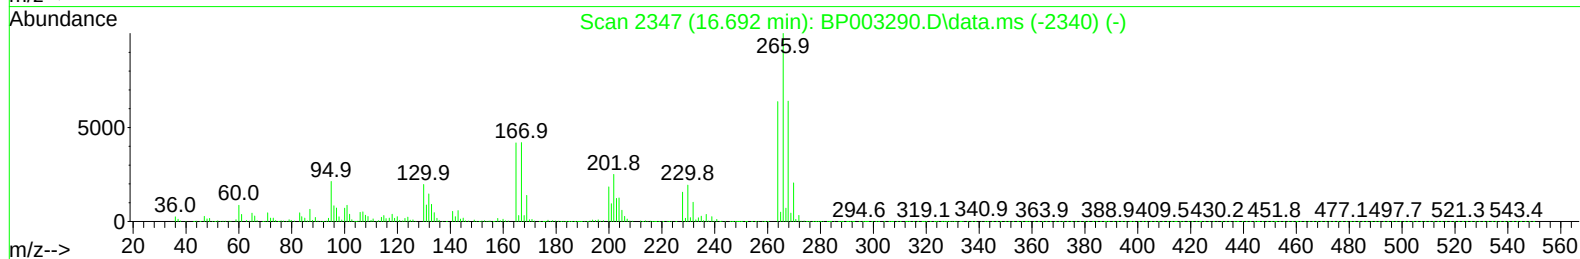
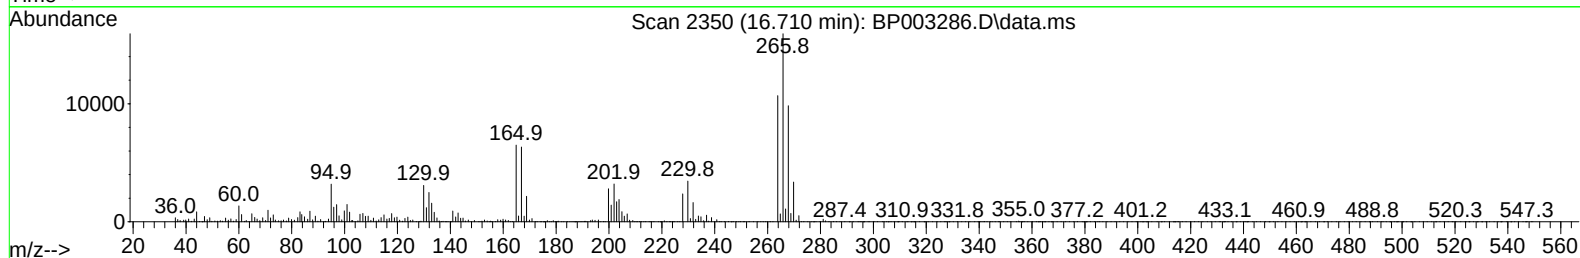


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091520\
Data File : BP003286.D
Acq On : 15 Sep 2020 13:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 10:21:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 17:55:44 2020
Response via : Initial Calibration

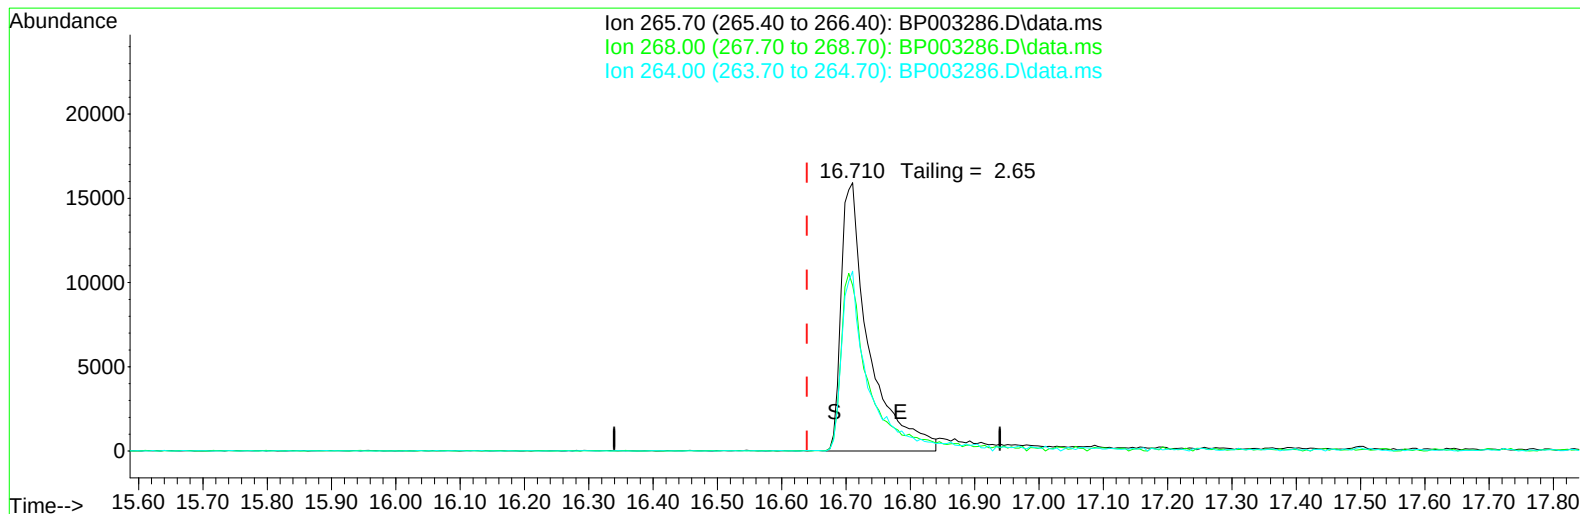

TIC: BP003286.D\data.ms

(70) Pentachlorophenol (C)




16.710min (+ 0.071) 319284.12 ng

response 47299

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	61.70
264.00	63.30	67.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091520\
 Data File : BP003286.D
 Acq On : 15 Sep 2020 13:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 10:21:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 28 17:55:44 2020
 Response via : Initial Calibration

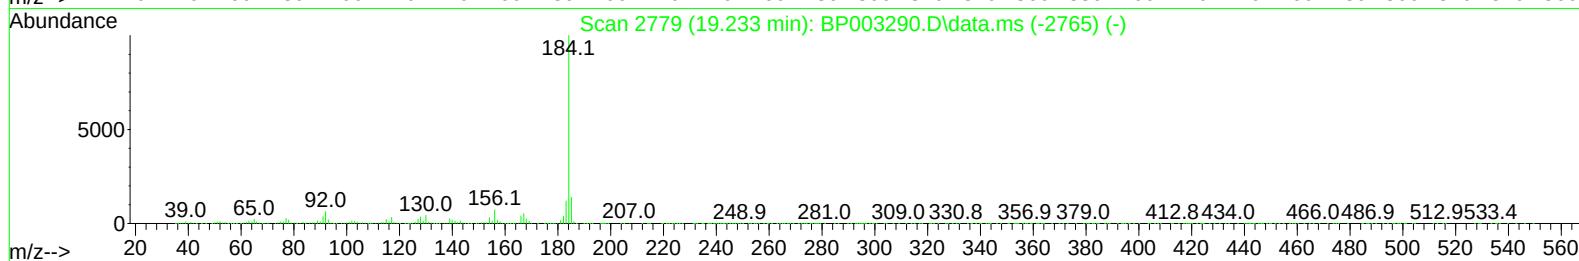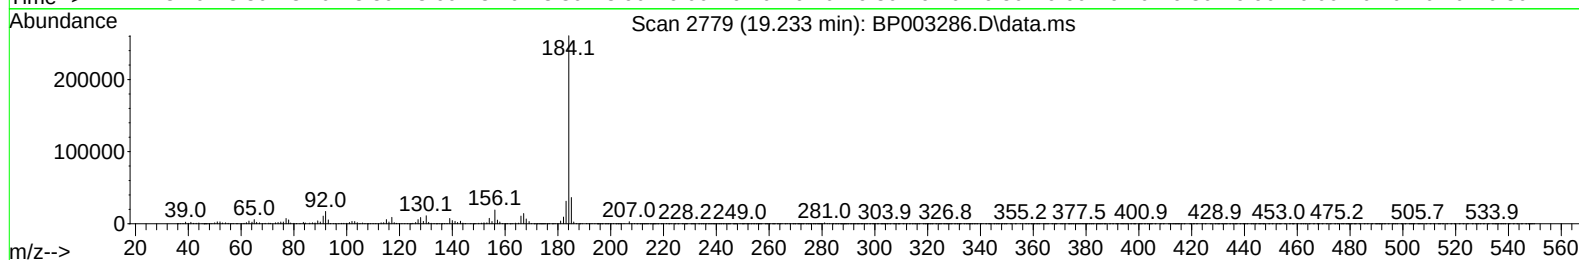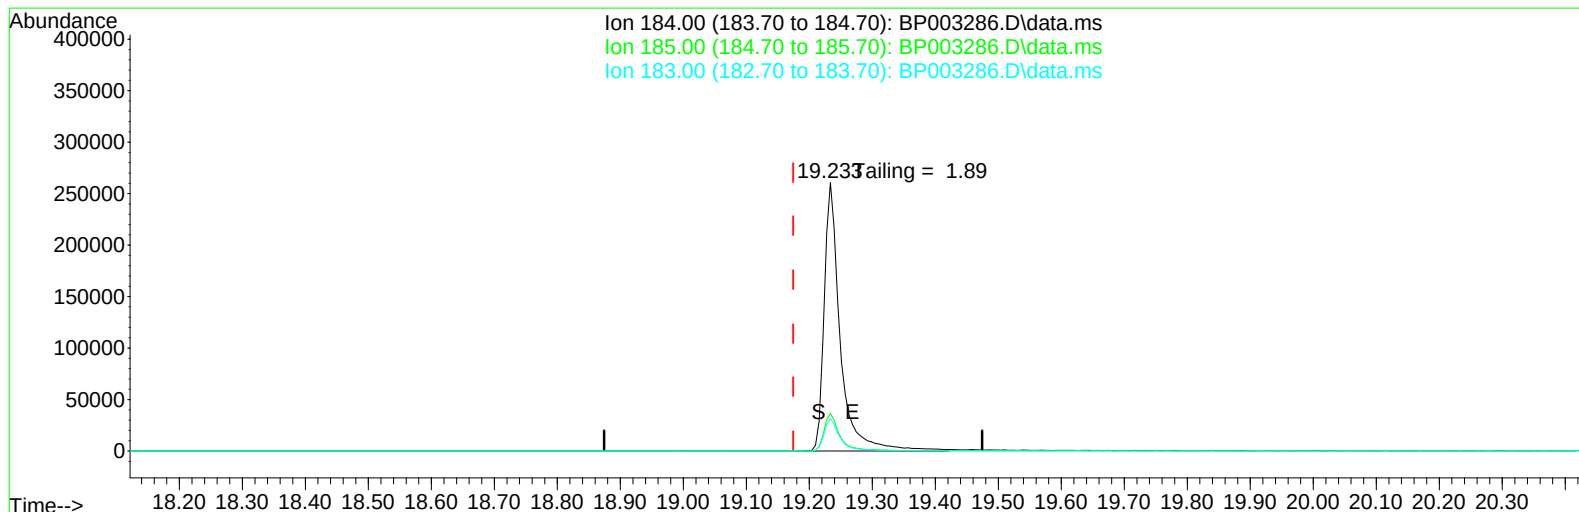

TIC: BP003286.D\data.ms

(77) Benzidine**19.233min (+ 0.059) 879142.81 ng****response 463440**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.96
183.00	12.00	12.03
0.00	0.00	0.00