
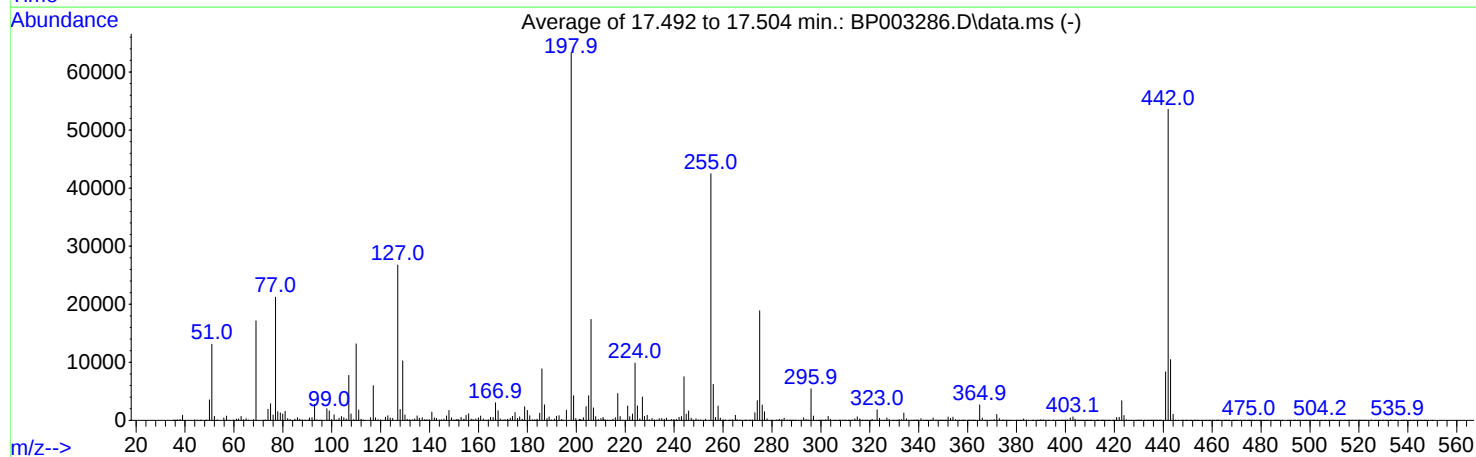


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP091520\  
Data File : BP003286.D  
Acq On : 15 Sep 2020 13:02  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP091520.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Sep 16 13:18:39 2020

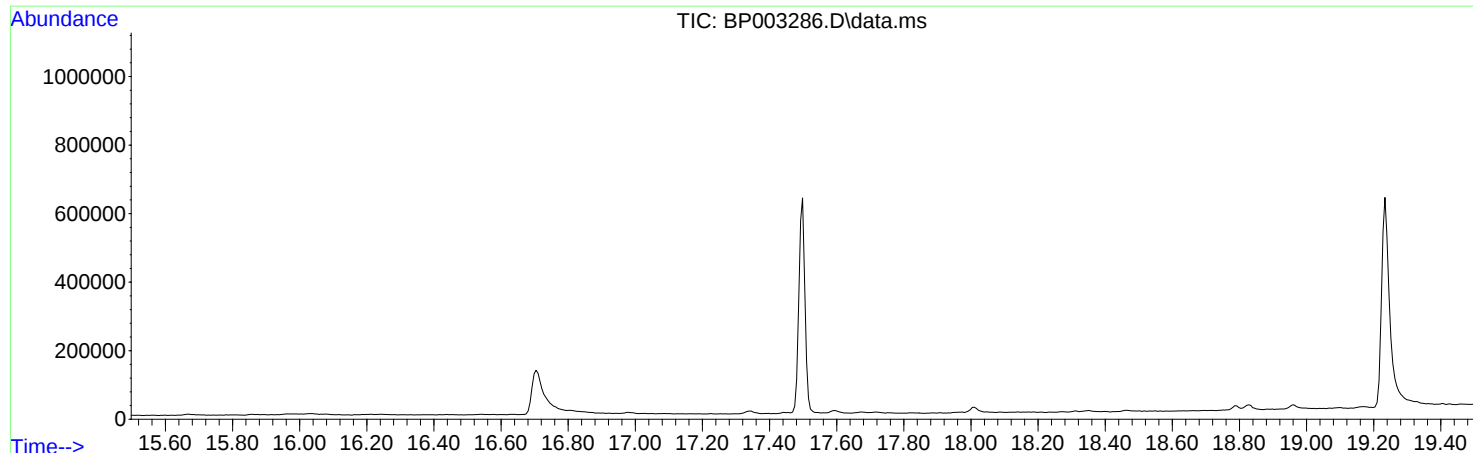

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2474

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 20.7         | 13131      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.8          | 139        | PASS                |
| 69             | 198             | 0.00            | 100             | 27.1         | 17147      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 42.2         | 26764      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 63358      | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 4244       | PASS                |
| 275            | 198             | 10              | 60              | 29.8         | 18883      | PASS                |
| 365            | 198             | 1               | 100             | 4.2          | 2677       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.2         | 8353       | PASS                |
| 442            | 198             | 50              | 100             | 84.5         | 53565      | PASS                |
| 443            | 442             | 15              | 24              | 19.6         | 10476      | PASS                |