

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
 Data File : BP017190.D
 Acq On : 15 Sep 2023 16:27
 Operator : MA/JU
 Sample : PB155306BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK306

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017190.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	34	38	45	rVB	57354	71005	2.11%	0.208%
2	3.746	109	112	130	rBV	435276	652357	19.37%	1.915%
3	4.058	161	165	169	rBV3	9495	12064	0.36%	0.035%
4	7.099	675	682	696	rBV	705244	1092427	32.43%	3.206%
5	7.293	708	715	725	rVB	563048	890066	26.43%	2.612%
6	7.469	738	745	754	rBV	712827	1107599	32.88%	3.251%
7	7.822	800	805	806	rBV5	2195	3541	0.11%	0.010%
8	7.946	820	826	836	rBV	533183	838948	24.91%	2.462%
9	8.434	905	909	912	rBV5	2717	3422	0.10%	0.010%
10	8.657	939	947	962	rBV	803361	1270806	37.73%	3.730%
11	9.146	1023	1030	1038	rBV	623595	988317	29.34%	2.901%
12	9.334	1061	1062	1070	rVB8	3436	4936	0.15%	0.014%
13	9.857	1145	1151	1166	rBV	484016	779845	23.15%	2.289%
14	10.387	1234	1241	1255	rBV	730361	1249500	37.10%	3.667%
15	10.775	1299	1307	1318	rBV	669948	1128358	33.50%	3.312%
16	10.934	1327	1334	1345	rBV	500587	858783	25.50%	2.521%
17	12.357	1569	1576	1584	rBV3	12214	20686	0.61%	0.061%
18	13.034	1688	1691	1695	rVB5	2140	3742	0.11%	0.011%
19	13.134	1705	1708	1712	rBV6	1862	3476	0.10%	0.010%
20	13.451	1757	1762	1768	rBV10	5456	10895	0.32%	0.032%
21	13.569	1778	1782	1791	rVB10	3506	7563	0.22%	0.022%
22	13.857	1827	1831	1834	rVB5	2053	3591	0.11%	0.011%
23	14.022	1852	1859	1877	rBV	1180262	1650010	48.99%	4.843%
24	14.304	1900	1907	1927	rBV	1335138	1936527	57.49%	5.684%
25	14.451	1930	1932	1939	rVB7	3233	6145	0.18%	0.018%
26	14.604	1951	1958	1969	rBV2	925144	1340962	39.81%	3.936%
27	14.828	1990	1996	2013	rBV	372003	705447	20.94%	2.070%
28	15.004	2024	2026	2029	rVB4	3193	3370	0.10%	0.010%
29	15.287	2070	2074	2076	rVB5	2667	3397	0.10%	0.010%
30	15.410	2091	2095	2097	rBV5	2804	3884	0.12%	0.011%
31	15.604	2120	2128	2143	rBV	1838718	2549029	75.68%	7.481%
32	15.728	2144	2149	2165	rVV	409783	605099	17.96%	1.776%
33	15.839	2165	2168	2174	rVB7	10021	15751	0.47%	0.046%
34	16.192	2226	2228	2232	rVB4	3074	3480	0.10%	0.010%
35	16.663	2306	2308	2313	rVB4	3666	4813	0.14%	0.014%
36	17.157	2390	2392	2395	rBV4	3223	3986	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
Data File : BP017190.D
Acq On : 15 Sep 2023 16:27
Operator : MA/JU
Sample : PB155306BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK306

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION

37	17.375	2422	2429	2439	rBV	1128619	1552870	46.10%	4.558%
38	17.475	2440	2446	2460	rVV	1941440	2713292	80.56%	7.963%
39	18.169	2562	2564	2567	rBV4	2724	3377	0.10%	0.010%
40	19.286	2751	2754	2758	rBV4	22654	27989	0.83%	0.082%
41	19.357	2763	2766	2769	rBV	17397	21618	0.64%	0.063%
42	19.716	2822	2827	2838	rBV	2608692	3173996	94.23%	9.316%
43	21.480	3122	3127	3133	rBV	1216896	1621111	48.13%	4.758%
44	23.833	3521	3527	3541	rVB2	1696904	3368228	100.00%	9.886%
45	24.004	3550	3556	3567	rVB	853480	1755559	52.12%	5.153%




Sum of corrected areas: 34071867

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
Data File : BP017190.D
Acq On : 15 Sep 2023 16:27
Operator : MA/JU
Sample : PB155306BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

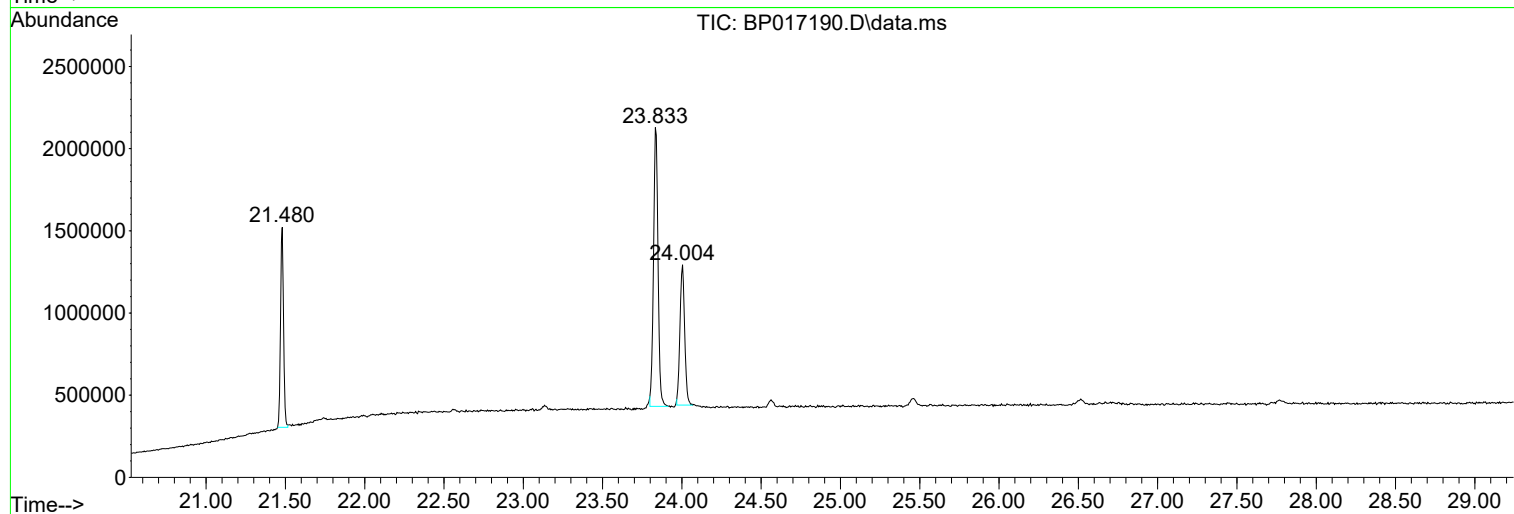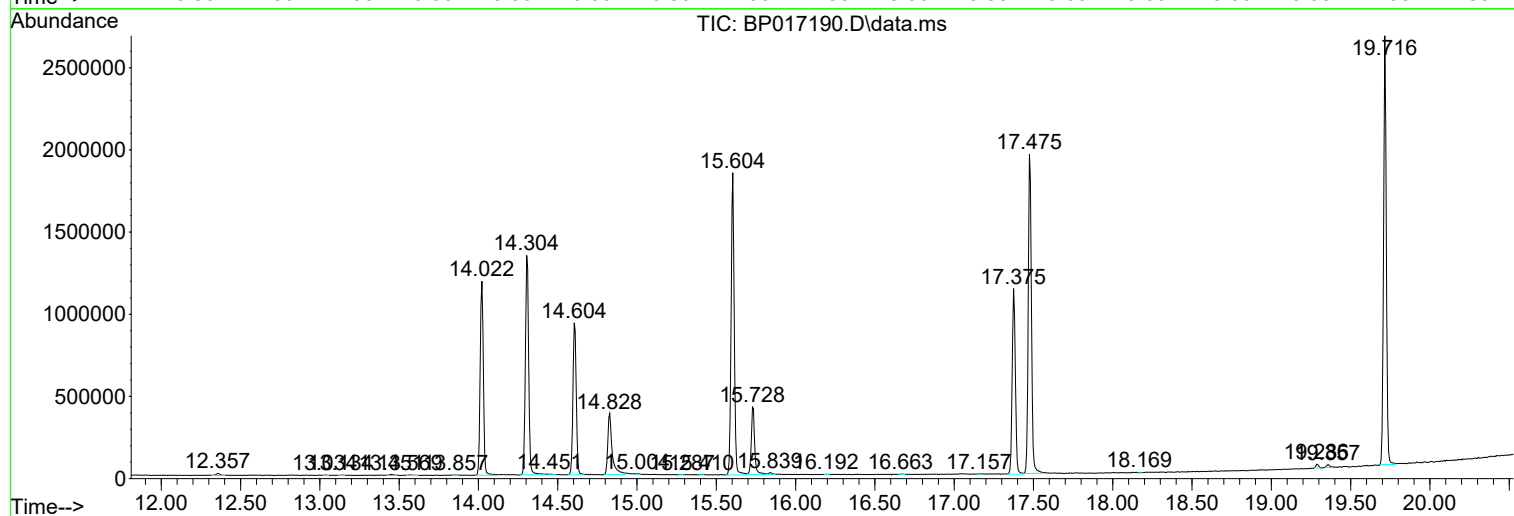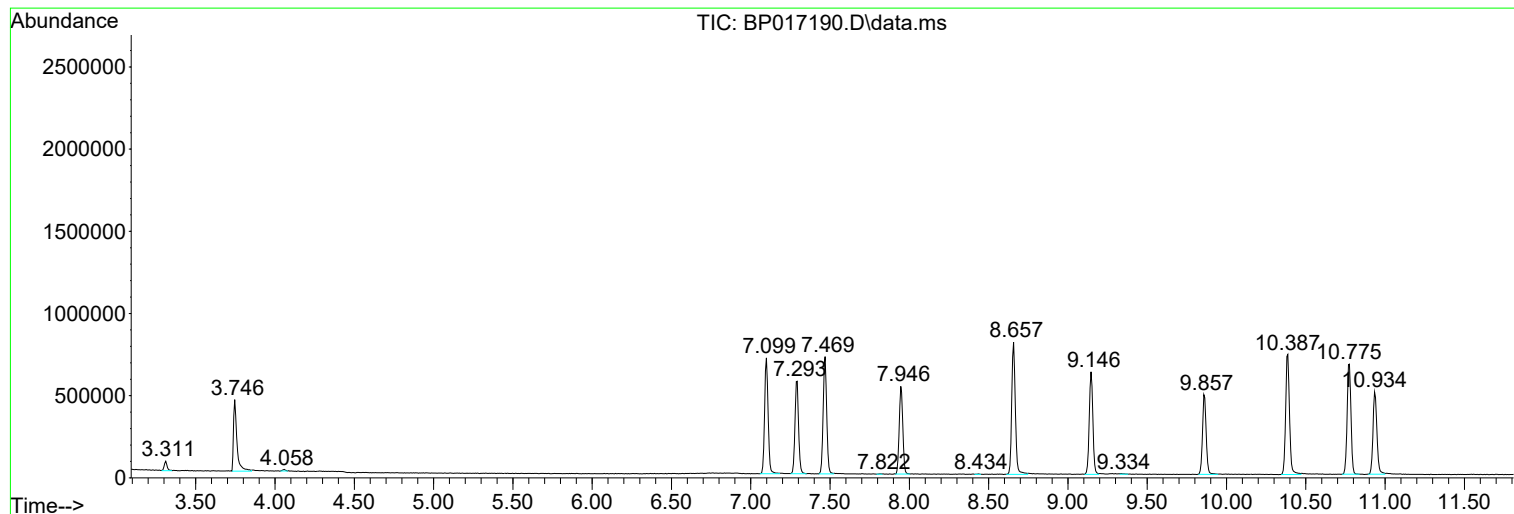

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
Data File : BP017190.D
Acq On : 15 Sep 2023 16:27
Operator : MA/JU
Sample : PB155306BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
Data File : BP017190.D
Acq On : 15 Sep 2023 16:27
Operator : MA/JU
Sample : PB155306BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------