

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
 Data File : BP017191.D
 Acq On : 15 Sep 2023 17:26
 Operator : MA/JU
 Sample : 04306-17
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH4L8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	23	29	54	rVB	2981312	4716945	100.00%	9.808%
2	3.605	85	88	91	rBV2	11640	15179	0.32%	0.032%
3	3.740	107	111	128	rBV	483482	737345	15.63%	1.533%
4	3.934	139	144	149	rVB	44501	66641	1.41%	0.139%
5	4.046	159	163	170	rVB	46202	62863	1.33%	0.131%
6	4.187	183	187	194	rVB7	16146	27189	0.58%	0.057%
7	4.505	239	241	247	rVB6	4184	5689	0.12%	0.012%
8	4.570	247	252	259	rBV	62763	92227	1.96%	0.192%
9	4.987	319	323	327	rVB	9653	13225	0.28%	0.027%
10	5.211	356	361	366	rBV2	16089	24737	0.52%	0.051%
11	5.570	418	422	429	rVB5	8815	18281	0.39%	0.038%
12	6.887	643	646	654	rVB7	9369	18389	0.39%	0.038%
13	7.087	673	680	689	rBV	597225	920312	19.51%	1.914%
14	7.187	692	697	701	rVB7	3325	6148	0.13%	0.013%
15	7.281	707	713	722	rVB	477825	730983	15.50%	1.520%
16	7.458	736	743	752	rBV	582164	905721	19.20%	1.883%
17	7.534	752	756	762	rVV	24453	41974	0.89%	0.087%
18	7.816	799	804	810	rBV	24859	35775	0.76%	0.074%
19	7.940	818	825	836	rVB	1026426	1618573	34.31%	3.365%
20	8.287	879	884	889	rVB3	14513	21586	0.46%	0.045%
21	8.646	937	945	956	rBV	692294	1140633	24.18%	2.372%
22	9.140	1020	1029	1037	rBV	509179	847277	17.96%	1.762%
23	9.258	1045	1049	1052	rVB5	3803	5362	0.11%	0.011%
24	9.852	1143	1150	1159	rBV	426039	678373	14.38%	1.411%
25	10.375	1232	1239	1249	rBV	692052	1135545	24.07%	2.361%
26	10.616	1273	1280	1287	rVV	247020	397344	8.42%	0.826%
27	10.769	1298	1306	1314	rBV	1416674	2370411	50.25%	4.929%
28	10.928	1325	1333	1345	rBV	685054	1176423	24.94%	2.446%
29	11.140	1362	1369	1377	rBV	68256	115556	2.45%	0.240%
30	11.710	1461	1466	1468	rBV6	3977	6764	0.14%	0.014%
31	11.828	1484	1486	1493	rVB8	4192	7818	0.17%	0.016%
32	12.257	1554	1559	1565	rVB7	4243	7440	0.16%	0.015%
33	12.352	1569	1575	1581	rVV2	56488	94435	2.00%	0.196%
34	12.928	1670	1673	1678	rBV7	3166	4934	0.10%	0.010%
35	13.363	1740	1747	1750	rBV8	5945	9814	0.21%	0.020%
36	13.451	1754	1762	1769	rVB	23988	41538	0.88%	0.086%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
 Data File : BP017191.D
 Acq On : 15 Sep 2023 17:26
 Operator : MA/JU
 Sample : 04306-17
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH4L8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	13.787	1815	1819	1822	rBV6	5628	9475	0.20%	0.020%
38	13.834	1822	1827	1835	rVB7	8373	19743	0.42%	0.041%
39	14.022	1853	1859	1874	rBV	1213581	1644132	34.86%	3.419%
40	14.304	1900	1907	1916	rBV	1291610	1904204	40.37%	3.959%
41	14.440	1926	1930	1932	rBV5	4477	5186	0.11%	0.011%
42	14.516	1940	1943	1946	rBV3	4343	6114	0.13%	0.013%
43	14.610	1951	1959	1967	rBV	2246072	3211565	68.09%	6.678%
44	14.722	1975	1978	1982	rVB5	4504	5263	0.11%	0.011%
45	14.828	1990	1996	2014	rBV	333808	613031	13.00%	1.275%
46	15.351	2082	2085	2089	rBV6	6054	6846	0.15%	0.014%
47	15.404	2090	2094	2100	rVB6	11915	21877	0.46%	0.045%
48	15.604	2121	2128	2139	rBV	1770620	2533421	53.71%	5.268%
49	15.734	2144	2150	2164	rVV	303565	439728	9.32%	0.914%
50	15.863	2166	2172	2182	rVB4	24438	53305	1.13%	0.111%
51	16.269	2233	2241	2244	rBV9	9106	20388	0.43%	0.042%
52	16.475	2272	2276	2282	rBV8	6604	8336	0.18%	0.017%
53	16.592	2292	2296	2301	rVB2	19828	27874	0.59%	0.058%
54	16.663	2305	2308	2313	rVV5	6377	9608	0.20%	0.020%
55	16.734	2317	2320	2324	rVV6	4222	5805	0.12%	0.012%
56	16.887	2344	2346	2350	rVB5	4744	5746	0.12%	0.012%
57	17.063	2374	2376	2381	rVB6	6150	6272	0.13%	0.013%
58	17.181	2389	2396	2397	rBV6	6799	13922	0.30%	0.029%
59	17.240	2403	2406	2410	rBV4	17649	21617	0.46%	0.045%
60	17.381	2423	2430	2441	rBV	2792534	3868720	82.02%	8.044%
61	17.481	2441	2447	2455	rBV	1897862	2612482	55.39%	5.432%
62	17.963	2526	2529	2533	rVB6	11232	15361	0.33%	0.032%
63	18.010	2533	2537	2543	rBV7	12733	20721	0.44%	0.043%
64	18.228	2569	2574	2579	rBV	167939	238913	5.06%	0.497%
65	18.422	2604	2607	2610	rVB4	16905	18063	0.38%	0.038%
66	19.363	2763	2767	2772	rBV	107488	144093	3.05%	0.300%
67	19.463	2780	2784	2789	rBV2	70534	91789	1.95%	0.191%
68	19.598	2805	2807	2812	rVB4	22086	22477	0.48%	0.047%
69	19.722	2823	2828	2836	rBV	2399734	3019980	64.02%	6.279%
70	21.169	3070	3074	3085	rVB5	86159	179056	3.80%	0.372%
71	21.486	3123	3128	3136	rBV	2891914	3593280	76.18%	7.471%
72	23.845	3524	3529	3544	rVB2	1109237	2313274	49.04%	4.810%
73	24.016	3551	3558	3572	rVB	1565108	3242623	68.74%	6.742%




Sum of corrected areas: 48093739

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
Data File : BP017191.D
Acq On : 15 Sep 2023 17:26
Operator : MA/JU
Sample : 04306-17
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH4L8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

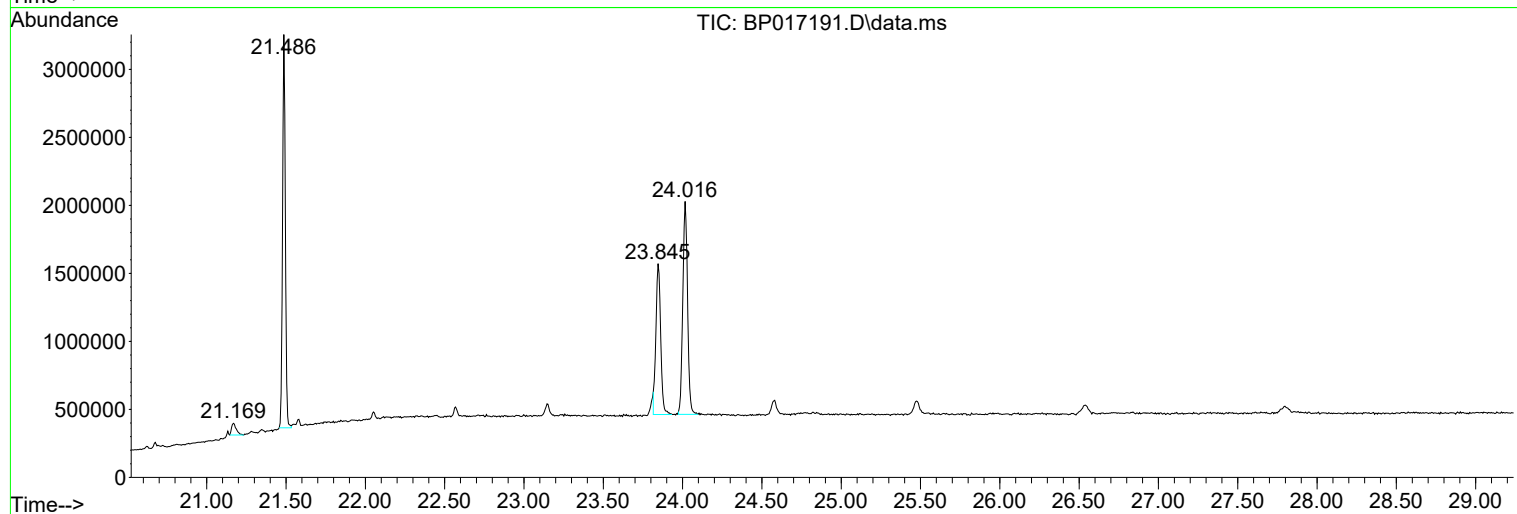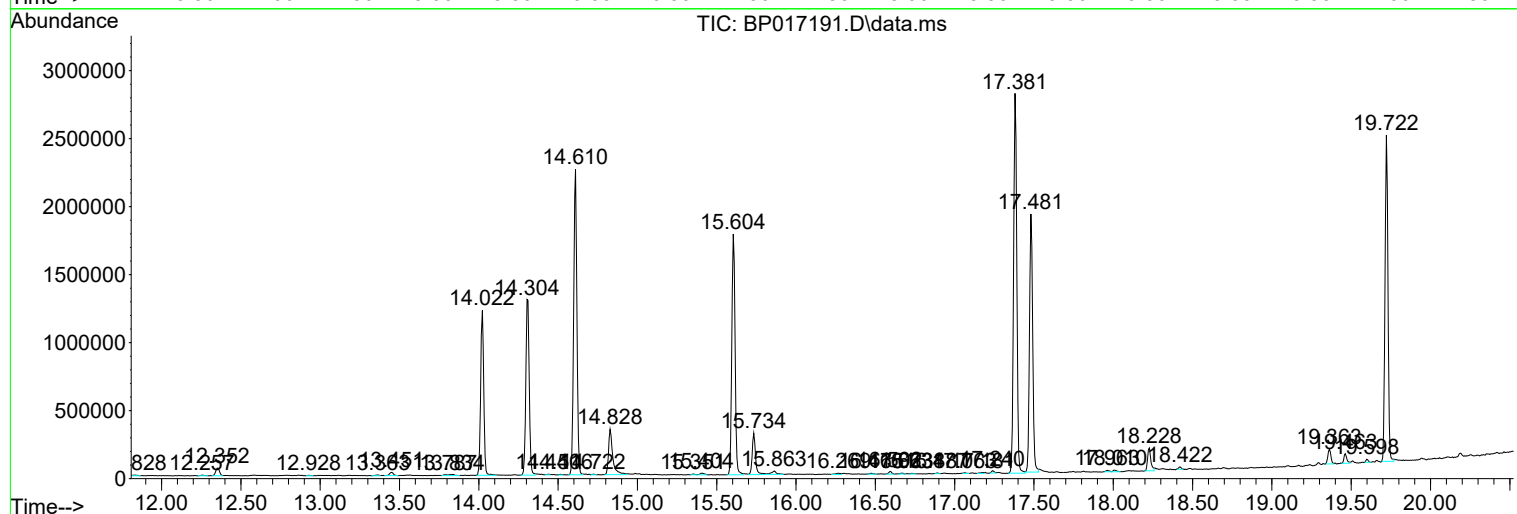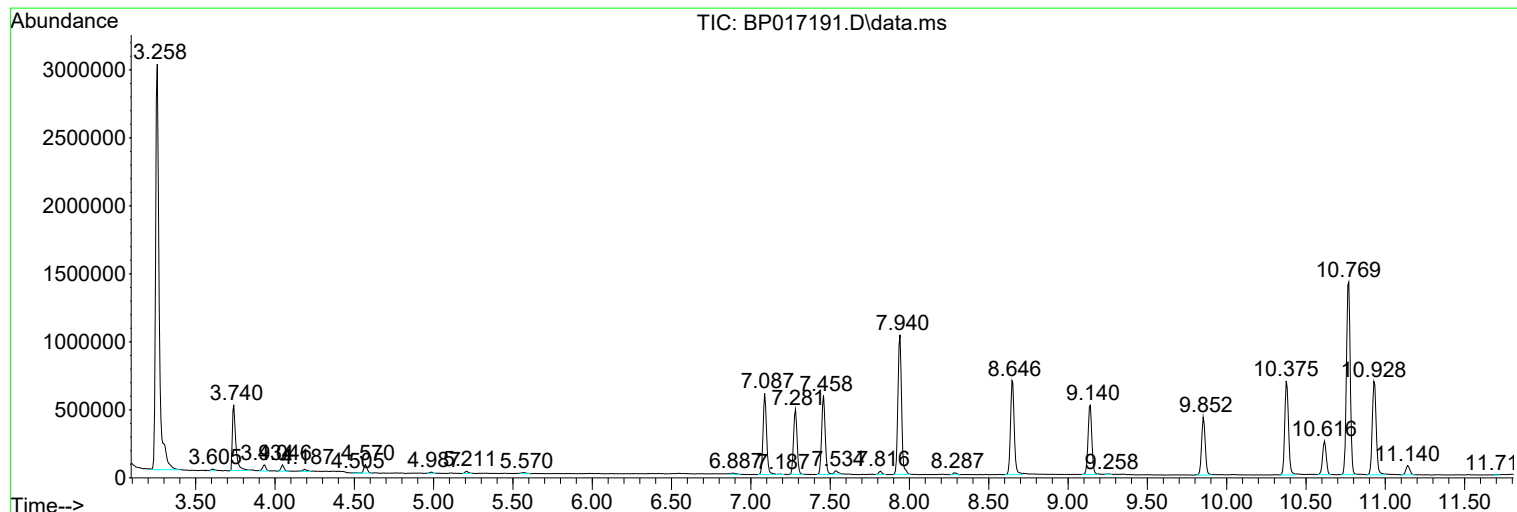

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
Data File : BP017191.D
Acq On : 15 Sep 2023 17:26
Operator : MA/JU
Sample : 04306-17
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH4L8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
Data File : BP017191.D
Acq On : 15 Sep 2023 17:26
Operator : MA/JU
Sample : 04306-17
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH4L8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------