

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
 Data File : BP017192.D
 Acq On : 15 Sep 2023 18:01
 Operator : MA/JU
 Sample : 04324-20
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	28	30	34	rVB5	10839	12045	0.26%	0.028%
2	3.311	34	38	44	rVB	46878	62241	1.32%	0.146%
3	3.746	109	112	126	rBV	252162	379386	8.04%	0.887%
4	3.940	140	145	151	rBV	39116	57206	1.21%	0.134%
5	4.052	161	164	170	rVB3	13828	20034	0.42%	0.047%
6	4.575	248	253	268	rVB	561548	828853	17.57%	1.938%
7	4.999	321	325	328	rVB3	7401	10527	0.22%	0.025%
8	5.575	418	423	425	rBV4	6900	9183	0.19%	0.021%
9	6.669	607	609	615	rBV7	3198	5318	0.11%	0.012%
10	7.093	676	681	691	rBV	166165	272946	5.78%	0.638%
11	7.287	707	714	722	rBV	721417	1096732	23.24%	2.564%
12	7.464	738	744	753	rBV	670607	1041401	22.07%	2.435%
13	7.946	819	826	837	rBV	618668	969043	20.54%	2.266%
14	8.652	940	946	958	rBV	483913	788806	16.72%	1.844%
15	9.146	1022	1030	1039	rBV	791100	1284509	27.22%	3.003%
16	9.858	1142	1151	1160	rBV	617580	984014	20.85%	2.301%
17	10.381	1232	1240	1251	rBV	893908	1466959	31.09%	3.430%
18	10.769	1298	1306	1316	rBV	836121	1343143	28.47%	3.140%
19	10.934	1325	1334	1347	rBV	857452	1473357	31.23%	3.445%
20	11.846	1486	1489	1493	rVB5	4098	6448	0.14%	0.015%
21	12.352	1569	1575	1582	rBV4	15430	27934	0.59%	0.065%
22	13.451	1756	1762	1769	rBV6	10048	18051	0.38%	0.042%
23	14.022	1852	1859	1871	rBV	1627609	2281620	48.36%	5.334%
24	14.104	1871	1873	1885	rVB	3929	10874	0.23%	0.025%
25	14.304	1900	1907	1921	rBV	1903543	2715696	57.56%	6.349%
26	14.604	1951	1958	1968	rBV	1145447	1652058	35.01%	3.862%
27	14.834	1990	1997	2010	rBV2	65449	151729	3.22%	0.355%
28	15.604	2120	2128	2141	rBV	2508877	3529440	74.80%	8.252%
29	15.728	2144	2149	2163	rVV	590392	833175	17.66%	1.948%
30	15.840	2164	2168	2172	rVB4	13231	19069	0.40%	0.045%
31	17.375	2422	2429	2439	rBV	1400298	1947465	41.27%	4.553%
32	17.475	2440	2446	2462	rVV	2628186	3758295	79.65%	8.787%
33	18.004	2532	2536	2537	rBV3	4968	5670	0.12%	0.013%
34	18.216	2568	2572	2579	rBV2	44809	68138	1.44%	0.159%
35	19.286	2751	2754	2758	rBV3	31382	42632	0.90%	0.100%
36	19.357	2763	2766	2773	rVB2	32195	47295	1.00%	0.111%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
Data File : BP017192.D
Acq On : 15 Sep 2023 18:01
Operator : MA/JU
Sample : 04324-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJA8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION

37	19.451	2779	2782	2791	rBV5	39175	69684	1.48%	0.163%
38	19.716	2822	2827	2834	rBV	3465221	4352393	92.24%	10.176%
39	21.480	3122	3127	3134	rBV	1575390	2099693	44.50%	4.909%
40	23.839	3521	3528	3545	rVB2	2288490	4718382	100.00%	11.031%
41	24.004	3549	3556	3569	rVB	1096084	2311228	48.98%	5.404%




Sum of corrected areas: 42772672

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
Data File : BP017192.D
Acq On : 15 Sep 2023 18:01
Operator : MA/JU
Sample : 04324-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

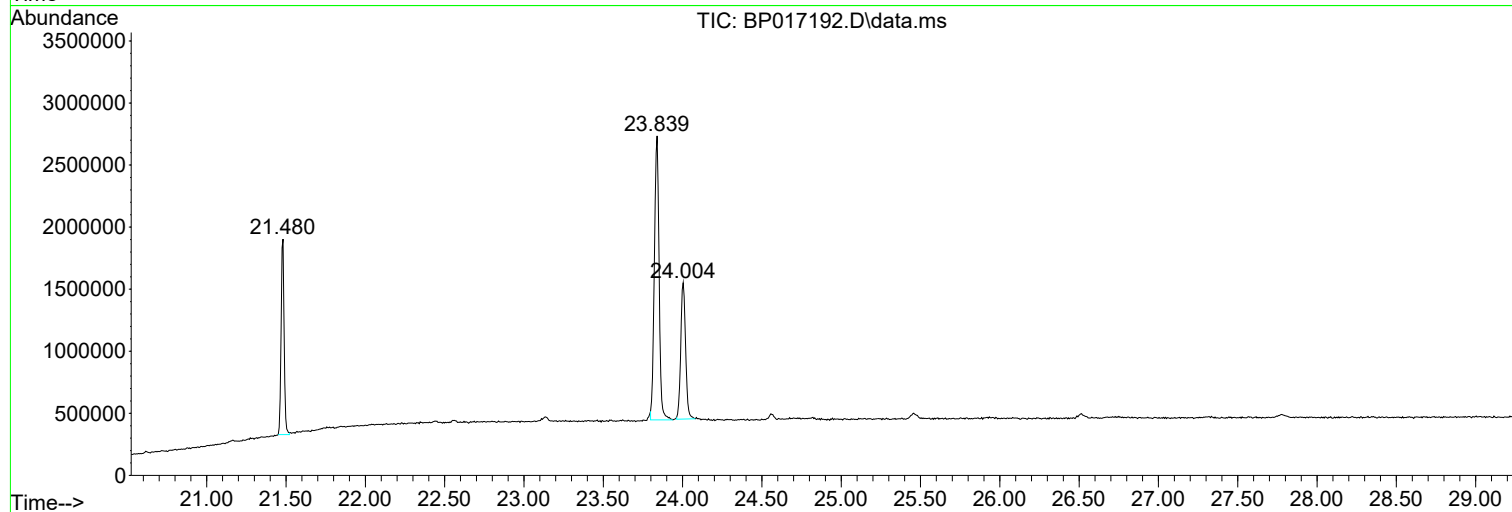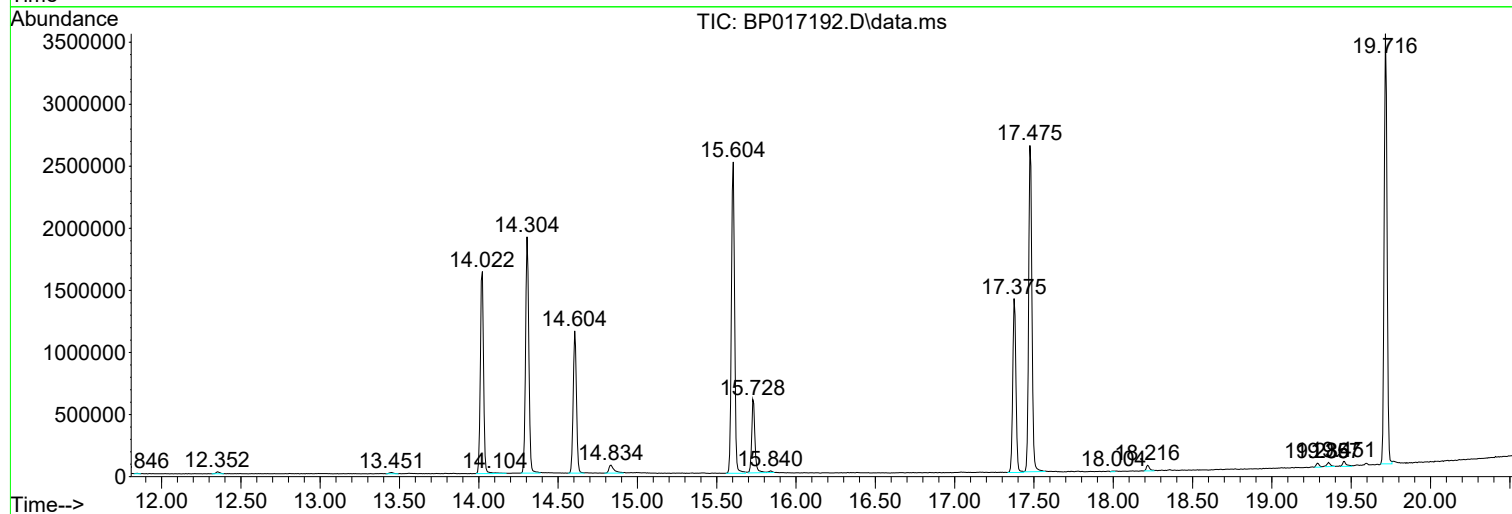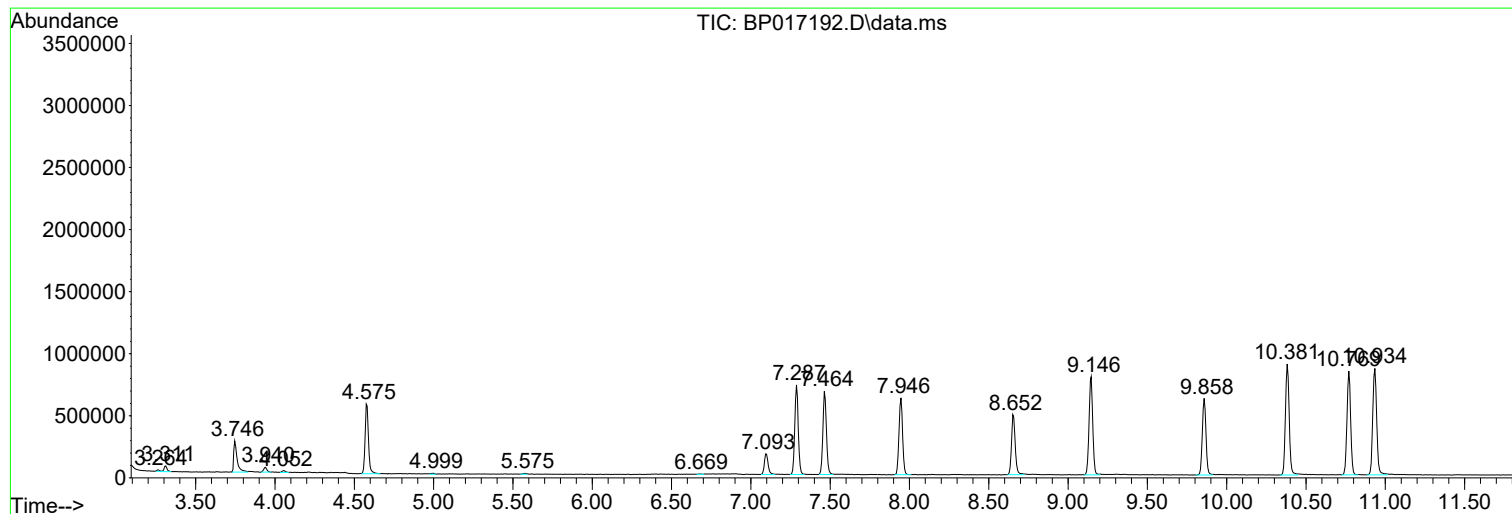

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
Data File : BP017192.D
Acq On : 15 Sep 2023 18:01
Operator : MA/JU
Sample : 04324-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJA8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.575	17.11 ng/ul	828853	1,4-Dichlorobenzene-d4	7.946

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	25

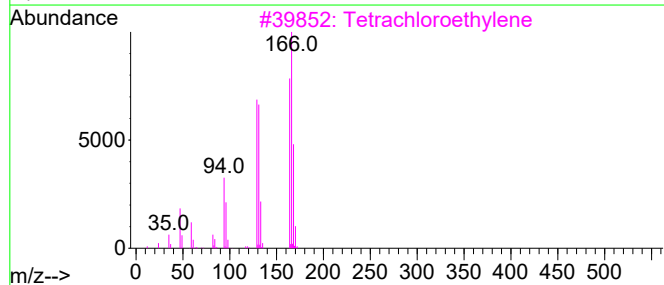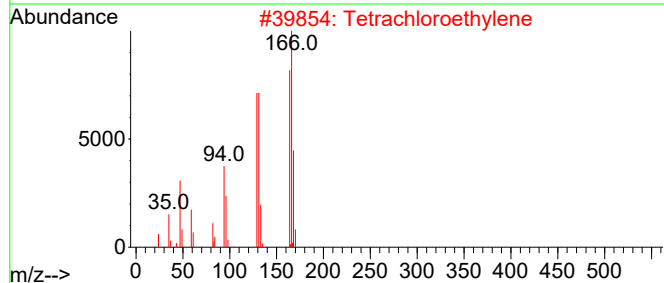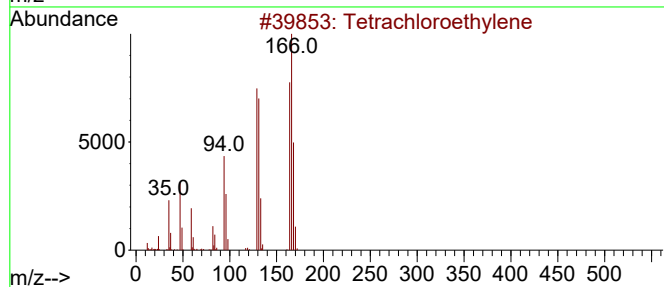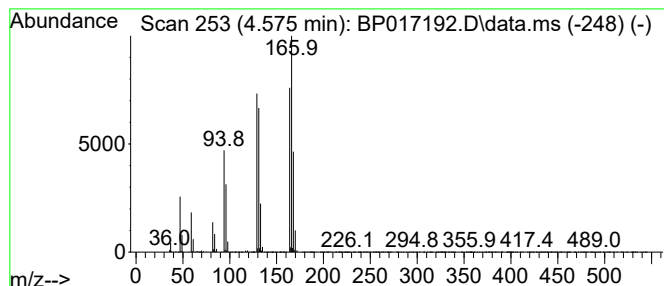

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091523\
Data File : BP017192.D
Acq On : 15 Sep 2023 18:01
Operator : MA/JU
Sample : 04324-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.575	17.1	ng/ul	828853	1	7.946	969043	20.0