

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091619\
 Data File : BP000251.D
 Acq On : 16 Sep 2019 21:12
 Operator : HP/JU
 Sample : K4871-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 VE-3-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	559	563	567	rBV	2527002	2432499	31.16%	1.132%
2	6.410	727	735	740	rVV2	1931118	2106478	26.98%	0.980%
3	6.557	753	760	763	rBV	5466822	4983877	63.84%	2.319%
4	6.787	796	799	802	rBV	2409909	1918495	24.57%	0.893%
5	6.945	822	826	829	rVB	6275706	5076121	65.02%	2.362%
6	7.345	885	894	897	rBV	4337104	4921064	63.03%	2.290%
7	7.434	905	909	913	rVB4	544866	687693	8.81%	0.320%
8	7.475	913	916	919	rBV2	616211	676738	8.67%	0.315%
9	7.563	926	931	933	rBV	1119154	1181344	15.13%	0.550%
10	7.587	933	935	941	rVB	1421657	1540286	19.73%	0.717%
11	7.722	955	958	962	rVB3	951839	1299646	16.65%	0.605%
12	7.810	967	973	976	rBV2	2278772	2525827	32.35%	1.175%
13	7.845	976	979	983	rVB2	750454	864170	11.07%	0.402%
14	7.898	983	988	993	rBV7	531376	913963	11.71%	0.425%
15	8.034	1004	1011	1013	rBV6	659996	1210207	15.50%	0.563%
16	8.069	1013	1017	1019	rBV2	3482194	3374665	43.23%	1.570%
17	8.092	1019	1021	1024	rVB	831569	803522	10.29%	0.374%
18	8.145	1028	1030	1032	rVB	1360834	860994	11.03%	0.401%
19	8.163	1032	1033	1037	rVB2	866185	697976	8.94%	0.325%
20	8.234	1041	1045	1046	rBV2	548513	602169	7.71%	0.280%
21	8.287	1051	1054	1056	rVB2	634279	558235	7.15%	0.260%
22	8.316	1056	1059	1061	rBV3	756136	798876	10.23%	0.372%
23	8.369	1067	1068	1071	rVB3	1243665	1022376	13.10%	0.476%
24	8.428	1075	1078	1080	rBV3	524952	562521	7.21%	0.262%
25	8.463	1080	1084	1087	rVB2	1747236	1850104	23.70%	0.861%
26	8.504	1088	1091	1093	rBV	2212436	2008957	25.73%	0.935%
27	8.545	1096	1098	1100	rVB	1871501	1407798	18.03%	0.655%
28	8.581	1101	1104	1107	rBV2	1018397	984616	12.61%	0.458%
29	8.663	1116	1118	1121	rBV4	909522	895599	11.47%	0.417%
30	8.734	1128	1130	1132	rVB3	755379	600899	7.70%	0.280%
31	8.769	1133	1136	1139	rVB3	1384300	1317711	16.88%	0.613%
32	8.828	1144	1146	1148	rBV2	674349	669251	8.57%	0.311%
33	8.904	1156	1159	1163	rBV4	452461	685282	8.78%	0.319%
34	8.986	1171	1173	1177	rVB4	1002137	1055196	13.52%	0.491%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091619\
 Data File : BP000251.D
 Acq On : 16 Sep 2019 21:12
 Operator : HP/JU
 Sample : K4871-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 VE-3-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	9.022	1177	1179	1181	rBV2	776582	652054	8.35%	0.303%
36	9.051	1181	1184	1186	rBV3	696452	725969	9.30%	0.338%
37	9.110	1191	1194	1197	rVB2	2871952	2477191	31.73%	1.153%
38	9.151	1197	1201	1203	rBV	8180487	7184635	92.03%	3.343%
39	9.239	1212	1216	1220	rBV5	1207056	2403065	30.78%	1.118%
40	9.416	1240	1246	1253	rBV	4658269	7807161	100.00%	3.633%
41	9.492	1255	1259	1262	rVV	5980246	6740885	86.34%	3.137%
42	9.522	1262	1264	1266	rVB	4916156	3510024	44.96%	1.633%
43	9.545	1266	1268	1270	rBV	2013833	1854823	23.76%	0.863%
44	9.569	1270	1272	1274	rVB	2747316	2115261	27.09%	0.984%
45	9.610	1276	1279	1281	rBV	2300355	2167017	27.76%	1.008%
46	9.751	1298	1303	1305	rBV3	1225233	1682344	21.55%	0.783%
47	9.834	1312	1317	1320	rBV4	3705075	4736183	60.66%	2.204%
48	9.939	1332	1335	1340	rVB	2815000	4454094	57.05%	2.072%
49	9.986	1340	1343	1348	rBV3	1153396	1698462	21.76%	0.790%
50	10.039	1349	1352	1356	rVB	4186910	4211134	53.94%	1.959%
51	10.081	1356	1359	1361	rBV	3887377	3081658	39.47%	1.434%
52	10.104	1361	1363	1368	rVB5	1045842	1349182	17.28%	0.628%
53	10.157	1369	1372	1375	rBV	3859127	3683389	47.18%	1.714%
54	10.186	1375	1377	1379	rVB	3020350	2093919	26.82%	0.974%
55	10.210	1379	1381	1384	rBV4	1088179	1164945	14.92%	0.542%
56	10.251	1384	1388	1389	rBV2	1564939	1903514	24.38%	0.886%
57	10.333	1400	1402	1405	rVB2	1129831	1109288	14.21%	0.516%
58	10.363	1405	1407	1409	rVV	2205615	1909022	24.45%	0.888%
59	10.416	1413	1416	1419	rVV2	1825969	2680582	34.33%	1.247%
60	10.457	1420	1423	1425	rVV2	3945022	4539171	58.14%	2.112%
61	10.504	1428	1431	1434	rVV	3701556	3798356	48.65%	1.767%
62	10.539	1434	1437	1443	rVB4	1676689	3062734	39.23%	1.425%
63	10.592	1443	1446	1448	rBV3	1371752	1905297	24.40%	0.887%
64	10.633	1450	1453	1456	rVV2	4480938	4457946	57.10%	2.074%
65	10.669	1456	1459	1464	rVB4	1469456	1989785	25.49%	0.926%
66	10.769	1471	1476	1479	rBV2	3469703	5374703	68.84%	2.501%
67	10.798	1479	1481	1484	rVB2	872835	859679	11.01%	0.400%
68	10.833	1485	1487	1489	rBV2	1078242	884170	11.33%	0.411%
69	10.857	1489	1491	1496	rVB4	1420442	1815303	23.25%	0.845%
70	10.975	1508	1511	1513	rBV	2525541	2649040	33.93%	1.233%
71	11.133	1536	1538	1541	rBV3	887010	858658	11.00%	0.400%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091619\
 Data File : BP000251.D
 Acq On : 16 Sep 2019 21:12
 Operator : HP/JU
 Sample : K4871-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 VE-3-1

Integration Parameters: rteint.p

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	11.239	1552	1556	1559	rBV4	2494120	2955045	37.85%	1.375%
73	11.304	1564	1567	1569	rBV2	1244169	1351386	17.31%	0.629%
74	11.333	1569	1572	1574	rVB	2234715	1689824	21.64%	0.786%
75	11.357	1574	1576	1577	rBV	1071049	839610	10.75%	0.391%
76	11.451	1588	1592	1598	rBV4	3749512	5467484	70.03%	2.544%
77	11.592	1614	1616	1619	rVB3	1201736	1082100	13.86%	0.503%
78	11.663	1625	1628	1631	rVB3	1341568	1426904	18.28%	0.664%
79	11.751	1639	1643	1648	rBV3	1405595	2199872	28.18%	1.024%
80	11.798	1648	1651	1653	rBV	1208967	1582416	20.27%	0.736%
81	11.839	1656	1658	1661	rVB2	1713308	1480926	18.97%	0.689%
82	11.869	1661	1663	1665	rVB	2184022	1406429	18.01%	0.654%
83	11.898	1665	1668	1669	rBV	2250888	2252115	28.85%	1.048%
84	11.945	1674	1676	1679	rVV2	2105231	2274140	29.13%	1.058%
85	11.975	1679	1681	1684	rVB	969804	675827	8.66%	0.314%
86	12.039	1689	1692	1695	rVB2	972481	1198167	15.35%	0.558%
87	12.110	1702	1704	1707	rVB3	1206449	942447	12.07%	0.439%
88	12.292	1732	1735	1737	rVB2	879311	800156	10.25%	0.372%
89	12.322	1738	1740	1748	rVB2	1601890	3060008	39.19%	1.424%
90	12.398	1750	1753	1756	rVB	2730207	2483051	31.80%	1.155%
91	12.522	1771	1774	1778	rVB3	1108866	1090567	13.97%	0.507%
92	12.680	1797	1801	1805	rVB2	3009283	2913394	37.32%	1.356%
93	12.810	1821	1823	1827	rVB2	831125	806189	10.33%	0.375%
94	12.845	1827	1829	1836	rVB2	1036461	1258808	16.12%	0.586%
95	12.933	1840	1844	1847	rBV	8222740	7491582	95.96%	3.486%
96	13.845	1997	1999	2006	rVB	849470	926755	11.87%	0.431%
97	13.992	2021	2024	2028	rBV	2731031	2685445	34.40%	1.250%
98	15.139	2216	2219	2223	rVB	519765	553832	7.09%	0.258%
99	15.474	2272	2276	2280	rVV	2071209	2569424	32.91%	1.196%
100	15.527	2282	2285	2293	rVB	551563	767697	9.83%	0.357%


Sum of corrected areas: 214917398

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091619\
Data File : BP000251.D
Acq On : 16 Sep 2019 21:12
Operator : HP/JU
Sample : K4871-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
VE-3-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

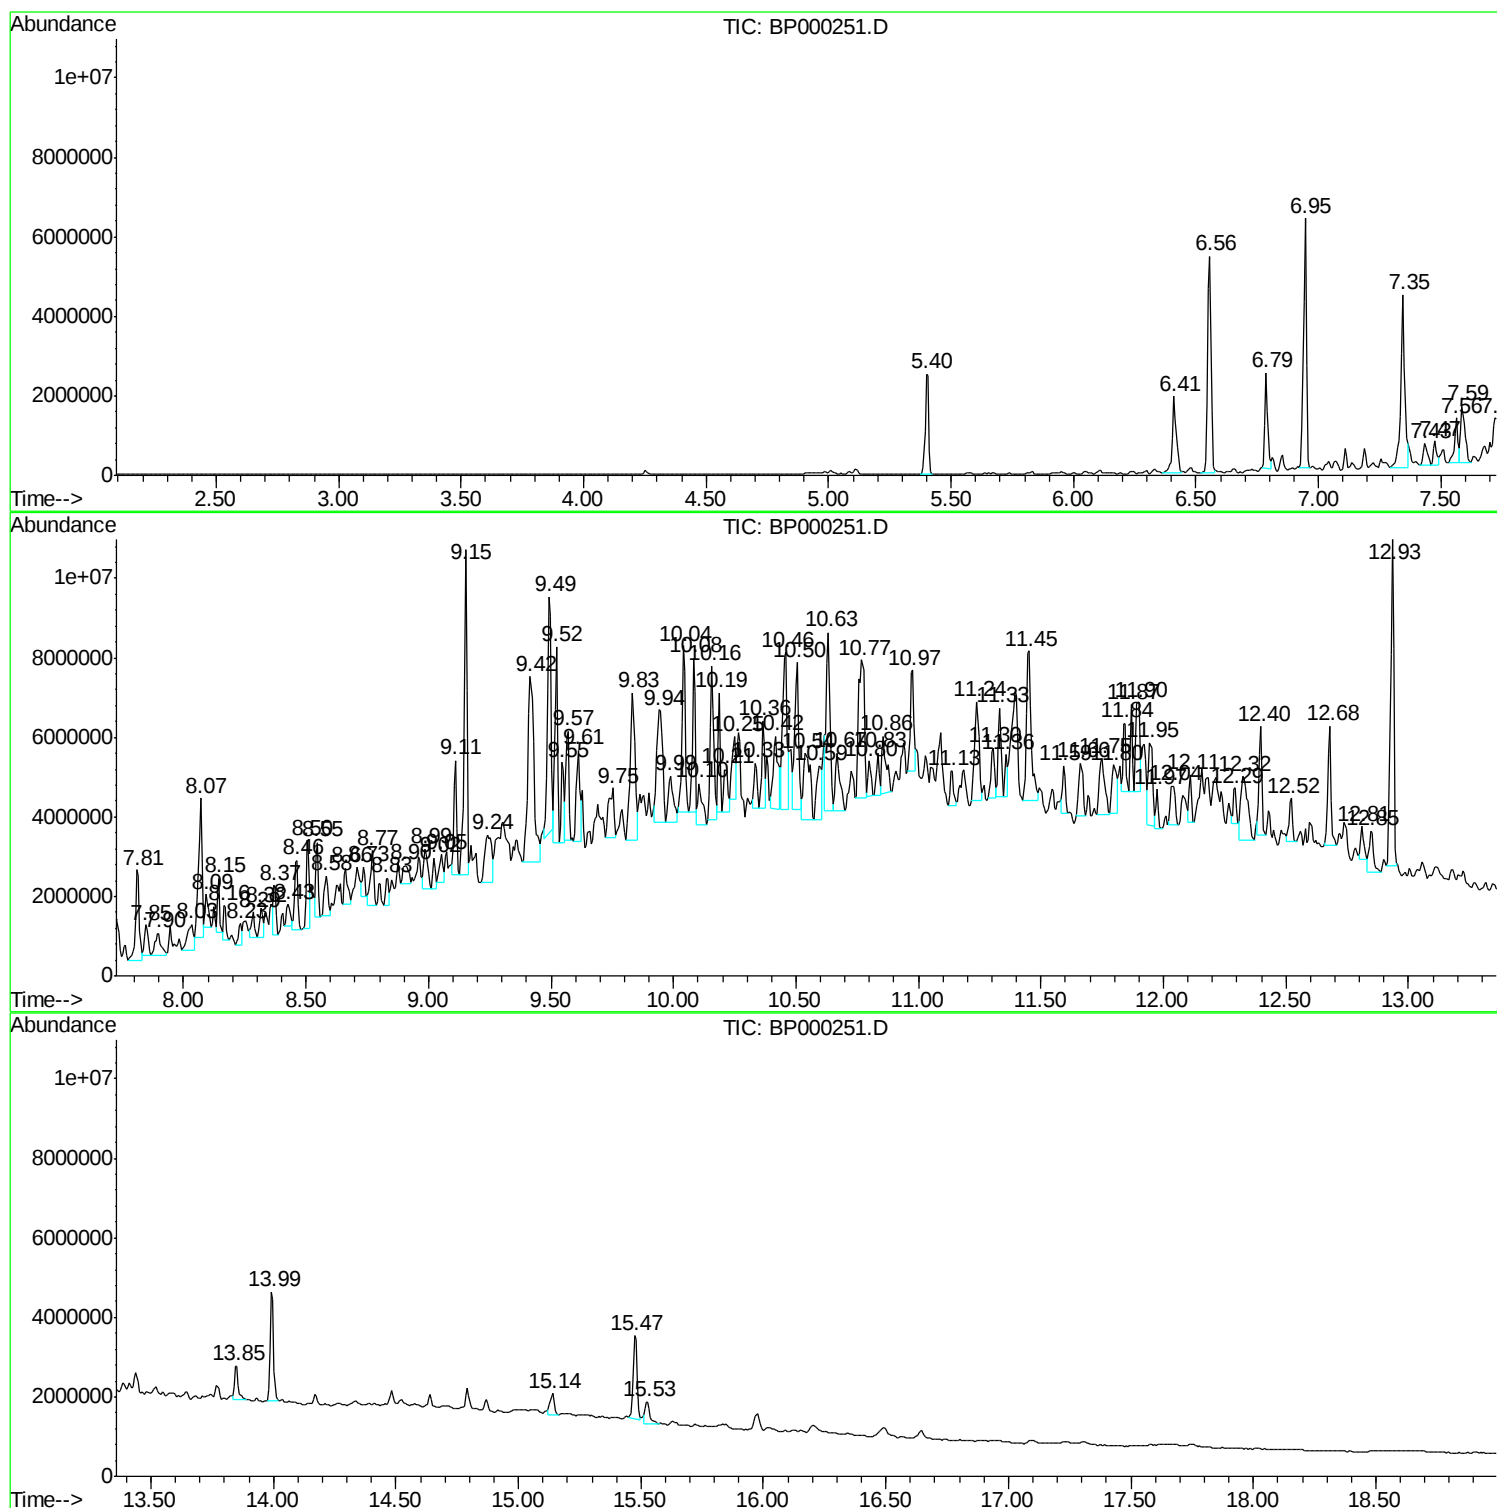

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091619\
Data_File : BP000251.D
Acq_On : 16-Sep-2019 21:122
Operator : HP/JUU
Sample : K4871-088
Misc :
ALS_Vial : 13 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
VE-3-1

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
