

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091619\
 Data File : BP000255.D
 Acq On : 16 Sep 2019 22:49
 Operator : HP/JU
 Sample : K4886-03 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-13-S(1.5-4)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.405	560	564	567	rBV	2733070	2321528	65.23%	6.283%
2	6.416	732	736	745	rBV	3038891	2527182	71.01%	6.840%
3	6.558	756	760	763	rBV	3032821	2599181	73.04%	7.035%
4	6.787	796	799	803	rBV	2378207	1828899	51.39%	4.950%
5	6.946	822	826	829	rBV	2555251	2045537	57.48%	5.536%
6	7.340	890	893	897	rBV	1661388	1456433	40.93%	3.942%
7	8.069	1014	1017	1020	rBV	3103839	2364262	66.43%	6.399%
8	9.146	1197	1200	1203	rBV	3996550	3018946	84.83%	8.171%
9	9.540	1264	1267	1271	rBV	245211	190560	5.35%	0.516%
10	9.687	1288	1292	1296	rBV	63861	65596	1.84%	0.178%
11	9.828	1313	1316	1320	rBV	3580201	2873901	80.76%	7.778%
12	10.616	1446	1450	1454	rBV	2442781	2036379	57.22%	5.512%
13	11.322	1566	1570	1573	rBV	3653518	2962710	83.25%	8.019%
14	11.346	1573	1574	1577	rVV	196675	105172	2.96%	0.285%
15	11.393	1580	1582	1585	rVB	59542	53953	1.52%	0.146%
16	11.857	1658	1661	1665	rBV	188433	163718	4.60%	0.443%
17	11.940	1672	1675	1678	rBV	59370	67570	1.90%	0.183%
18	12.546	1774	1778	1781	rBV	565562	492451	13.84%	1.333%
19	12.775	1812	1817	1820	rBV	490857	480231	13.49%	1.300%
20	12.922	1838	1842	1845	rBV	3756682	2936324	82.51%	7.947%
21	13.840	1996	1998	2004	rVB	302104	309187	8.69%	0.837%
22	13.987	2019	2023	2026	rBV	3429201	3558772	100.00%	9.632%
23	15.469	2271	2275	2279	rVB	2161511	2488673	69.93%	6.736%


Sum of corrected areas: 36947165

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091619\
Data File : BP000255.D
Acq On : 16 Sep 2019 22:49
Operator : HP/JU
Sample : K4886-03 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
TP-13-S(1.5-4)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

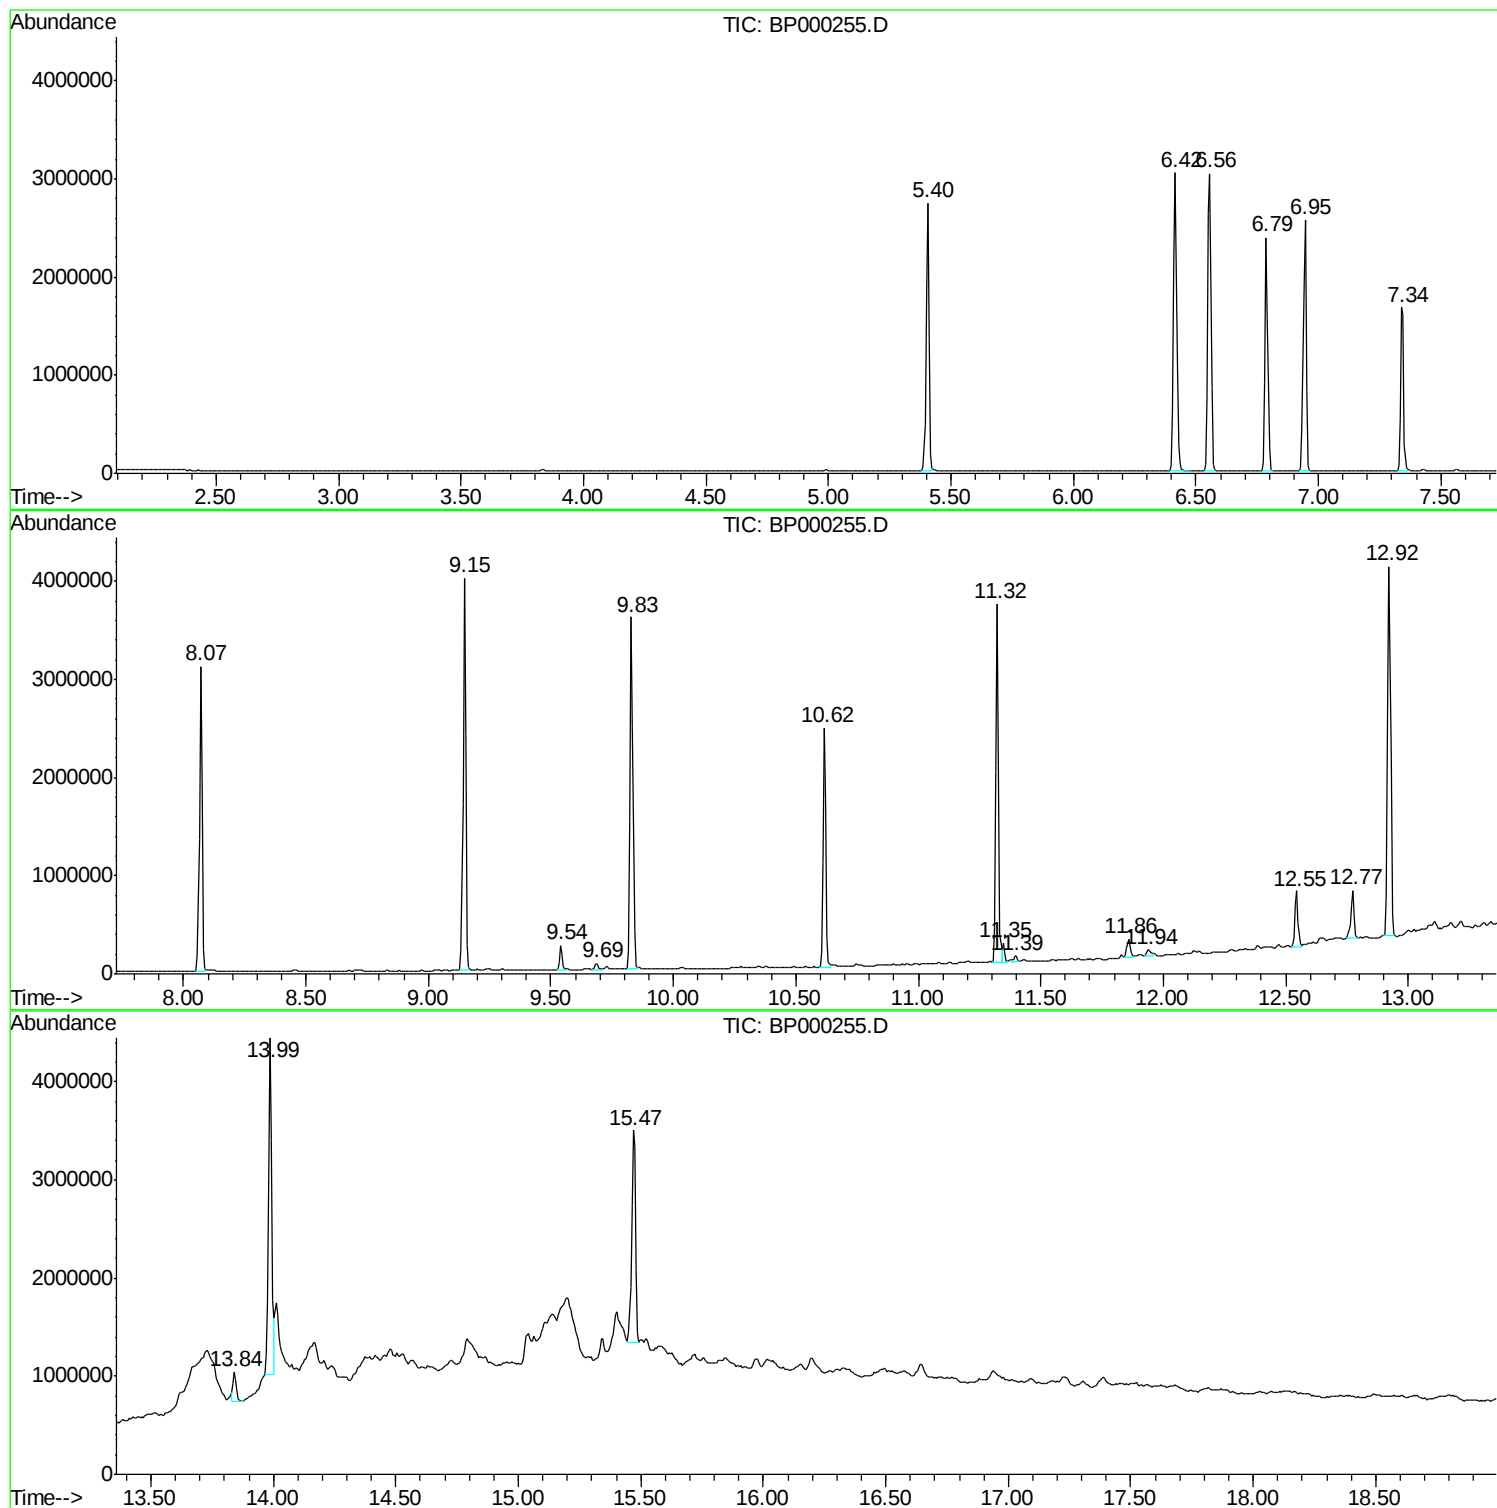

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091619\
Data File : BP000255.D
Acq On : 16 Sep 2019 22:49
Operator : HP/JU
Sample : K4886-03 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-13-S(1.5-4)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.56 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.56	28.42 ng	2599180	1,4-Dichlorobenzene-d4	6.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	16
3		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
4		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

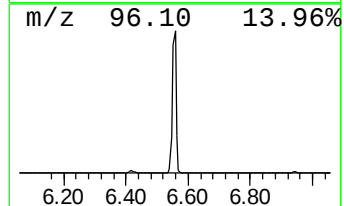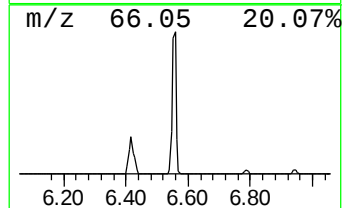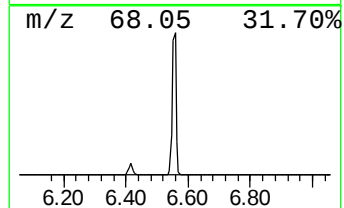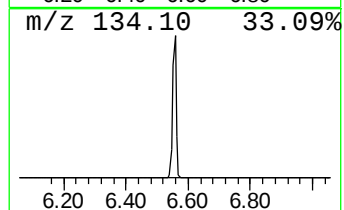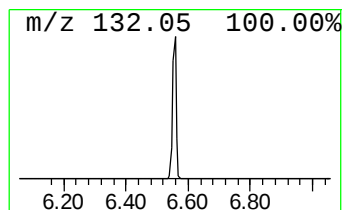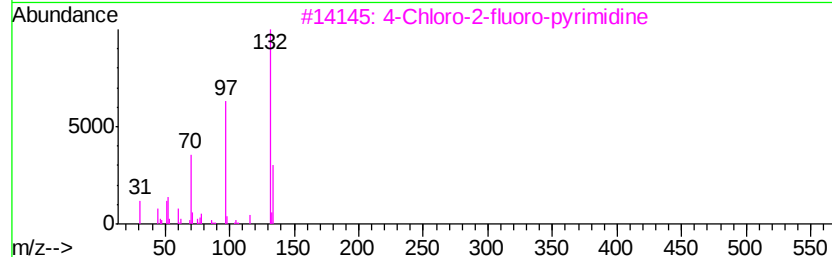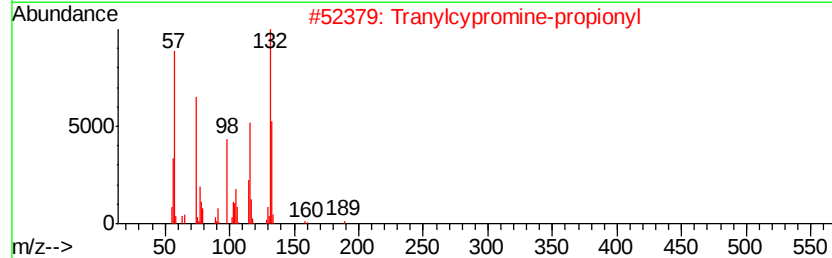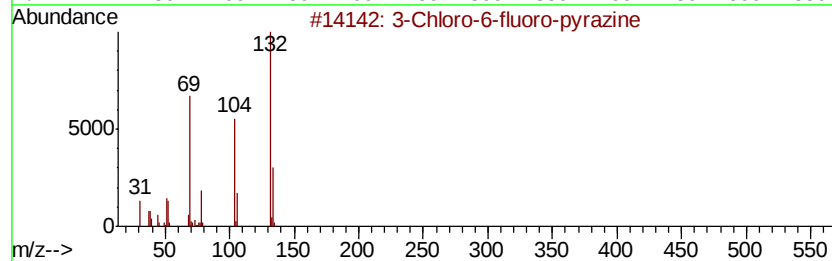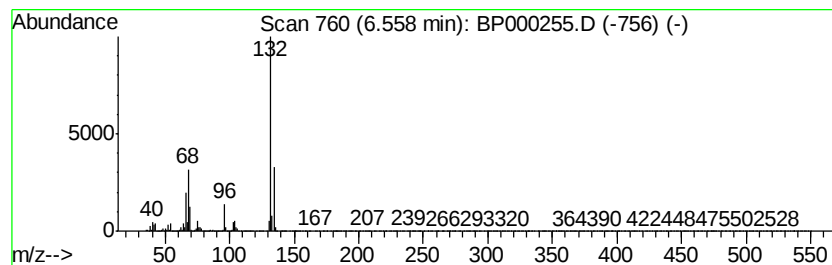

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091619\
Data File : BP000255.D
Acq On : 16 Sep 2019 22:49
Operator : HP/JU
Sample : K4886-03 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-13-S(1.5-4)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.56	6.56	28.4	ng	2599180	1	6.79	1828900	20.0