
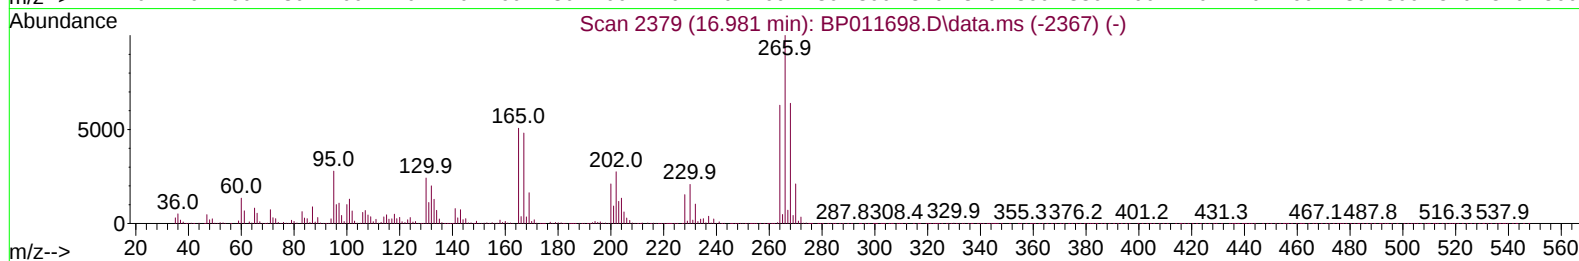
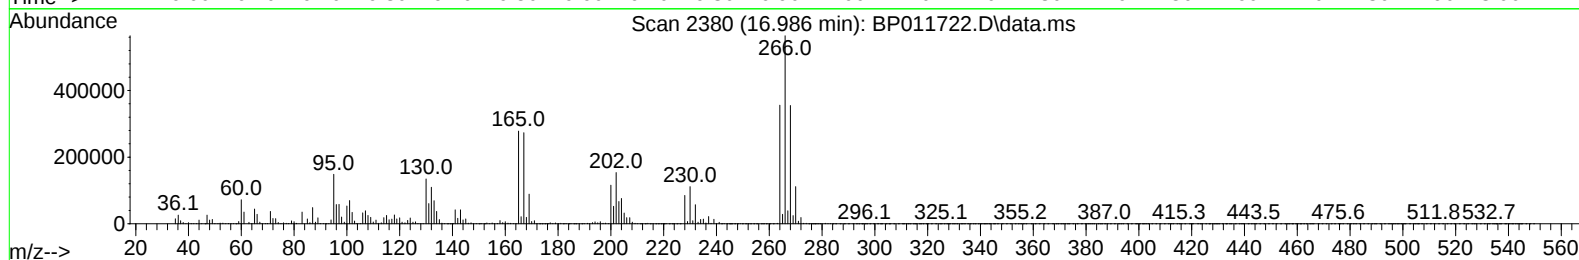


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP091622\  
Data File : BP011722.D  
Acq On : 16 Sep 2022 09:10  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 15:30:53 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP091422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 14 19:12:50 2022  
Response via : Initial Calibration

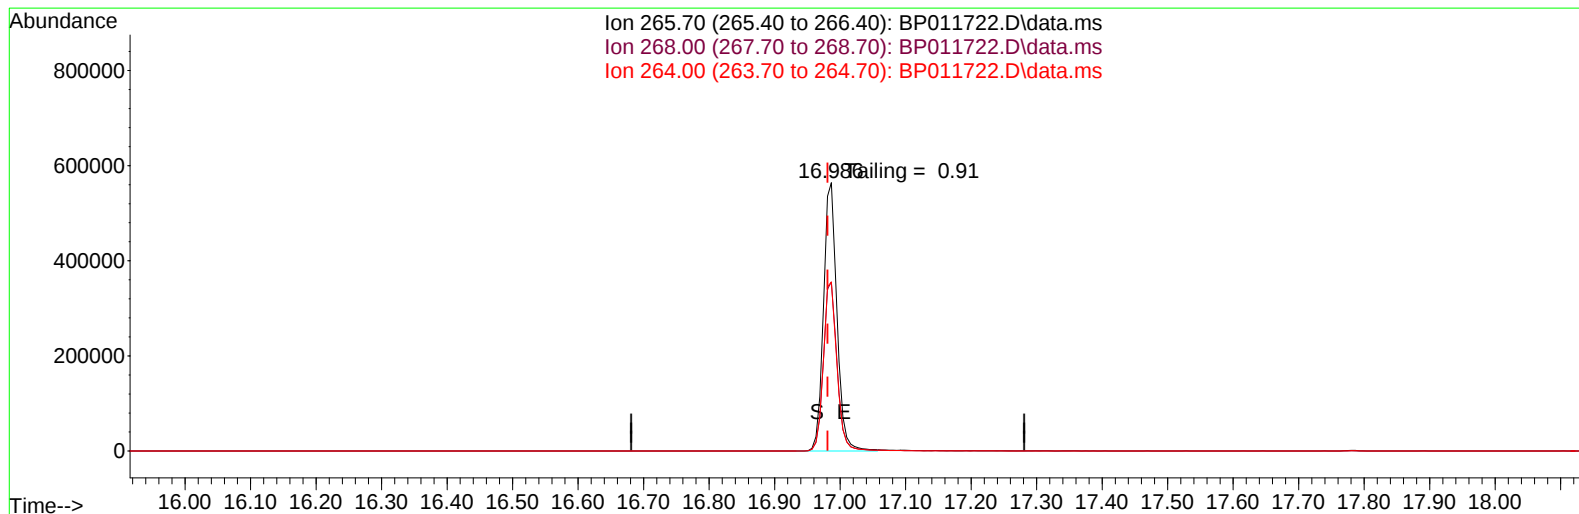

TIC: BP011722.D\data.ms

**(70) Pentachlorophenol (C)**




**16.986min (+ 0.005) 87277.44 ng**

**response 813323**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.10  | 62.89  |
| 264.00 | 63.00  | 63.03  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP091622\  
Data File : BP011722.D  
Acq On : 16 Sep 2022 09:10  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 15:30:53 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP091422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 14 19:12:50 2022  
Response via : Initial Calibration

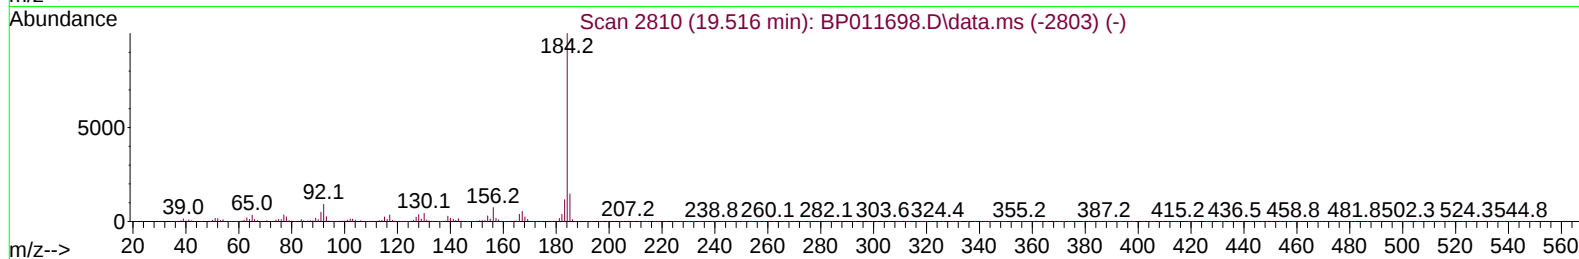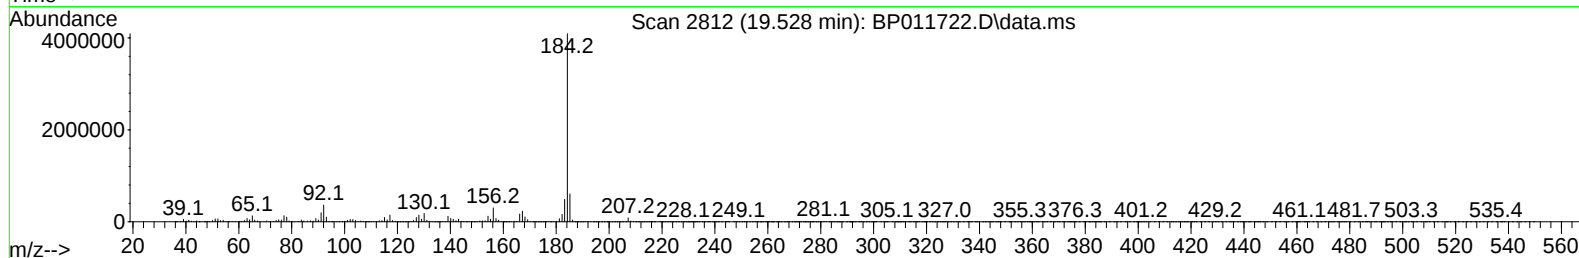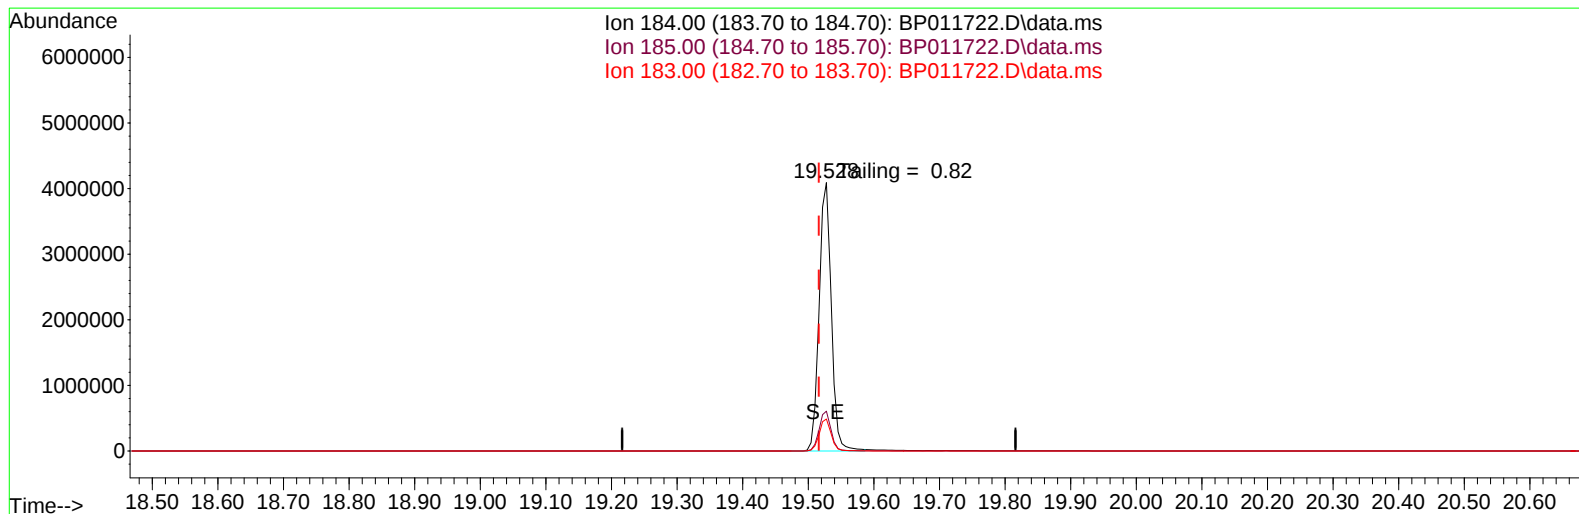

TIC: BP011722.D\data.ms

**(77) Benzidine****19.528min (+ 0.012) 4893.70 ng****response 5354792**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.40  | 14.83  |
| 183.00 | 11.30  | 11.92  |
| 0.00   | 0.00   | 0.00   |