
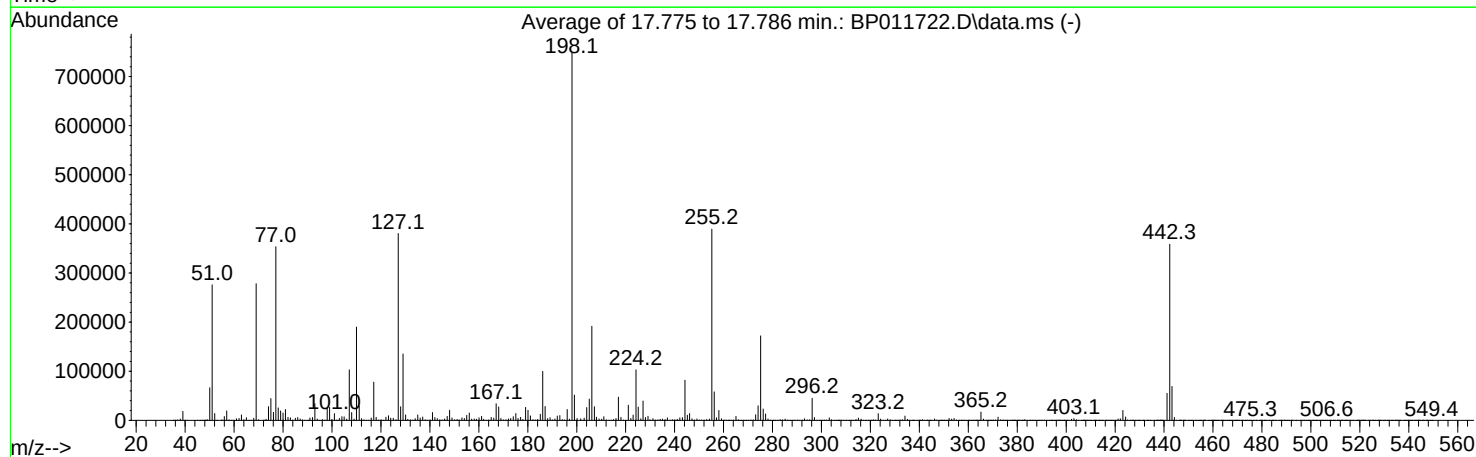


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091622\
 Data File : BP011722.D
 Acq On : 16 Sep 2022 09:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 14 19:12:50 2022

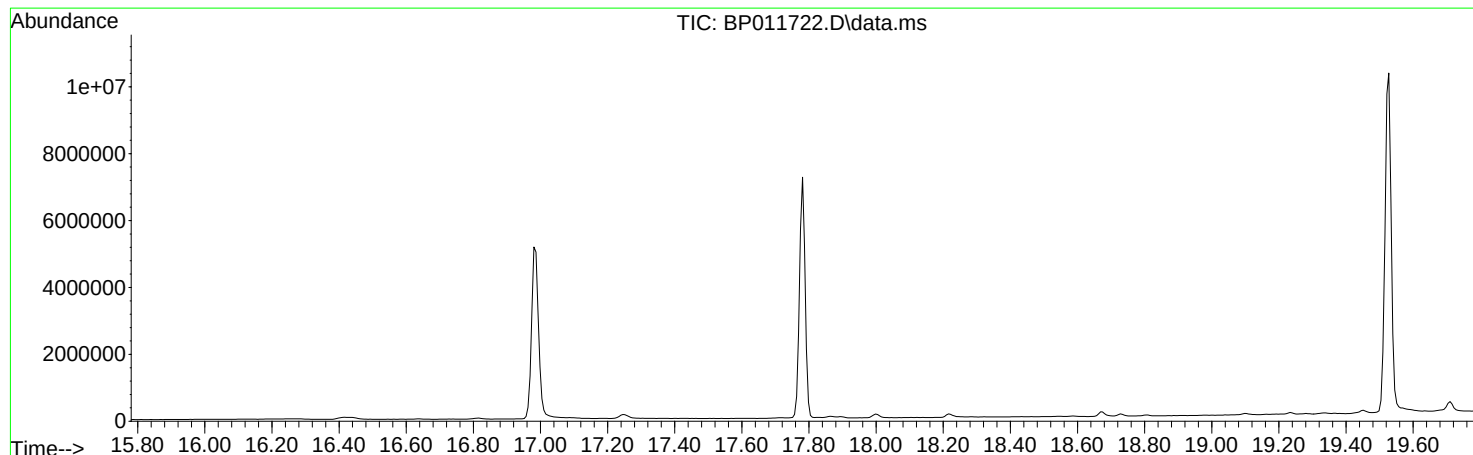

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	276034	PASS
68	69	0.00	2	1.5	4146	PASS
69	198	0.00	100	37.2	278329	PASS
70	69	0.00	2	0.4	1176	PASS
127	198	10	80	50.8	380355	PASS
197	198	0.00	2	0.4	2712	PASS
198	198	100	100	100.0	748915	PASS
199	198	5	9	6.9	51536	PASS
275	198	10	60	23.0	172106	PASS
365	198	1	100	2.3	17106	PASS
441	198	0.01	100	7.3	54925	PASS
442	442	100	100	100.0	358507	PASS
443	442	15	24	19.3	69221	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/16/2022	BNA_P	<u>BP011722.D</u>
Compound Name	Response	Retention Time
DDT	2331708	20.72
DDD	12923	20.29
DDE	1790	19.8
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14713	2346421	0.63

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091622\
Data File : BP011722.D
Acq On : 16 Sep 2022 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 16 15:30:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 19:12:50 2022
Response via : Initial Calibration

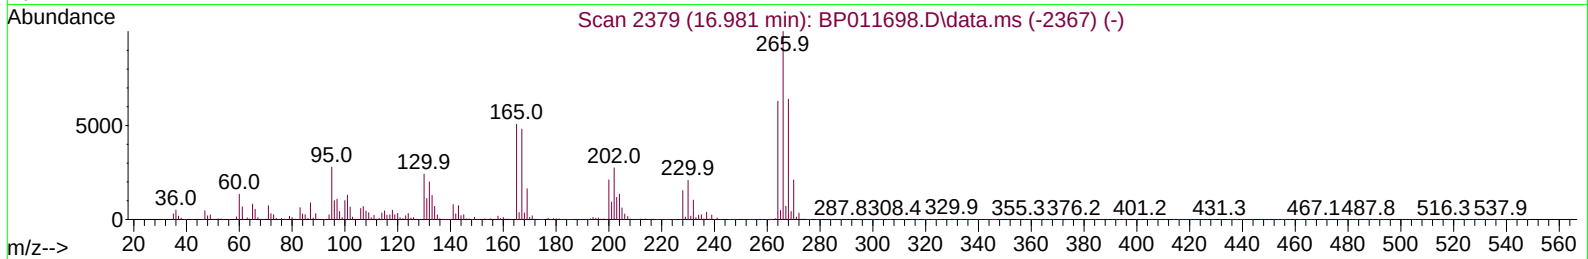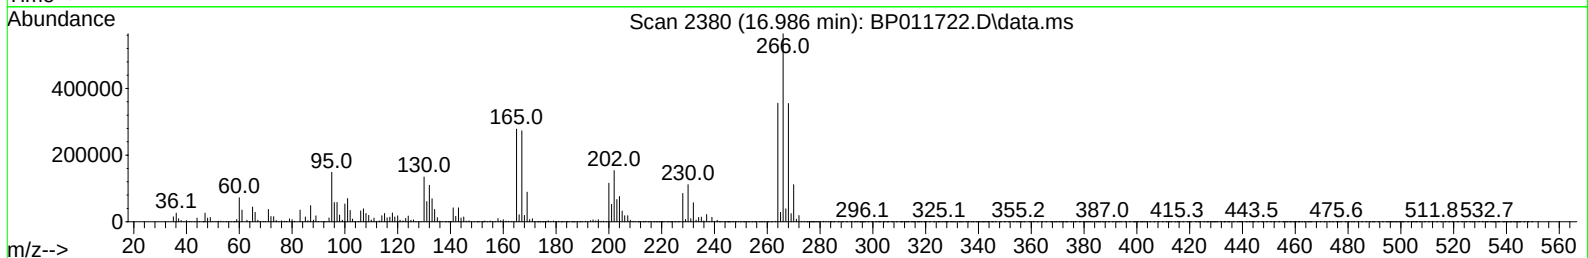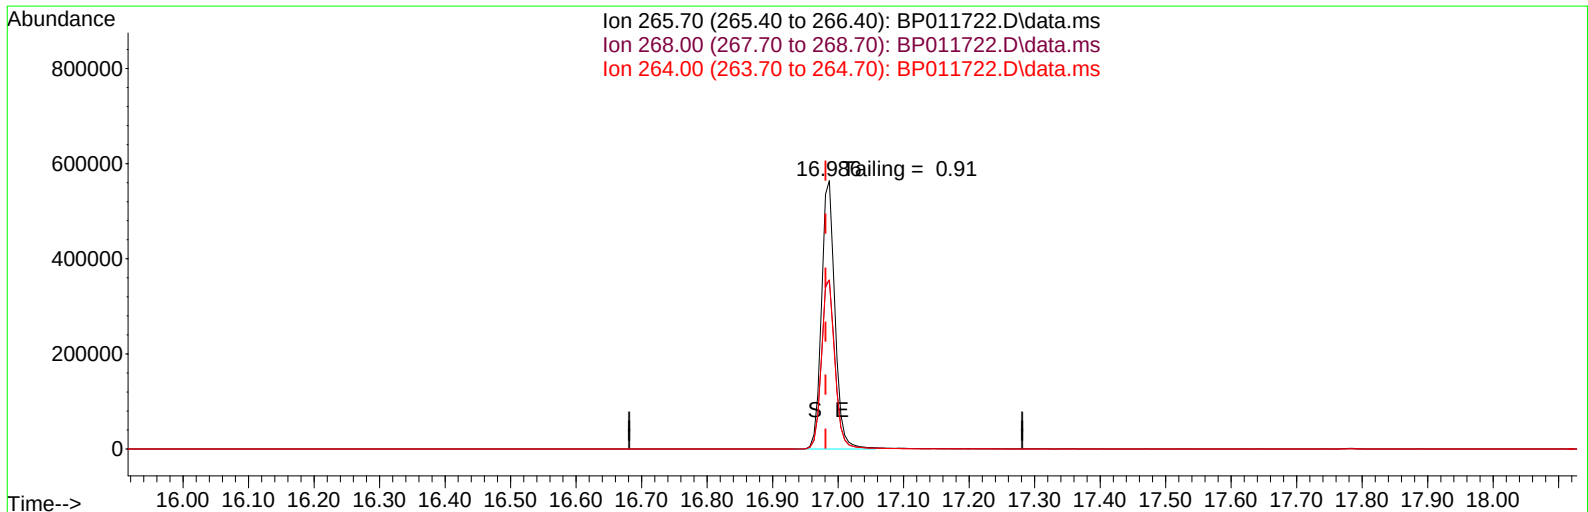

TIC: BP011722.D\data.ms

(70) Pentachlorophenol (C)

16.986min (+ 0.005) 87277.44 ng




response 813323

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.89
264.00	63.00	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091622\
Data File : BP011722.D
Acq On : 16 Sep 2022 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 16 15:30:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 19:12:50 2022
Response via : Initial Calibration

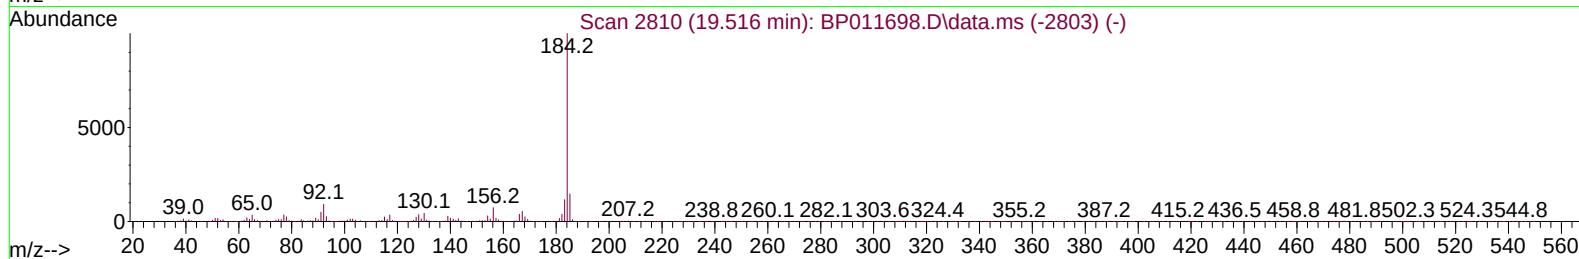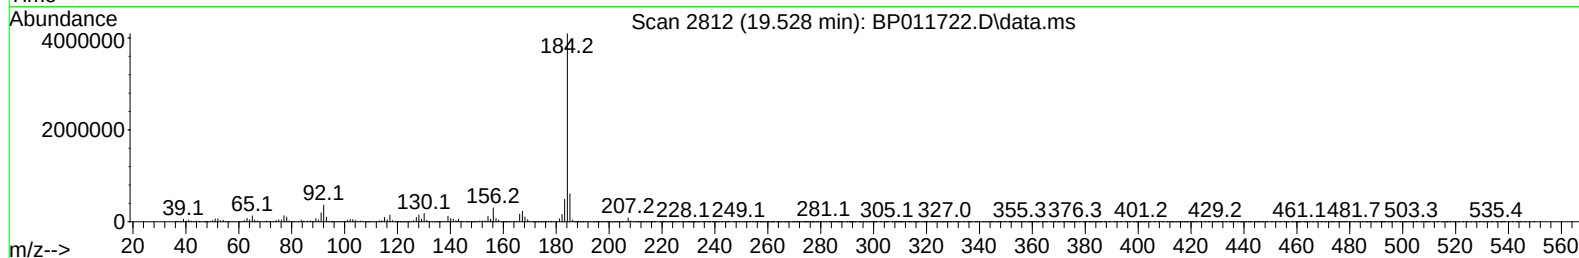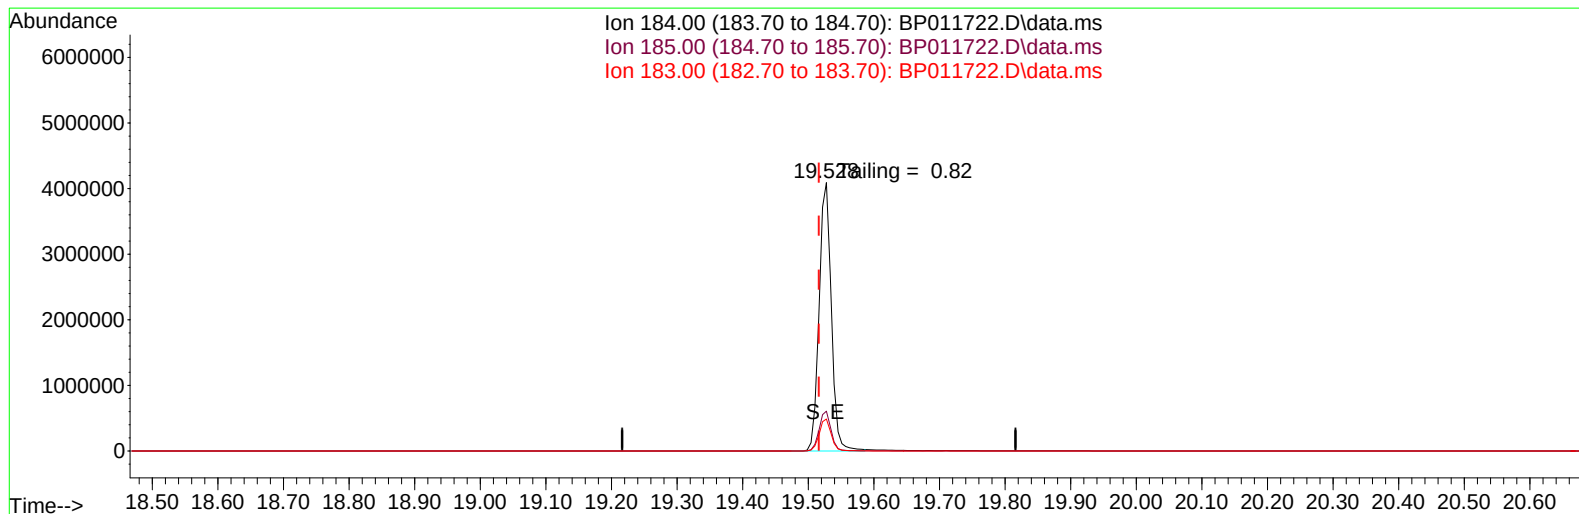

TIC: BP011722.D\data.ms

(77) Benzidine

19.528min (+ 0.012) 4893.70 ng

response 5354792

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.83
183.00	11.30	11.92
0.00	0.00	0.00