
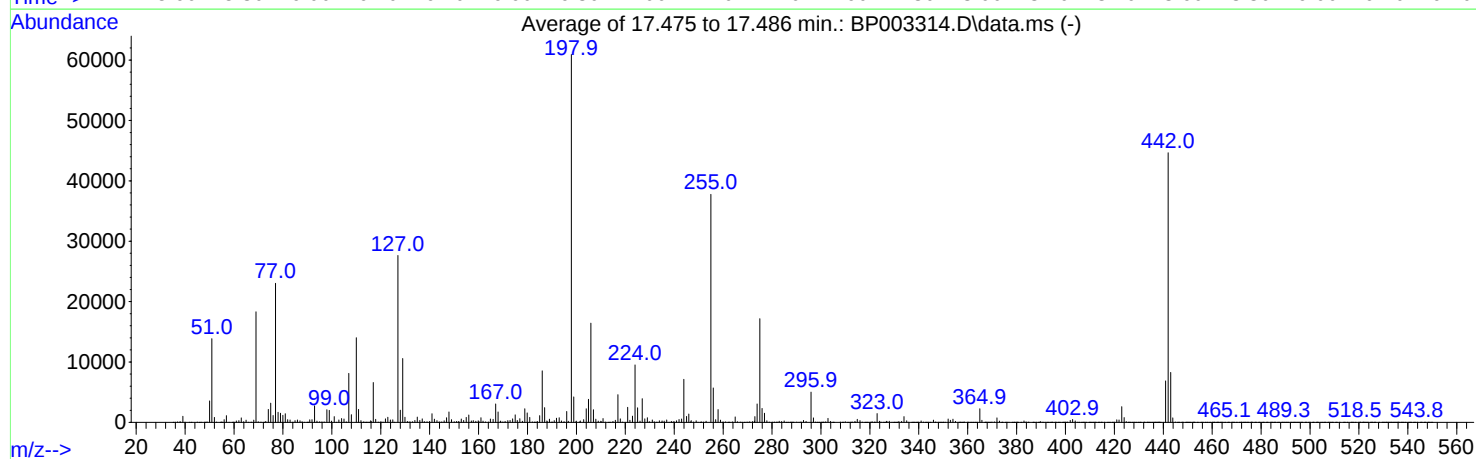


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091720\
Data File : BP003314.D
Acq On : 17 Sep 2020 13:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 18 14:13:41 2020

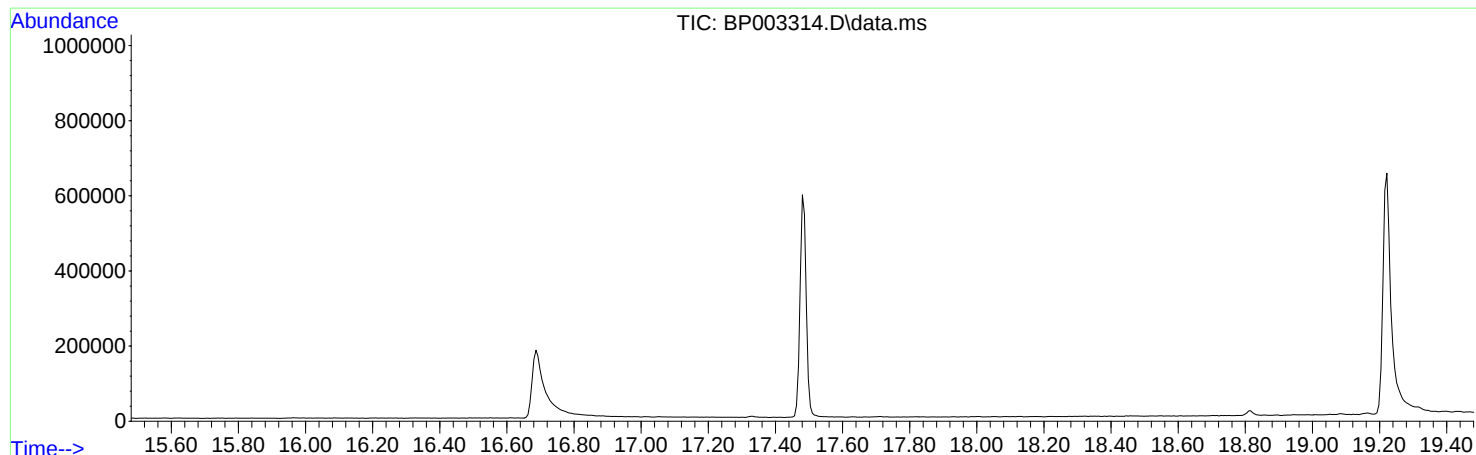

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.8	13869	PASS
68	69	0.00	2	2.0	362	PASS
69	198	0.00	100	30.1	18323	PASS
70	69	0.00	2	0.6	118	PASS
127	198	10	80	45.4	27653	PASS
197	198	0.00	2	0.3	183	PASS
198	198	100	100	100.0	60923	PASS
199	198	5	9	6.9	4220	PASS
275	198	10	60	28.2	17171	PASS
365	198	1	100	3.7	2267	PASS
441	198	0.01	100	11.3	6874	PASS
442	198	50	100	73.3	44653	PASS
443	442	15	24	18.5	8260	PASS