

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091819\
 Data File : BP000311.D
 Acq On : 18 Sep 2019 20:51
 Operator : HP/JU
 Sample : K4918-10DL 2X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SB-11DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.411	561	565	569	rBV	2261738	2060173	23.64%	1.936%
2	6.428	734	738	749	rVB	2507648	2251254	25.83%	2.115%
3	6.564	757	761	764	rBV	2872011	2316528	26.58%	2.177%
4	6.793	796	800	803	rBV	2195846	1629125	18.69%	1.531%
5	6.952	823	827	830	rBV	2257628	1952802	22.41%	1.835%
6	7.346	890	894	898	rBV	1513857	1201316	13.78%	1.129%
7	8.075	1014	1018	1021	rBV	2719526	2089754	23.98%	1.964%
8	9.152	1197	1201	1204	rBV	4076667	3080089	35.34%	2.894%
9	9.493	1255	1259	1262	rBV	1033330	96597	1.11%	0.091%
10	9.546	1265	1268	1273	rVB	335754	251807	2.89%	0.237%
11	9.693	1290	1293	1298	rVB	220115	170196	1.95%	0.160%
12	9.834	1314	1317	1320	rVV	3005212	2397217	27.50%	2.253%
13	9.869	1320	1323	1326	rVB	528718	431715	4.95%	0.406%
14	10.040	1349	1352	1356	rVB	359476	284645	3.27%	0.267%
15	10.387	1407	1411	1416	rVB	343903	325889	3.74%	0.306%
16	10.546	1435	1438	1443	rVB	168321	148431	1.70%	0.139%
17	10.628	1448	1452	1456	rBV	2231112	1954035	22.42%	1.836%
18	10.752	1468	1473	1476	rBV3	97095	113797	1.31%	0.107%
19	11.069	1522	1527	1529	rBV3	98411	123390	1.42%	0.116%
20	11.134	1535	1538	1542	rVB	565019	513536	5.89%	0.483%
21	11.187	1542	1547	1551	rBV4	125458	213095	2.44%	0.200%
22	11.222	1551	1553	1559	rVB	440302	409030	4.69%	0.384%
23	11.334	1568	1572	1573	rBV	2644424	2499652	28.68%	2.349%
24	11.357	1573	1576	1579	rVV	7581126	6637273	76.15%	6.237%
25	11.404	1582	1584	1587	rVV	1317195	1029473	11.81%	0.967%
26	11.440	1587	1590	1594	rVB	131124	122440	1.40%	0.115%
27	11.557	1605	1610	1613	rBV	892389	825842	9.48%	0.776%
28	11.628	1619	1622	1625	rVB	148914	122930	1.41%	0.116%
29	11.663	1625	1628	1634	rVB3	189295	173819	1.99%	0.163%
30	11.834	1654	1657	1660	rBV	716450	678284	7.78%	0.637%
31	11.863	1660	1662	1666	rVB	1134321	933469	10.71%	0.877%
32	11.910	1667	1670	1673	rBV	315580	265858	3.05%	0.250%
33	11.952	1673	1677	1679	rBV2	1012884	1125939	12.92%	1.058%
34	11.969	1679	1680	1684	rVB	530079	381939	4.38%	0.359%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091819\
 Data File : BP000311.D
 Acq On : 18 Sep 2019 20:51
 Operator : HP/JU
 Sample : K4918-10DL 2X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SB-11DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.016	1685	1688	1690	rBV3	72328	89357	1.03%	0.084%
36	12.134	1705	1708	1710	rBV	705025	586018	6.72%	0.551%
37	12.157	1710	1712	1716	rVV	1107767	850897	9.76%	0.800%
38	12.210	1719	1721	1725	rBV	88512	93186	1.07%	0.088%
39	12.287	1732	1734	1737	rVB2	202391	140504	1.61%	0.132%
40	12.316	1737	1739	1741	rBV	157620	115570	1.33%	0.109%
41	12.340	1741	1743	1746	rVB	159167	132763	1.52%	0.125%
42	12.393	1749	1752	1755	rBV	504863	490471	5.63%	0.461%
43	12.434	1755	1759	1761	rVV2	191985	249483	2.86%	0.234%
44	12.475	1764	1766	1772	rVB2	598854	615711	7.06%	0.579%
45	12.563	1776	1781	1784	rVB	8907484	8715751	100.00%	8.190%
46	12.616	1784	1790	1794	rBV3	182357	294035	3.37%	0.276%
47	12.651	1794	1796	1798	rVB	113794	88740	1.02%	0.083%
48	12.687	1798	1802	1803	rBV2	241337	251805	2.89%	0.237%
49	12.704	1803	1805	1810	rVB	326813	336568	3.86%	0.316%
50	12.793	1813	1820	1823	rBV2	7488432	8629065	99.01%	8.108%
51	12.834	1825	1827	1833	rVB2	328378	355557	4.08%	0.334%
52	12.904	1836	1839	1841	rBV	481252	499693	5.73%	0.470%
53	12.928	1841	1843	1850	rVB2	3571818	3439836	39.47%	3.232%
54	13.010	1851	1857	1860	rBV2	496336	876965	10.06%	0.824%
55	13.034	1860	1861	1864	rVB	188905	109222	1.25%	0.103%
56	13.069	1864	1867	1869	rBV3	124868	147704	1.69%	0.139%
57	13.093	1869	1871	1873	rVV2	357089	413696	4.75%	0.389%
58	13.116	1873	1875	1878	rVB	674858	577590	6.63%	0.543%
59	13.151	1878	1881	1883	rBV2	108306	126398	1.45%	0.119%
60	13.187	1884	1887	1889	rVB	220025	191763	2.20%	0.180%
61	13.222	1889	1893	1896	rBV2	796011	769377	8.83%	0.723%
62	13.281	1900	1903	1906	rBV2	135999	148396	1.70%	0.139%
63	13.316	1906	1909	1912	rVB	355789	276713	3.17%	0.260%
64	13.346	1912	1914	1918	rBV	410467	389630	4.47%	0.366%
65	13.628	1959	1962	1967	rVB	1046005	953028	10.93%	0.896%
66	13.740	1977	1981	1984	rBV2	900022	1050874	12.06%	0.987%
67	13.769	1984	1986	1988	rVV	723116	587910	6.75%	0.552%
68	13.793	1988	1990	1994	rVV2	536449	762777	8.75%	0.717%
69	13.840	1995	1998	2004	rVB	1121459	1181101	13.55%	1.110%
70	13.910	2008	2010	2015	rVV	169882	175920	2.02%	0.165%
71	13.993	2017	2024	2027	rBV3	4827408	7226308	82.91%	6.790%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091819\
Data File : BP000311.D
Acq On : 18 Sep 2019 20:51
Operator : HP/JU
Sample : K4918-10DL 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB-11DL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	14.028	2027	2030	2035	rVB	4065069	3844138	44.11%	3.612%
73	14.104	2041	2043	2045	rVB	311831	214833	2.46%	0.202%
74	14.216	2059	2062	2066	rBV2	478367	552687	6.34%	0.519%
75	14.351	2083	2085	2087	rBV	204770	193289	2.22%	0.182%
76	14.387	2089	2091	2094	rVV	670998	583181	6.69%	0.548%
77	14.422	2094	2097	2100	rVB2	470323	463236	5.31%	0.435%
78	14.510	2110	2112	2114	rBV	276054	256360	2.94%	0.241%
79	15.057	2199	2205	2208	rBV	3283934	5577425	63.99%	5.241%
80	15.157	2220	2222	2226	rVB	518471	503740	5.78%	0.473%
81	15.357	2252	2256	2262	rVB	1939057	2617509	30.03%	2.460%
82	15.422	2262	2267	2273	rVB	2571929	3231255	37.07%	3.036%
83	15.487	2273	2278	2281	rBV	1851871	2529703	29.02%	2.377%
84	15.516	2281	2283	2289	rVB	865869	1021727	11.72%	0.960%
85	16.975	2525	2531	2539	rVB2	1181116	2359227	27.07%	2.217%
86	17.416	2601	2606	2617	rVB	836931	1721739	19.75%	1.618%


Sum of corrected areas: 106421770

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091819\
Data File : BP000311.D
Acq On : 18 Sep 2019 20:51
Operator : HP/JU
Sample : K4918-10DL 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB-11DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

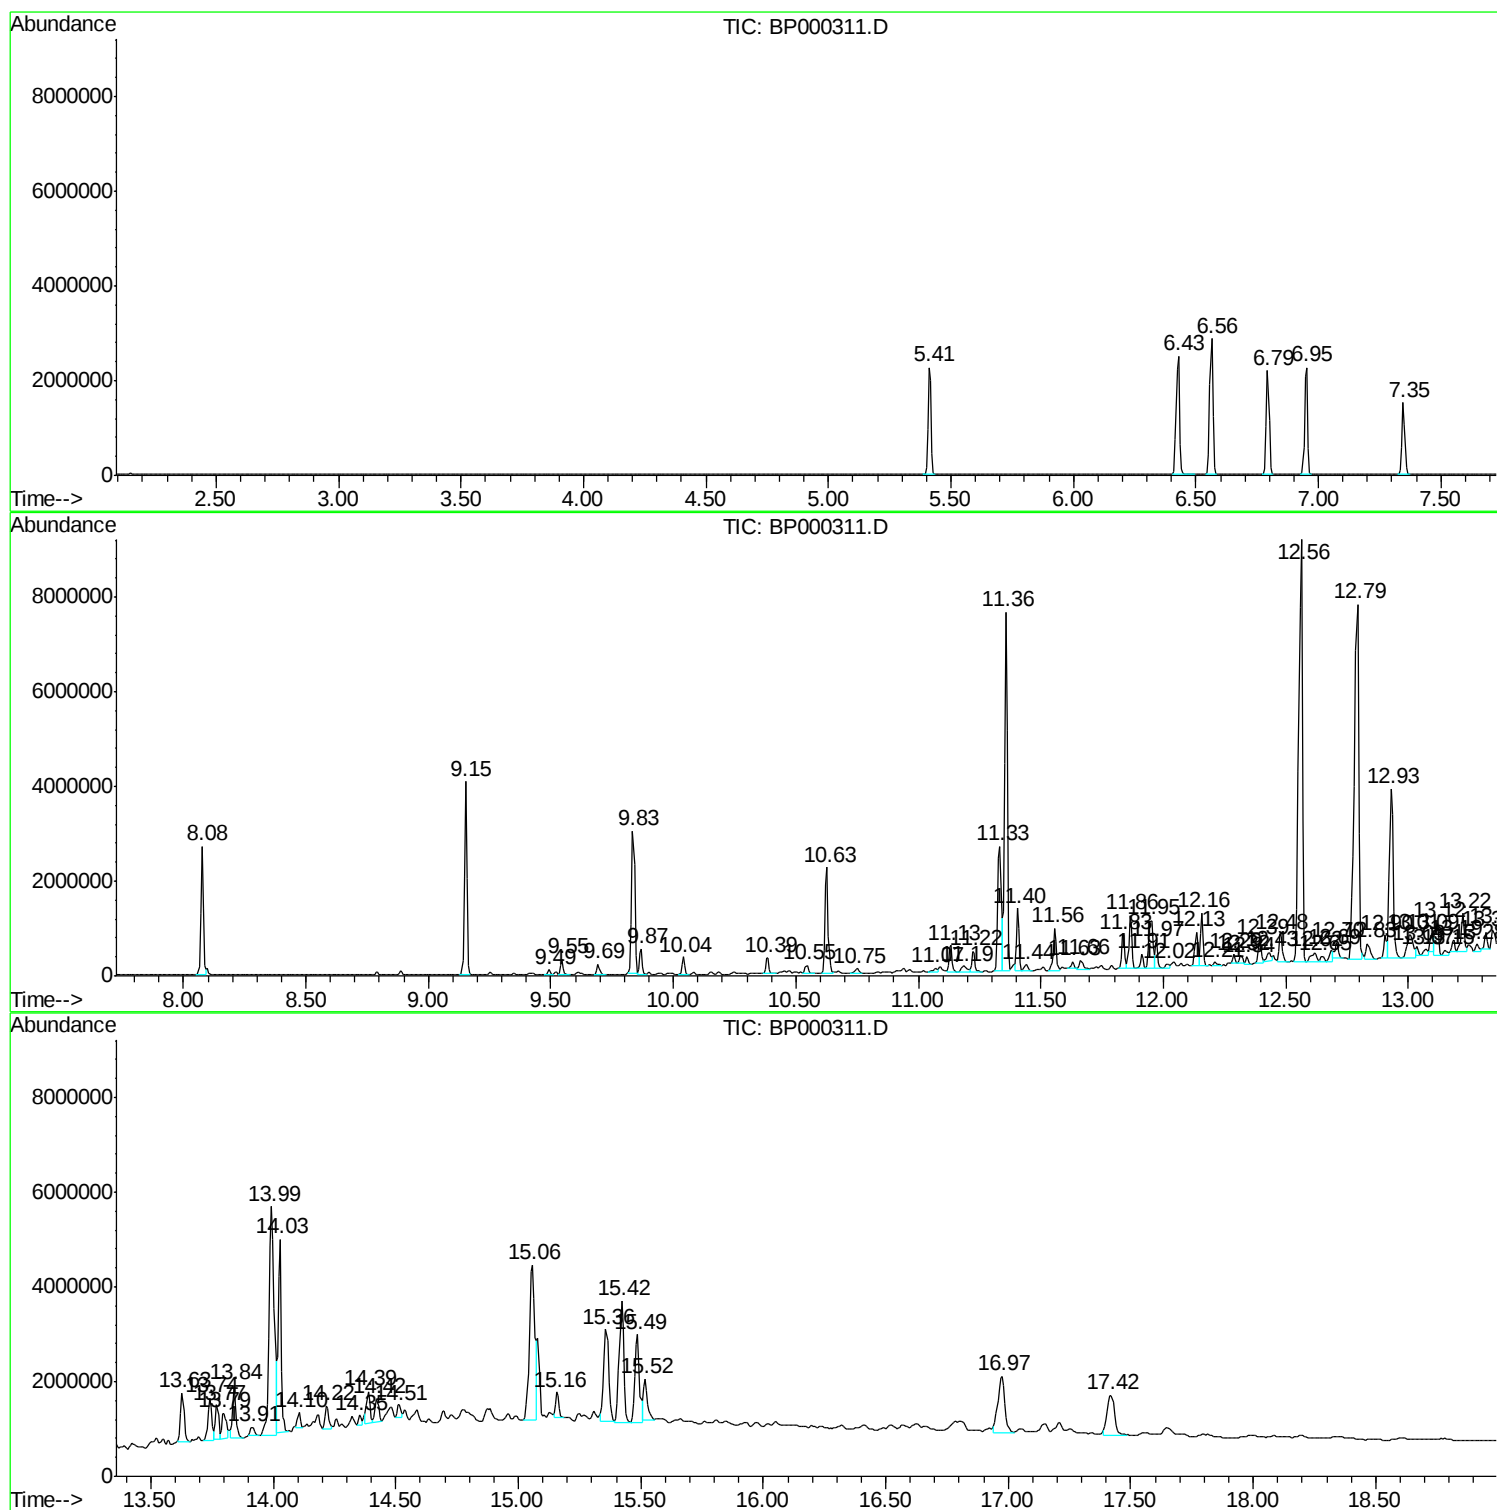

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091819\
Data_File : BP000311.D
Acq_On : 18-Sep-2019 20:511
Operator : HP/JUU
Sample : K4918-10DL_2X
Misc :
ALS_Vial : 23 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
SB-11DL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
