


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091819\
 Data File : BP000289.D
 Acq On : 18 Sep 2019 11:26
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 19 14:44:51 2019

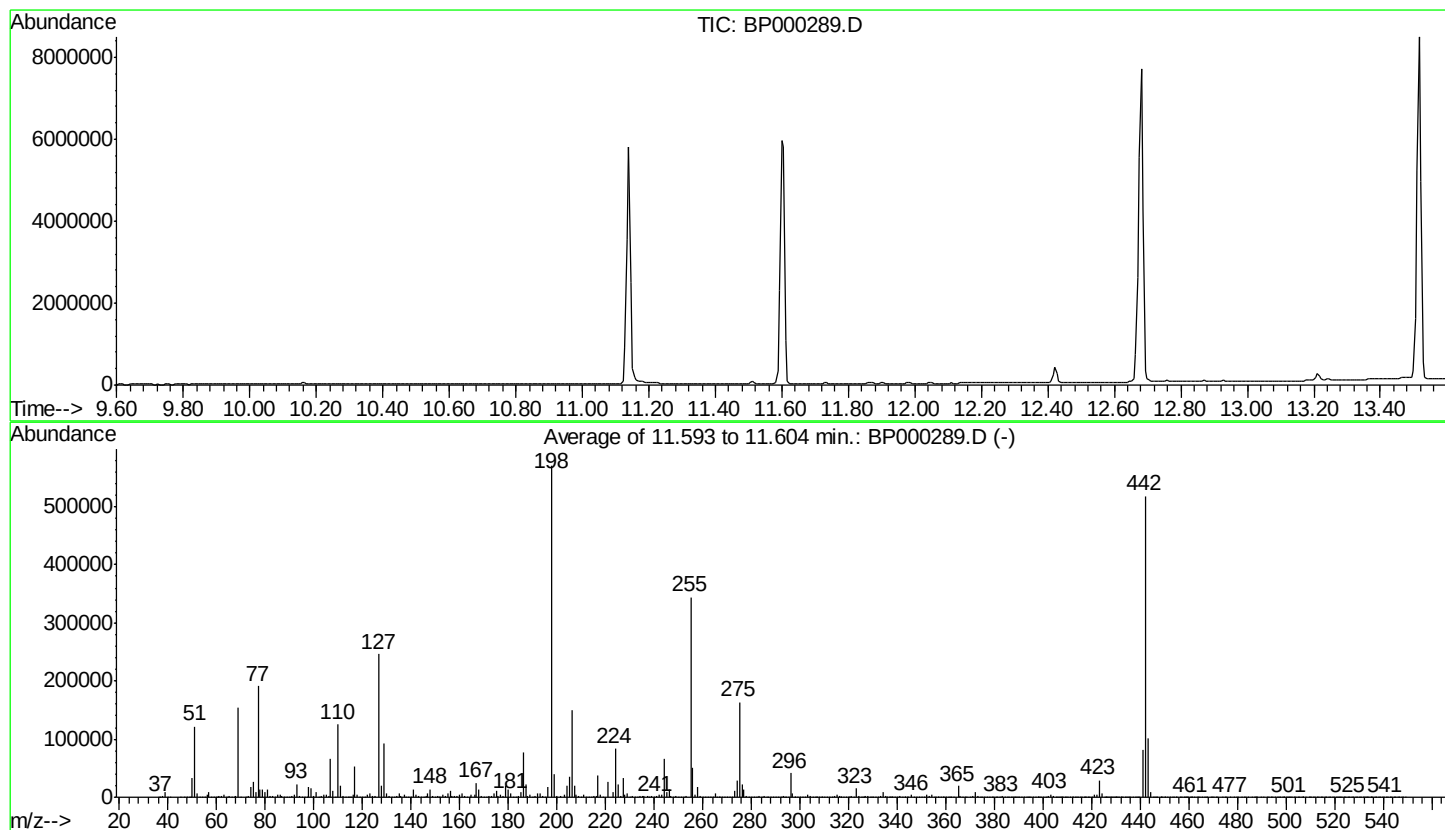

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.4	122084	PASS
68	69	0.00	2	1.0	1511	PASS
69	198	0.00	100	26.9	153535	PASS
70	69	0.00	2	0.5	701	PASS
127	198	10	80	43.1	245920	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	570471	PASS
199	198	5	9	6.9	39478	PASS
275	198	10	60	28.6	163397	PASS
365	198	1	100	3.4	19168	PASS
441	198	0.01	100	14.4	82236	PASS
442	198	50	100	90.7	517557	PASS
443	442	15	24	19.4	100365	PASS