

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP091823\  
 Data File : BP017201.D  
 Acq On : 18 Sep 2023 12:49  
 Operator : MA/JU  
 Sample : 04330-20  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 EZYL5

Quant Time: Sep 18 22:31:17 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP091223.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sat Sep 16 03:18:48 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| -----                         |        |      |          |        |        |          |
| Internal Standards            |        |      |          |        |        |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.945  | 152  | 183313   | 20.000 | ng/ul  | 0.00     |
| 20) Naphthalene-d8            | 10.769 | 136  | 762811   | 20.000 | ng/ul  | 0.00     |
| 38) Acenaphthene-d10          | 14.604 | 164  | 479526   | 20.000 | ng/ul  | 0.00     |
| 64) Phenanthrene-d10          | 17.374 | 188  | 1091326  | 20.000 | ng/ul  | 0.00     |
| 79) Chrysene-d12              | 21.474 | 240  | 839764   | 20.000 | ng/ul  | 0.00     |
| 88) Perylene-d12              | 23.998 | 264  | 797851   | 20.000 | ng/ul  | 0.00     |
| System Monitoring Compounds   |        |      |          |        |        |          |
| 3) 1,4-Dioxane-d8             | 3.310  | 96   | 11140    | 2.554  | ng/uL  | 0.00     |
| 4) Pyridine-d5                | 3.757  | 84   | 20083    | 1.609  | ng/ul  | 0.01     |
| 7) Phenol-d5                  | 7.093  | 99   | 188974   | 12.678 | ng/ul  | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.287  | 67   | 131979   | 14.166 | ng/ul  | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.463  | 132  | 145342   | 12.223 | ng/ul  | 0.00     |
| 15) 4-Methylphenol-d8         | 8.651  | 113  | 105020   | 8.501  | ng/ul  | 0.00     |
| 21) Nitrobenzene-d5           | 9.145  | 128  | 75024    | 14.046 | ng/ul  | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.857  | 143  | 57678    | 10.115 | ng/ul  | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.381 | 165  | 122599   | 11.117 | ng/ul  | 0.00     |
| 31) 4-Chloroaniline-d4        | 10.934 | 131  | 192028   | 11.552 | ng/ul  | 0.00     |
| 46) Dimethylphthalate-d6      | 14.016 | 166  | 524840   | 15.380 | ng/ul  | 0.00     |
| 49) Acenaphthylene-d8         | 14.304 | 160  | 546959   | 14.126 | ng/ul  | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.810 | 143  | 6        | 0.001  | ng/ul  | -0.02    |
| 60) Fluorene-d10              | 15.598 | 176  | 470465   | 15.945 | ng/ul  | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.733 | 200  | 670      | 0.110  | ng/ul  | 0.00     |
| 73) Anthracene-d10            | 17.474 | 188  | 734325   | 15.837 | ng/ul  | 0.00     |
| 81) Pyrene-d10                | 19.715 | 212  | 1015938  | 23.068 | ng/ul  | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.827 | 264  | 700198   | 18.594 | ng/ul  | -0.01    |
| Target Compounds              |        |      |          |        |        |          |
|                               |        |      |          |        | Qvalue |          |
| 16) Acetophenone              | 8.792  | 105  | 41241    | 2.133  | ng/ul  | 95       |
| -----                         |        |      |          |        |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP091823\  
Data File : BP017201.D  
Acq On : 18 Sep 2023 12:49  
Operator : MA/JU  
Sample : 04330-20  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
EZY5

Quant Time: Sep 18 22:31:17 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP091223.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Sep 16 03:18:48 2023  
Response via : Initial Calibration

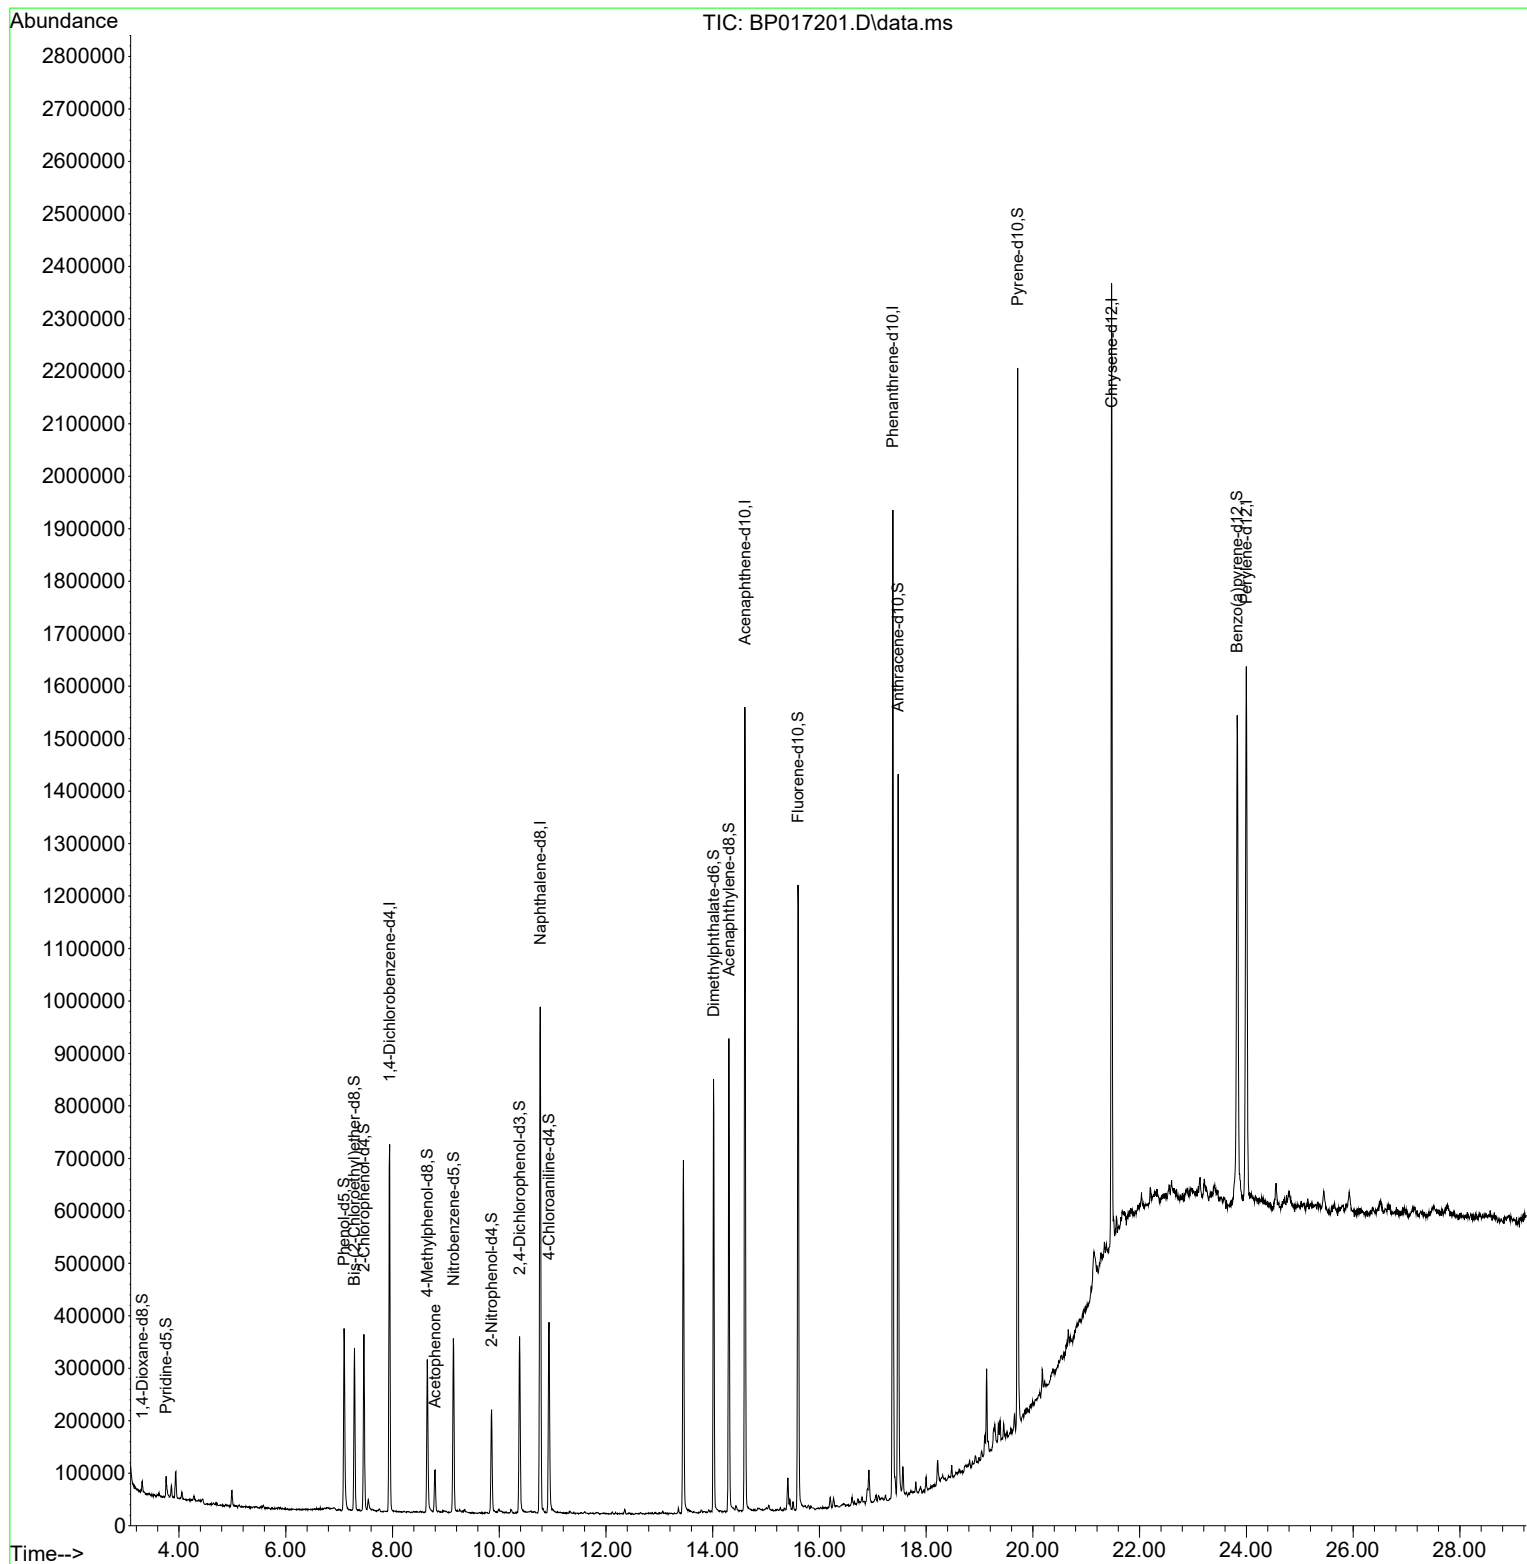

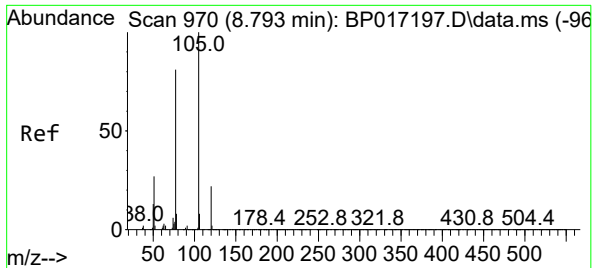

#16  
 Acetophenone  
 Concen: 2.133 ng/ul  
 RT: 8.792 min Scan# 91  
 Delta R.T. -0.006 min  
 Lab File: BP017201.D  
 Acq: 18 Sep 2023 12:49

Instrument :  
 BNA\_P  
 ClientSampleId :  
 EZYL5

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 105   | Resp: | 41241 |
| Ion      | Ratio | Lower | Upper |
| 105      | 100   |       |       |
| 77       | 82.8  | 63.0  | 94.4  |
| 51       | 29.0  | 20.5  | 30.7  |

