

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017204.D
 Acq On : 18 Sep 2023 14:33
 Operator : MA/JU
 Sample : 04332-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC4

Quant Time: Sep 18 22:31:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 16 03:18:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	180964	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136	766820	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.604	164	474774	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.375	188	1039894	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240	771497	20.000	ng/ul	0.00
88) Perylene-d12	23.998	264	724644	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	13975	3.245	ng/uL	0.00
4) Pyridine-d5	3.734	84	284	0.023	ng/ul	-0.01
7) Phenol-d5	7.099	99	216073	14.684	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	185517	20.171	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	198890	16.943	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	131003	10.742	ng/ul	0.00
21) Nitrobenzene-d5	9.146	128	107912	20.097	ng/ul	0.00
24) 2-Nitrophenol-d4	9.857	143	113911	19.872	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	196431	17.719	ng/ul	0.00
31) 4-Chloroaniline-d4	10.934	131	148625	8.895	ng/ul	0.00
46) Dimethylphthalate-d6	14.022	166	709579	21.002	ng/ul	0.00
49) Acenaphthylene-d8	14.304	160	772678	20.155	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	62515	9.574	ng/ul	0.00
60) Fluorene-d10	15.604	176	619805	21.217	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.734	200	70943	12.211	ng/ul	0.00
73) Anthracene-d10	17.475	188	946012	21.411	ng/ul	0.00
81) Pyrene-d10	19.716	212	1105642	27.326	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.833	264	734253	21.468	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.793	105	61212	3.207	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017204.D
Acq On : 18 Sep 2023 14:33
Operator : MA/JU
Sample : 04332-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC4

Quant Time: Sep 18 22:31:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 16 03:18:48 2023
Response via : Initial Calibration

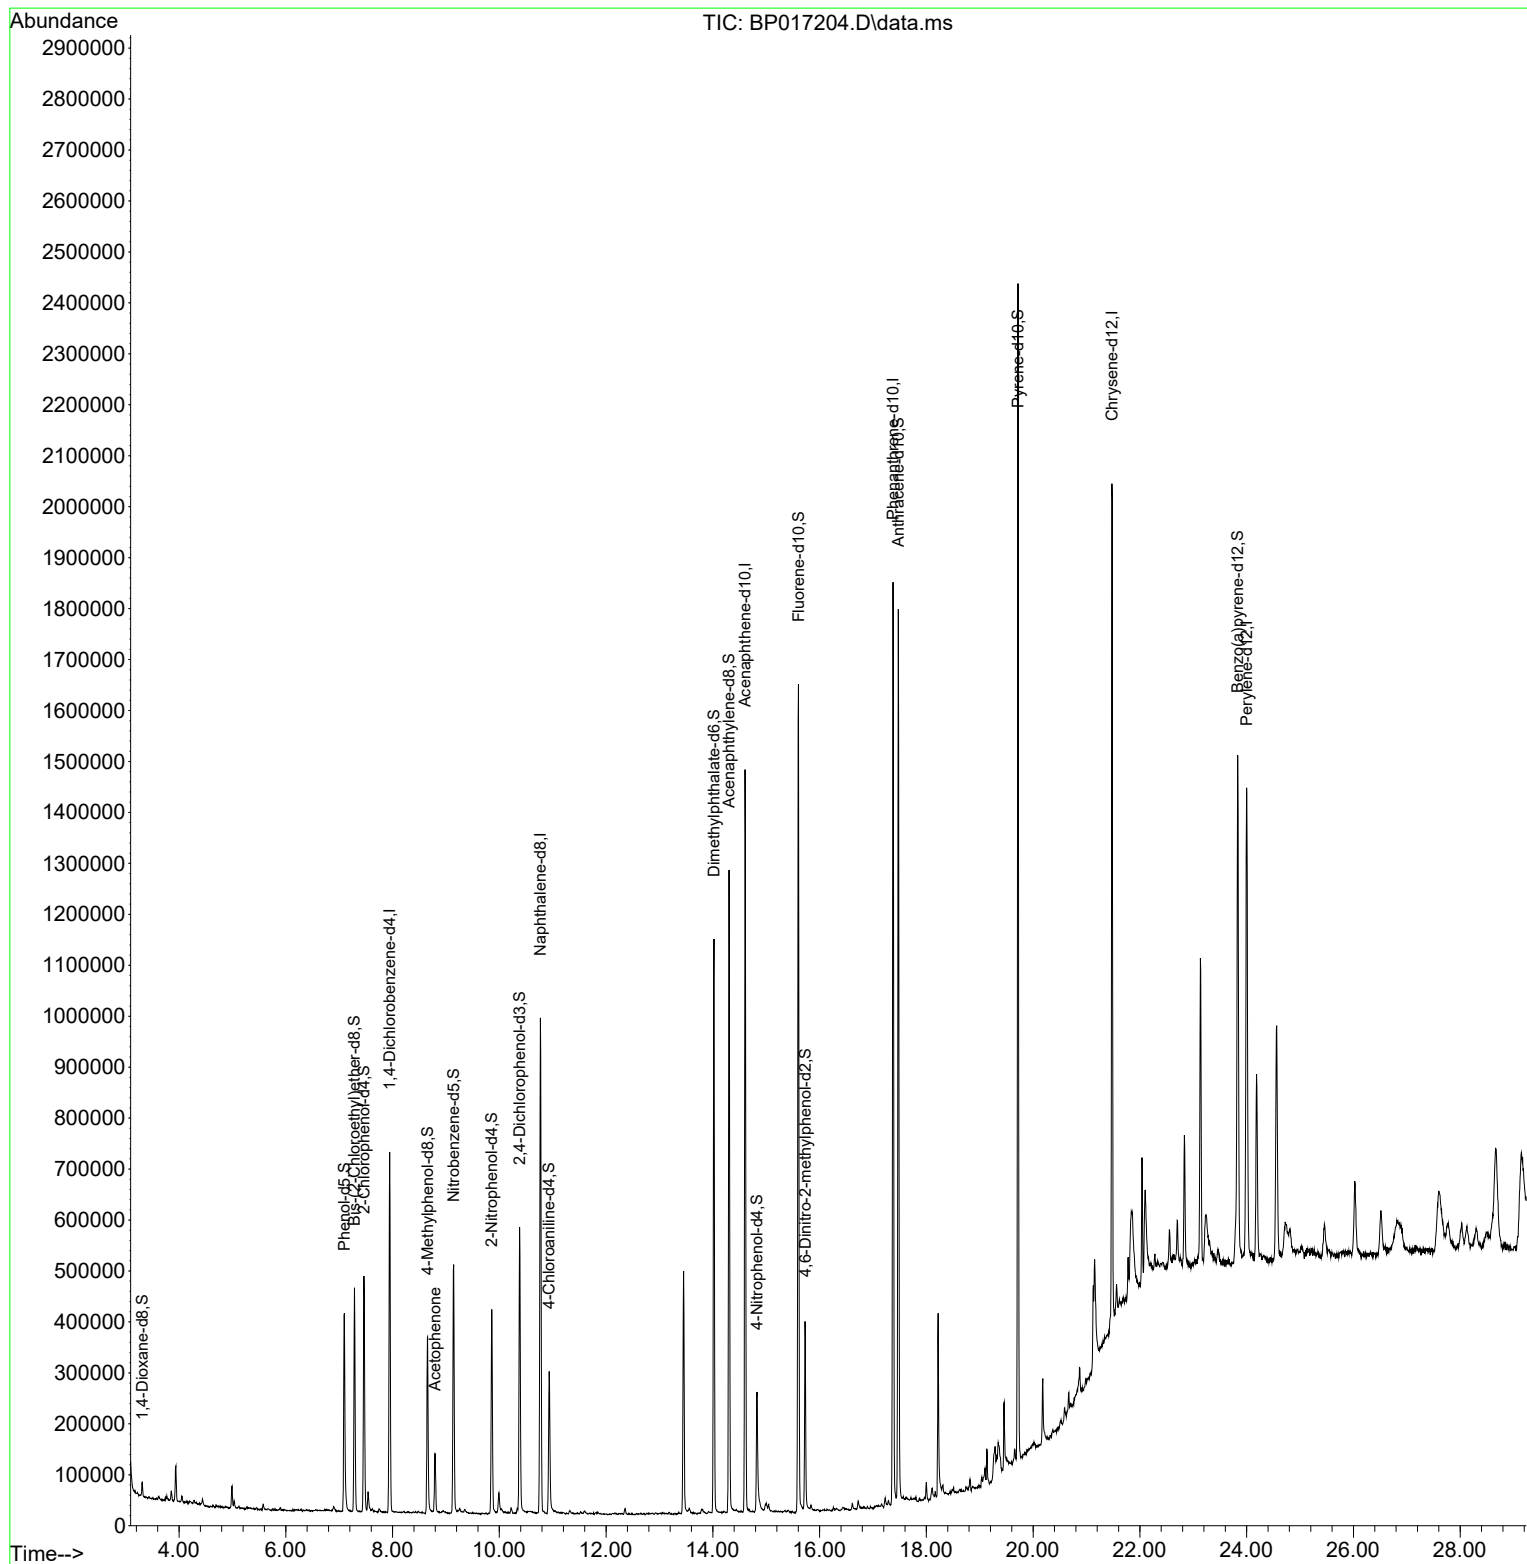

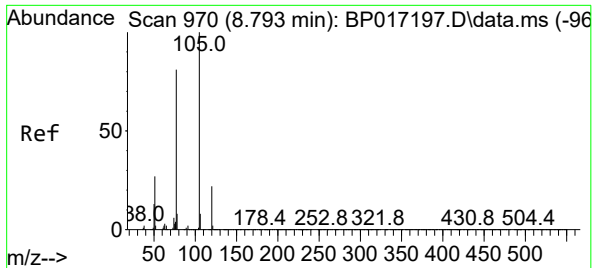

#16
 Acetophenone
 Concen: 3.207 ng/ul
 RT: 8.793 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP017204.D
 Acq: 18 Sep 2023 14:33

Instrument :
 BNA_P
 ClientSampleId :
 C0AC4

Tgt Ion:	105	Resp:	61212
Ion Ratio	Lower	Upper	
105	100		
77	78.6	63.0	94.4
51	27.8	20.5	30.7

