

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017206.D
 Acq On : 18 Sep 2023 15:41
 Operator : MA/JU
 Sample : 04332-20
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG8

Quant Time: Sep 18 22:32:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 16 03:18:48 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	186130	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136	800467	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.604	164	514483	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.375	188	1171254	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	953663	20.000	ng/ul	0.00
88) Perylene-d12	24.004	264	902356	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	20901	4.719	ng/uL	0.00
4) Pyridine-d5	3.746	84	291083	22.973	ng/ul	0.00
7) Phenol-d5	7.099	99	389787	25.754	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	251728	26.611	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	314457	26.044	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	309305	24.659	ng/ul	0.00
21) Nitrobenzene-d5	9.146	128	150542	26.858	ng/ul	0.00
24) 2-Nitrophenol-d4	9.857	143	164484	27.488	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	301369	26.042	ng/ul	0.00
31) 4-Chloroaniline-d4	10.934	131	436413	25.020	ng/ul	0.00
46) Dimethylphthalate-d6	14.022	166	1000422	27.325	ng/ul	0.00
49) Acenaphthylene-d8	14.304	160	1117732	26.906	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	117853	16.655	ng/ul	0.00
60) Fluorene-d10	15.604	176	887855	28.047	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.728	200	104488	15.968	ng/ul	0.00
73) Anthracene-d10	17.475	188	1389022	27.912	ng/ul	0.00
81) Pyrene-d10	19.716	212	1598910	31.969	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.833	264	1190628	27.956	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.339	149	108736	3.516	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017206.D
Acq On : 18 Sep 2023 15:41
Operator : MA/JU
Sample : 04332-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG8

Quant Time: Sep 18 22:32:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 16 03:18:48 2023
Response via : Initial Calibration

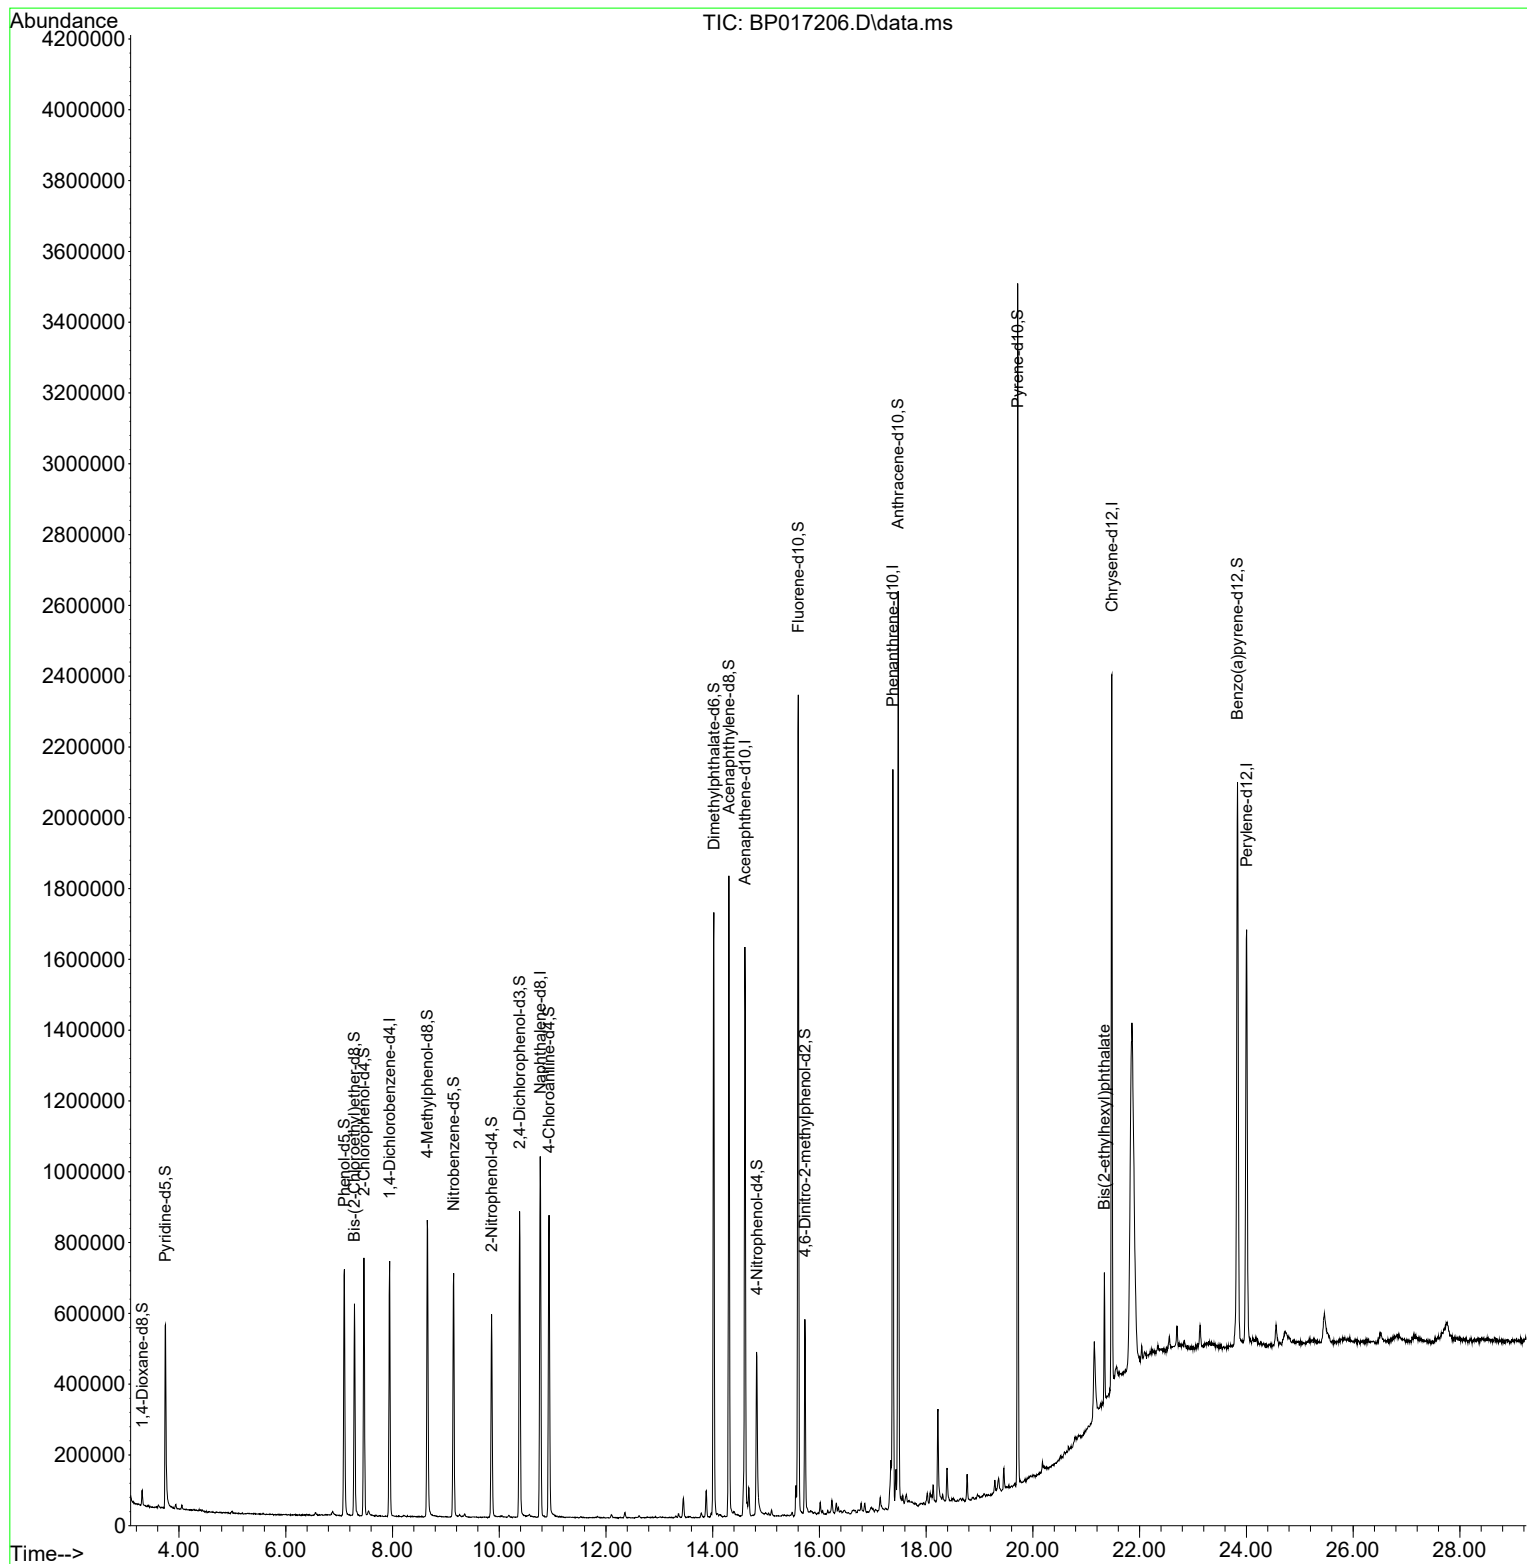

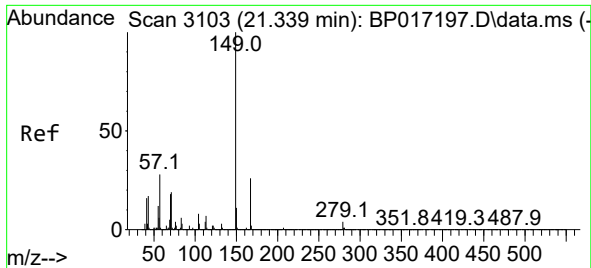

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 3.516 ng/ul
 RT: 21.339 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BP017206.D
 Acq: 18 Sep 2023 15:41

Instrument :
 BNA_P
 ClientSampleId :
 C0AG8

Tgt Ion:149 Resp: 108736
 Ion Ratio Lower Upper
 149 100
 167 26.2 21.3 31.9
 279 3.8 3.4 5.2

