

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017214.D
 Acq On : 18 Sep 2023 20:16
 Operator : MA/JU
 Sample : 04330-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF6

Quant Time: Sep 18 22:34:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 16 03:18:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	319306	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136	1347672	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.604	164	826259	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.375	188	1784086	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	1187422	20.000	ng/ul	0.00
88) Perylene-d12	24.004	264	1228448	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	17678	2.327	ng/uL	0.00
4) Pyridine-d5	3.758	84	20356	0.936	ng/ul	0.01
7) Phenol-d5	7.093	99	347714	13.392	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	221741	13.664	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	284849	13.752	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	174215	8.096	ng/ul	0.00
21) Nitrobenzene-d5	9.140	128	134684	14.272	ng/ul	0.00
24) 2-Nitrophenol-d4	9.857	143	149566	14.846	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	263758	13.537	ng/ul	0.00
31) 4-Chloroaniline-d4	10.934	131	185357	6.312	ng/ul	0.00
46) Dimethylphthalate-d6	14.016	166	886031	15.069	ng/ul	0.00
49) Acenaphthylene-d8	14.304	160	944560	14.158	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	79631	7.007	ng/ul	0.00
60) Fluorene-d10	15.598	176	809226	15.917	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.728	200	73361	7.360	ng/ul	0.00
73) Anthracene-d10	17.475	188	1253741	16.540	ng/ul	0.00
81) Pyrene-d10	19.716	212	1369534	21.992	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.833	264	976114	16.835	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.793	105	170406	5.060	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017214.D
Acq On : 18 Sep 2023 20:16
Operator : MA/JU
Sample : 04330-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF6

Quant Time: Sep 18 22:34:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 16 03:18:48 2023
Response via : Initial Calibration

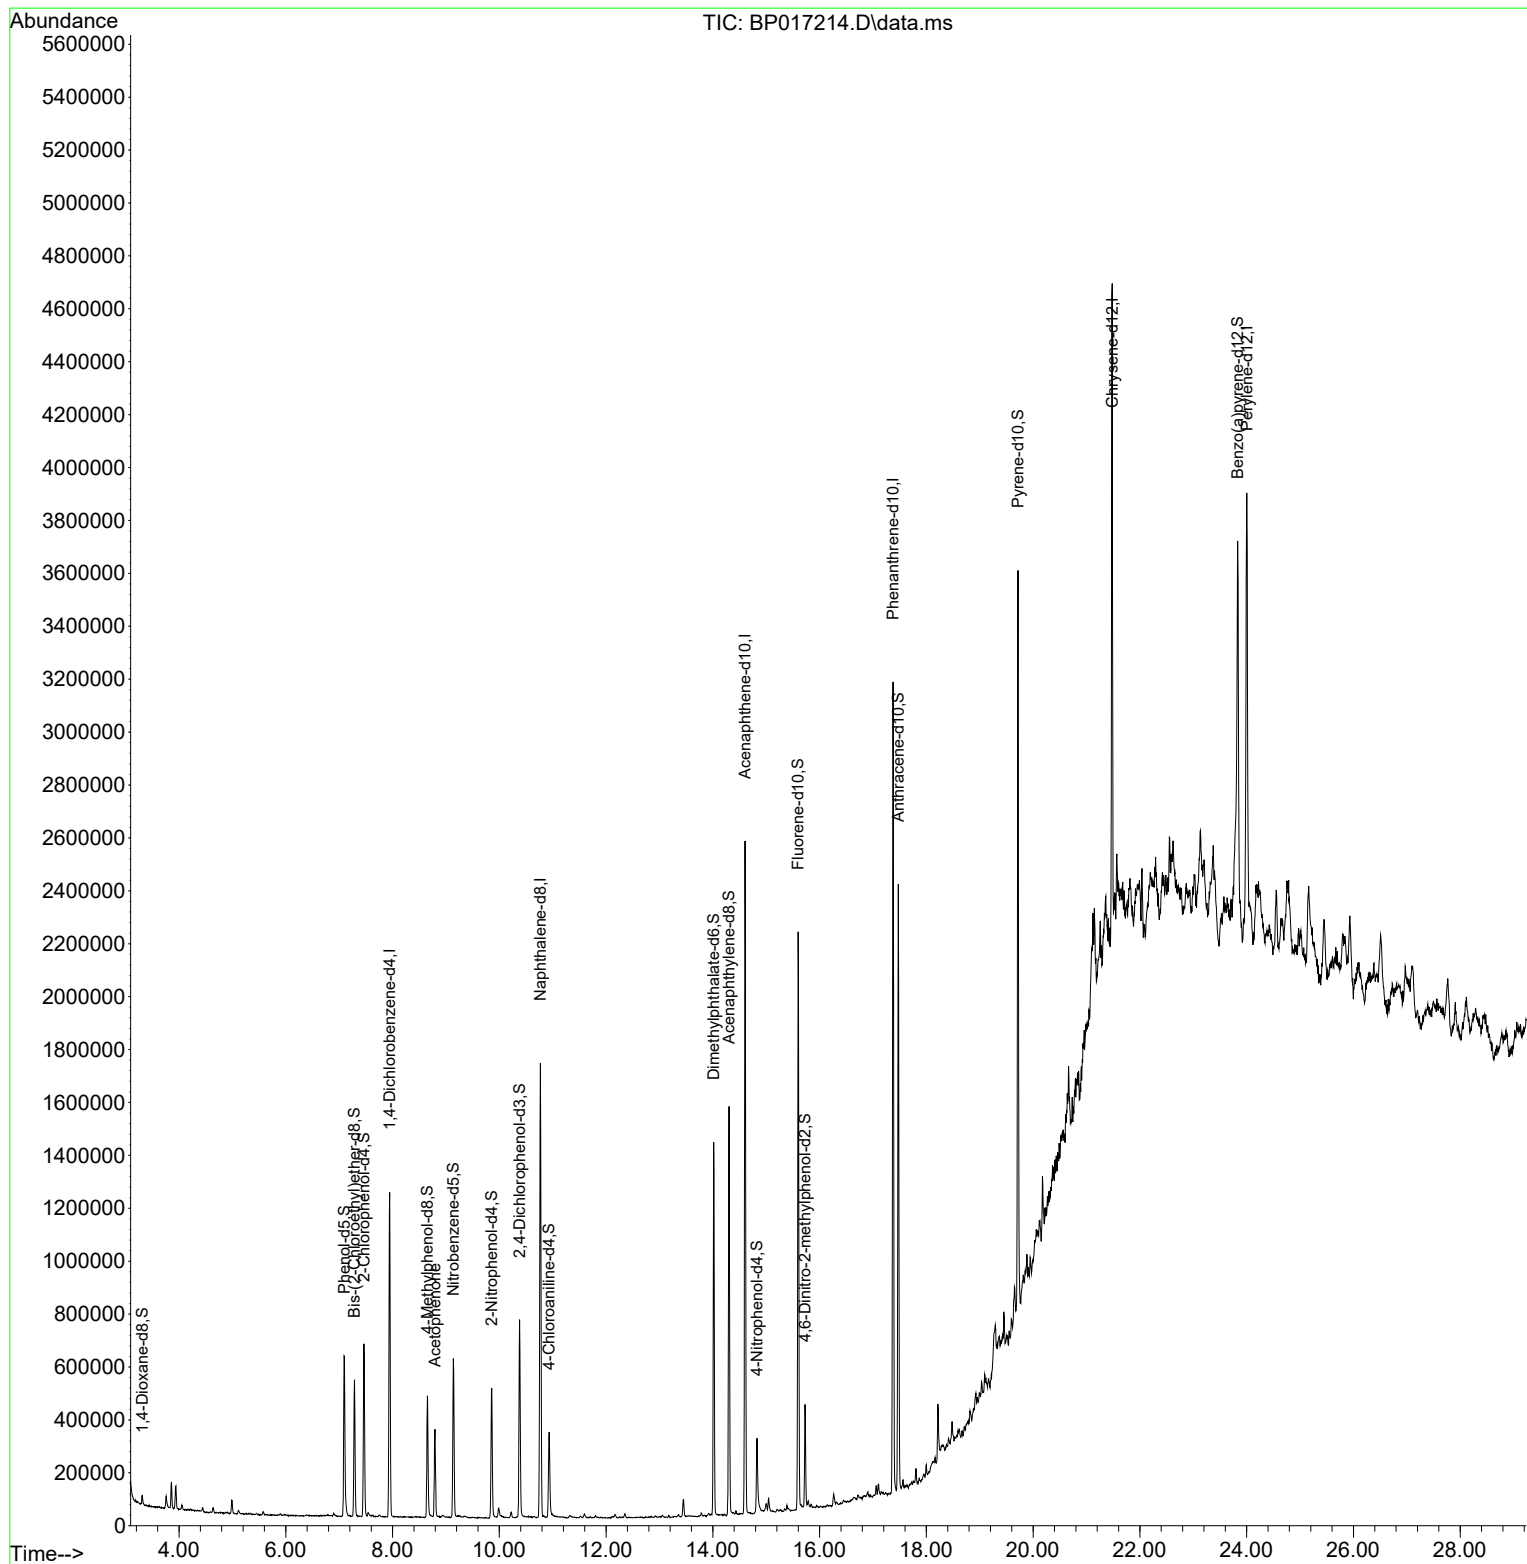

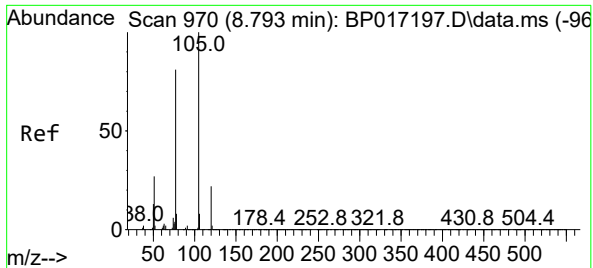

#16
 Acetophenone
 Concen: 5.060 ng/ul
 RT: 8.793 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP017214.D
 Acq: 18 Sep 2023 20:16

Instrument :
 BNA_P
 ClientSampleId :
 EZYF6

Tgt Ion:105 Resp: 170406

Ion	Ratio	Lower	Upper
105	100		
77	79.3	63.0	94.4
51	26.5	20.5	30.7

