

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017205.D
 Acq On : 18 Sep 2023 15:07
 Operator : MA/JU
 Sample : 04332-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC6

Quant Time: Sep 18 23:12:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 16 03:18:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.945	152	209106	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	889825	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.604	164	547287	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.374	188	1228089	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	1003402	20.000	ng/u1	0.00
88) Perylene-d12	24.003	264	922551	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.310	96	12725	2.557	ng/uL	0.00
4) Pyridine-d5	3.757	84	19124	1.343	ng/u1	0.01
7) Phenol-d5	7.098	99	193023	11.352	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	185170	17.424	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	199844	14.733	ng/u1	0.00
15) 4-Methylphenol-d8	8.657	113	98796	7.011	ng/u1	0.00
21) Nitrobenzene-d5	9.145	128	108620	17.433	ng/u1	0.00
24) 2-Nitrophenol-d4	9.857	143	116237	17.474	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	199269	15.490	ng/u1	0.00
31) 4-Chloroaniline-d4	10.934	131	38304	1.975	ng/u1	0.00
46) Dimethylphthalate-d6	14.022	166	679514	17.448	ng/u1	0.00
49) Acenaphthylene-d8	14.304	160	747895	16.924	ng/u1	0.00
54) 4-Nitrophenol-d4	14.827	143	42707	5.674	ng/u1	0.00
60) Fluorene-d10	15.604	176	597619	17.747	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	65531	9.551	ng/u1	0.00
73) Anthracene-d10	17.474	188	872806	16.727	ng/u1	0.00
81) Pyrene-d10	19.715	212	1107385	21.044	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	767726	17.632	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.122	94	18627	1.039	ng/u1	99
16) Acetophenone	8.798	105	103181	4.678	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017205.D
Acq On : 18 Sep 2023 15:07
Operator : MA/JU
Sample : 04332-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC6

Quant Time: Sep 18 23:12:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 16 03:18:48 2023
Response via : Initial Calibration




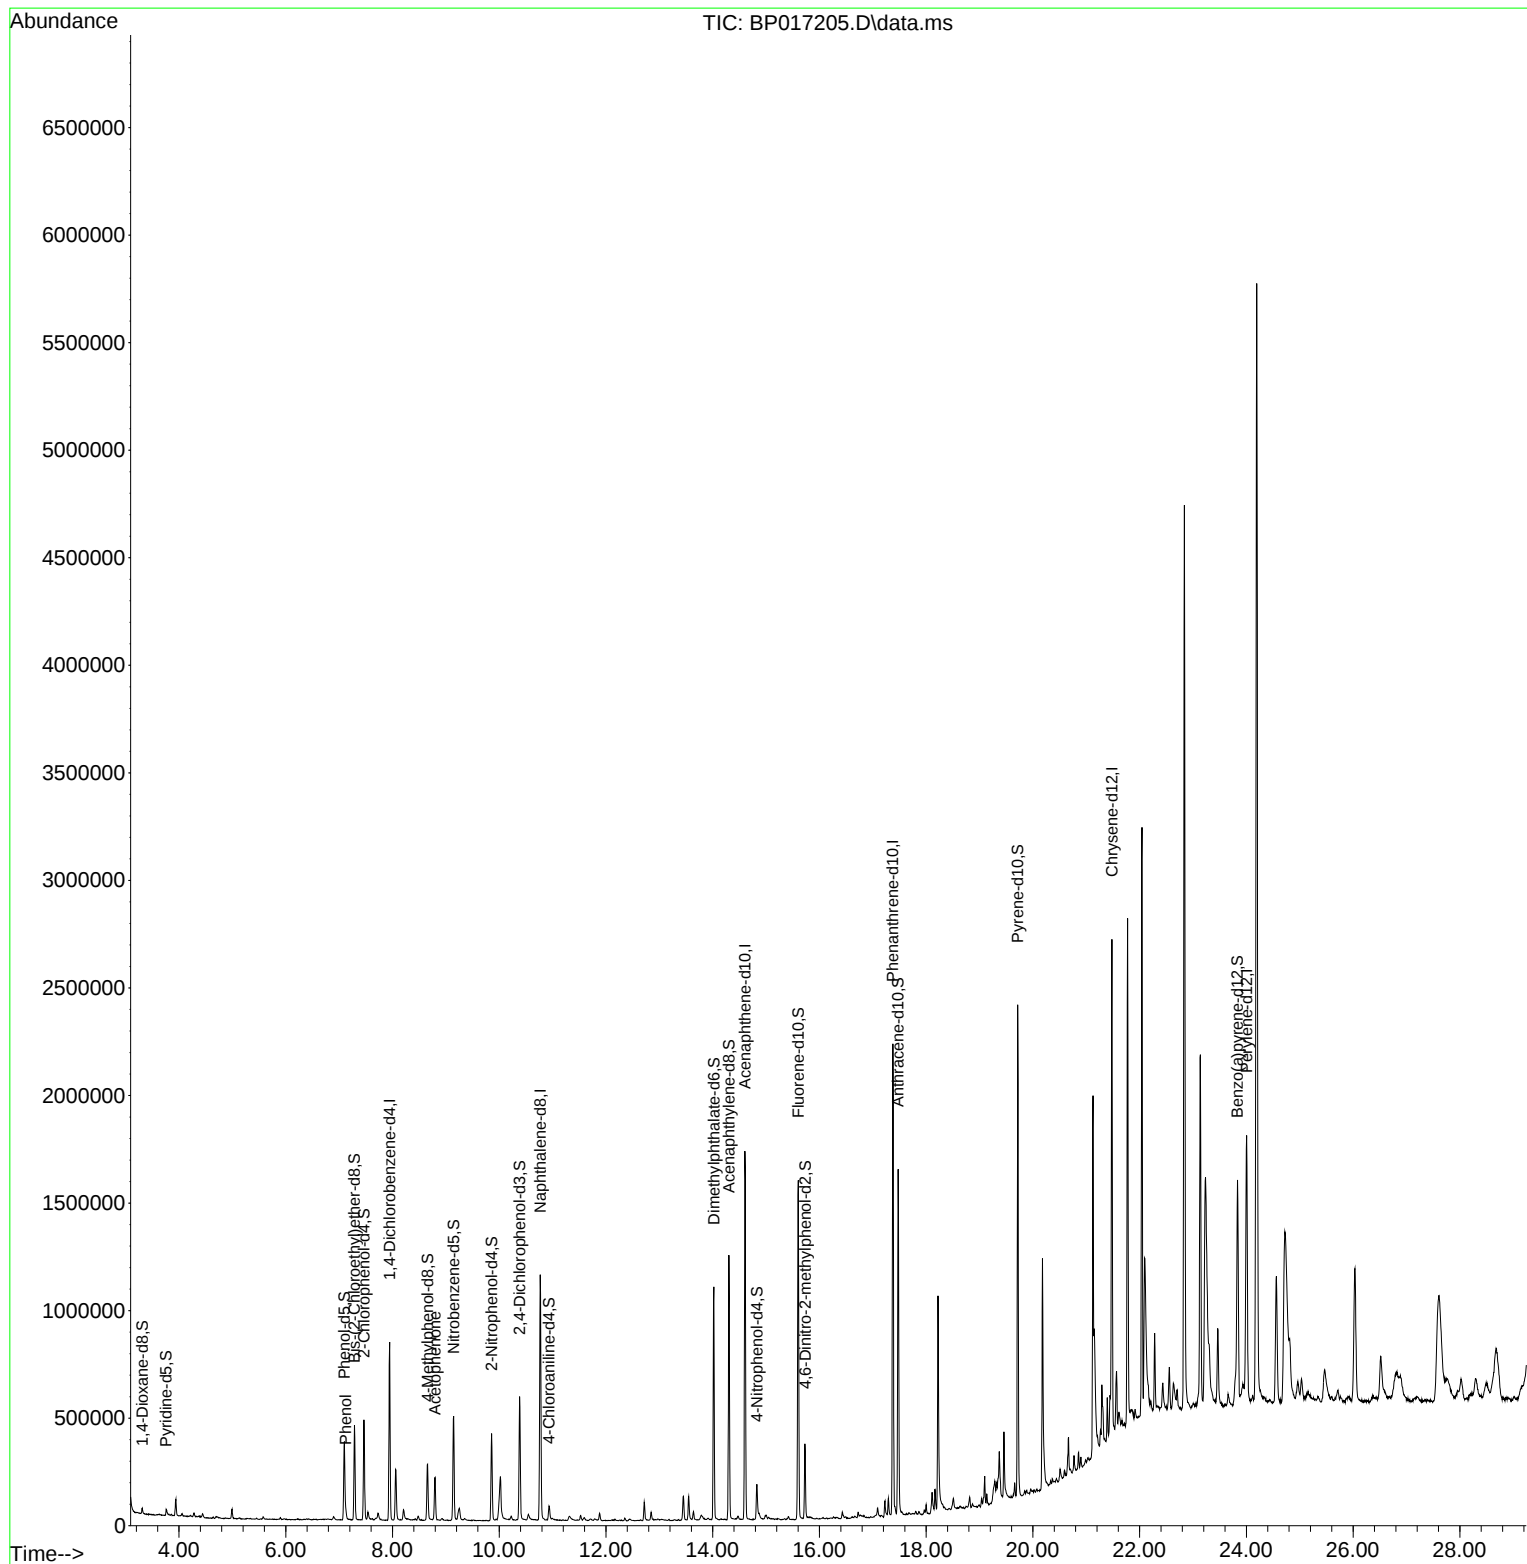


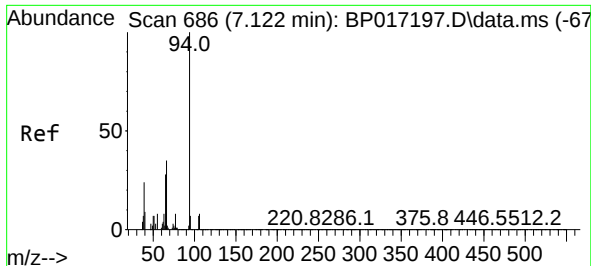

#8
Phenol
Concen: 1.039 ng/ul
RT: 7.122 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP017205.D
Acq: 18 Sep 2023 15:07

Instrument :
BNA_P
ClientSampleId :
C0AC6

Tgt Ion:	94	Resp:	18627
Ion	Ratio	Lower	Upper
94	100		
65	29.5	22.7	34.1
66	36.5	29.6	44.4

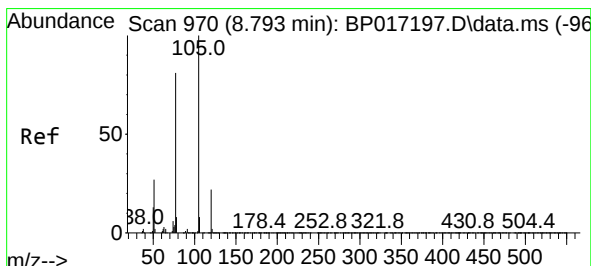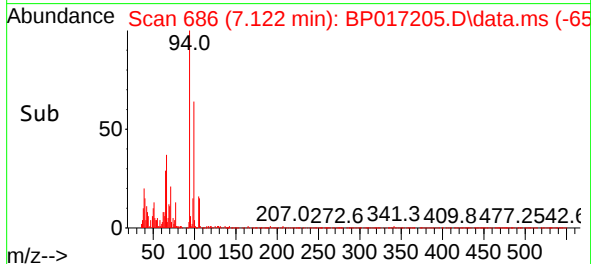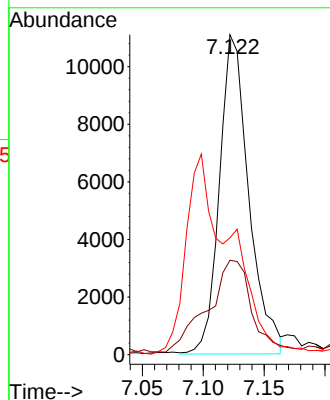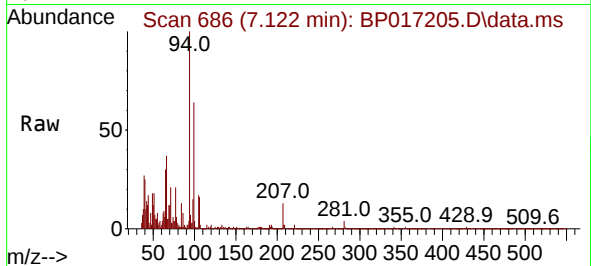

#16
Acetophenone
Concen: 4.678 ng/ul
RT: 8.798 min Scan# 971
Delta R.T. -0.000 min
Lab File: BP017205.D
Acq: 18 Sep 2023 15:07

Tgt Ion:	105	Resp:	103181
Ion	Ratio	Lower	Upper
105	100		
77	78.5	63.0	94.4
51	26.5	20.5	30.7

