

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017215.D
 Acq On : 18 Sep 2023 20:51
 Operator : MA/JU
 Sample : 04330-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYW7

Quant Time: Sep 18 23:53:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 16 03:18:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	283188	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	1188194	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.604	164	721057	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.375	188	1526120	20.000	ng/u1	0.00
79) Chrysene-d12	21.474	240	981062	20.000	ng/u1	0.00
88) Perylene-d12	24.004	264	1084545	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	19784	2.936	ng/uL	0.00
4) Pyridine-d5	3.758	84	26233	1.361	ng/u1	0.01
7) Phenol-d5	7.099	99	380635	16.530	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	246697	17.141	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	317019	17.258	ng/u1	0.00
15) 4-Methylphenol-d8	8.657	113	171286	8.975	ng/u1	0.00
21) Nitrobenzene-d5	9.146	128	155165	18.650	ng/u1	0.00
24) 2-Nitrophenol-d4	9.857	143	172407	19.410	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	291324	16.959	ng/u1	0.00
31) 4-Chloroaniline-d4	10.934	131	245735	9.491	ng/u1	0.00
46) Dimethylphthalate-d6	14.016	166	980777	19.114	ng/u1	0.00
49) Acenaphthylene-d8	14.304	160	1063890	18.273	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	81943	8.263	ng/u1	0.00
60) Fluorene-d10	15.604	176	894765	20.167	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	71457	8.381	ng/u1	0.00
73) Anthracene-d10	17.475	188	1345928	20.757	ng/u1	0.00
81) Pyrene-d10	19.716	212	1414234	27.487	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	1073097	20.964	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.793	105	94730	3.171	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017215.D
Acq On : 18 Sep 2023 20:51
Operator : MA/JU
Sample : 04330-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYW7

Quant Time: Sep 18 23:53:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 16 03:18:48 2023
Response via : Initial Calibration

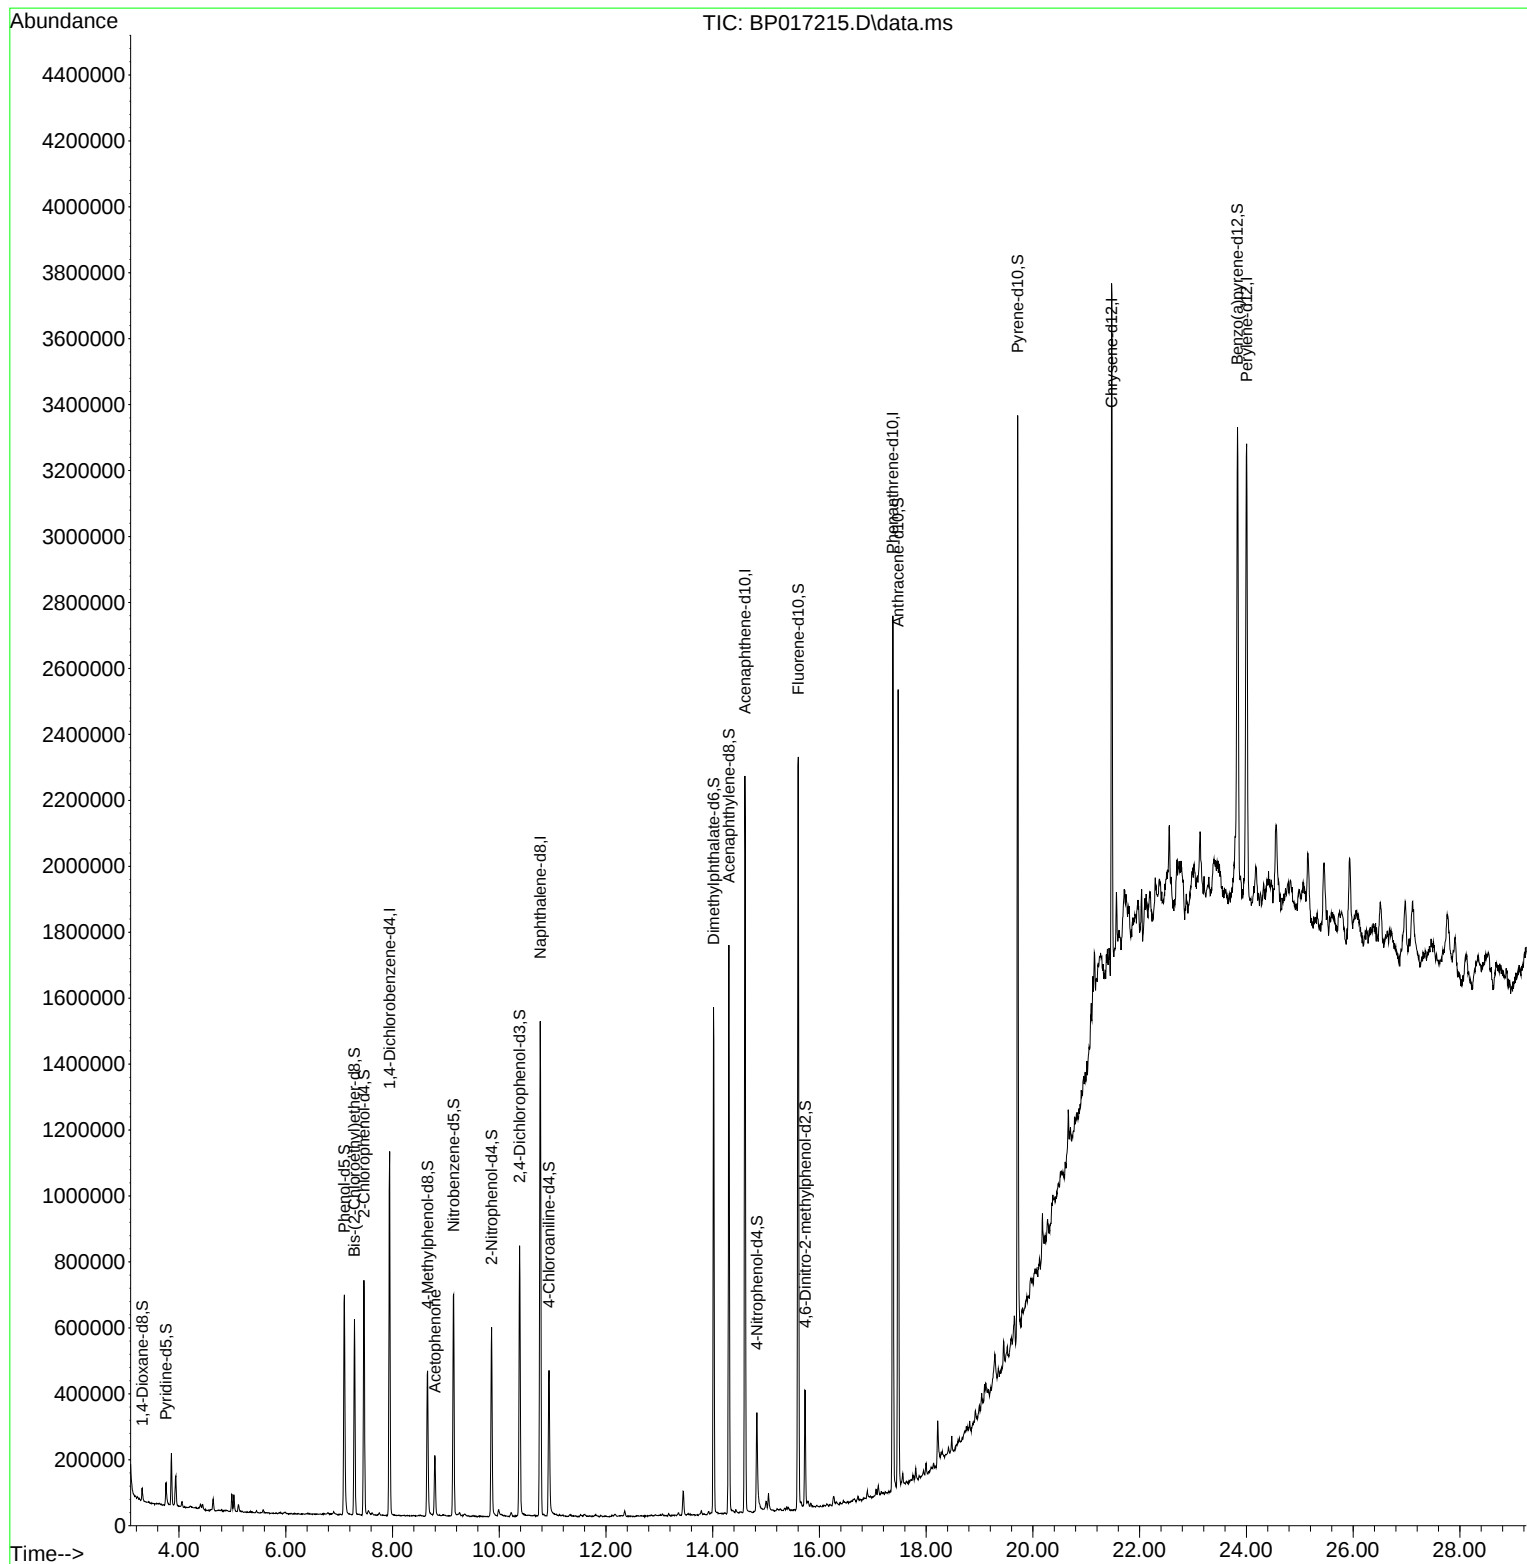

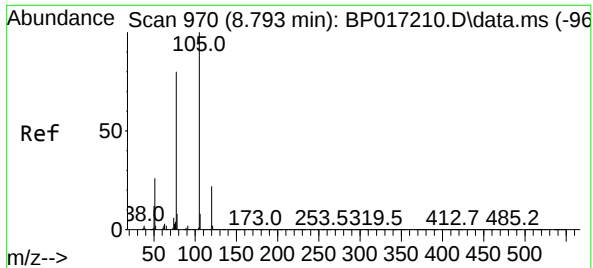

#16
 Acetophenone
 Concen: 3.171 ng/ul
 RT: 8.793 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP017215.D
 Acq: 18 Sep 2023 20:51

Instrument :
 BNA_P
 ClientSampleId :
 EZYW7

Tgt Ion:	105	Resp:	94730
Ion	Ratio	Lower	Upper
105	100		
77	81.5	63.0	94.4
51	27.0	20.5	30.7

