

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017216.D
 Acq On : 18 Sep 2023 21:25
 Operator : MA/JU
 Sample : 04330-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF9

Quant Time: Sep 18 23:55:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 16 03:18:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	294605	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	1229606	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.604	164	758271	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.375	188	1643353	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	1106913	20.000	ng/u1	0.00
88) Perylene-d12	24.004	264	1129428	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	17408	2.483	ng/uL	0.00
4) Pyridine-d5	3.758	84	23027	1.148	ng/u1	0.01
7) Phenol-d5	7.099	99	322860	13.478	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	214909	14.353	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	270239	14.141	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	130712	6.584	ng/u1	0.00
21) Nitrobenzene-d5	9.140	128	133376	15.491	ng/u1	0.00
24) 2-Nitrophenol-d4	9.857	143	136954	14.899	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	249259	14.022	ng/u1	0.00
31) 4-Chloroaniline-d4	10.934	131	242517	9.051	ng/u1	0.00
46) Dimethylphthalate-d6	14.016	166	849960	15.752	ng/u1	0.00
49) Acenaphthylene-d8	14.304	160	956714	15.625	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	49964	4.791	ng/u1	0.00
60) Fluorene-d10	15.604	176	777579	16.666	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.734	200	36061	3.928	ng/u1	0.00
73) Anthracene-d10	17.475	188	1154473	16.534	ng/u1	0.00
81) Pyrene-d10	19.716	212	1328016	22.876	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.839	264	929930	17.445	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.793	105	79987	2.574	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017216.D
Acq On : 18 Sep 2023 21:25
Operator : MA/JU
Sample : 04330-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF9

Quant Time: Sep 18 23:55:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 16 03:18:48 2023
Response via : Initial Calibration

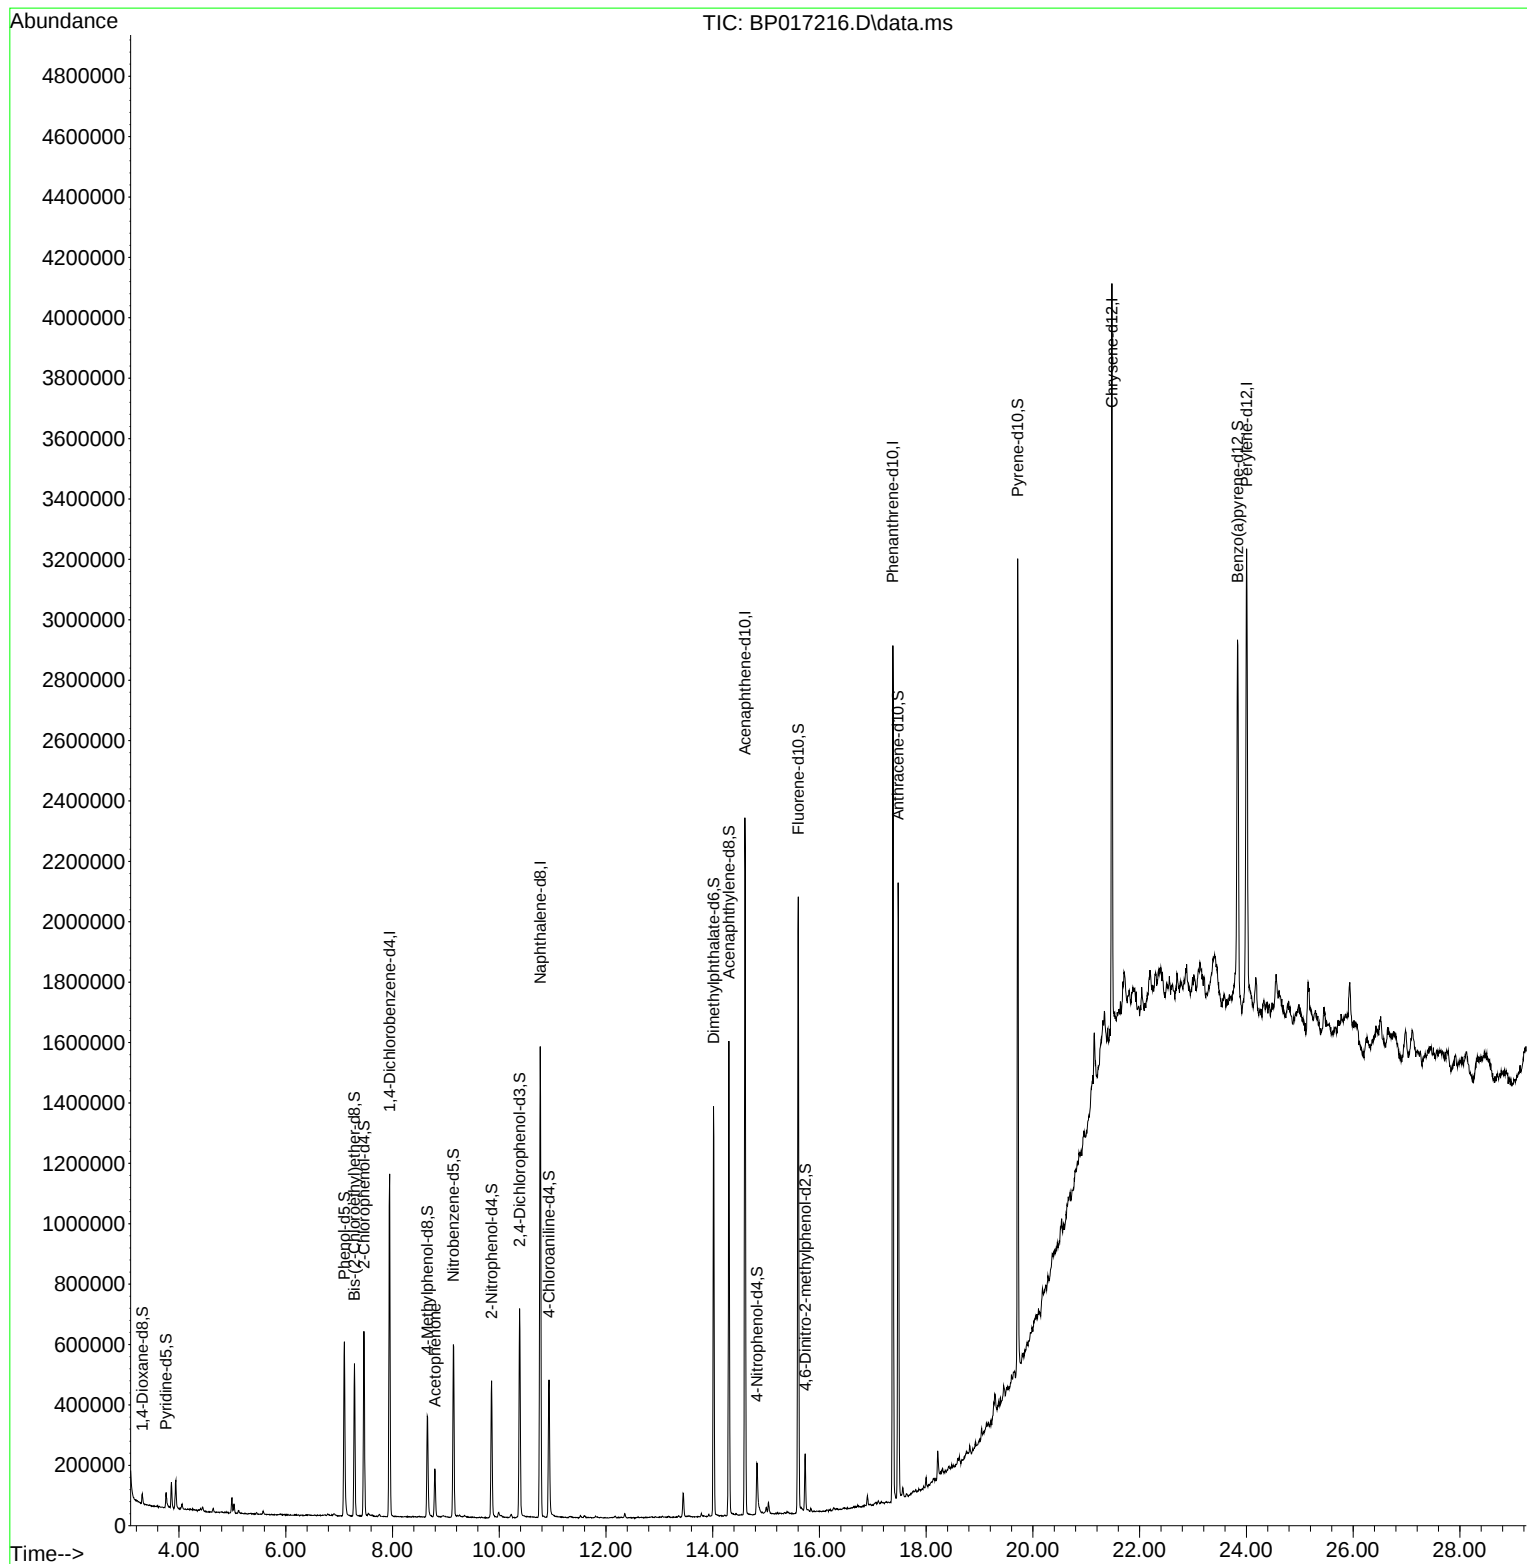

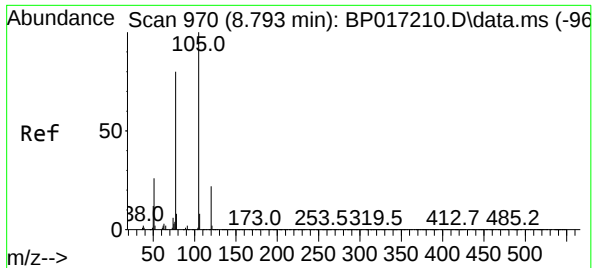

#16

Acetophenone

Concen: 2.574 ng/ul

RT: 8.793 min Scan# 91

Delta R.T. -0.006 min

Lab File: BP017216.D

Acq: 18 Sep 2023 21:25

Instrument :
BNA_P
ClientSampleId :
EZYF9

Tgt Ion:	105	Resp:	79987
Ion Ratio	Lower	Upper	
105	100		
77	83.3	63.0	94.4
51	28.1	20.5	30.7

