

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017220.D
 Acq On : 18 Sep 2023 23:42
 Operator : MA/JU
 Sample : 04330-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF8

Quant Time: Sep 19 01:02:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 16 03:18:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	302904	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	1156485	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.604	164	594253	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.375	188	1109550	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	1028456	20.000	ng/u1	0.00
88) Perylene-d12	24.004	264	1290079	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	19280	2.675	ng/uL	0.00
4) Pyridine-d5	3.764	84	14948	0.725	ng/u1	0.02
7) Phenol-d5	7.099	99	347541	14.110	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	232061	15.074	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	293337	14.929	ng/u1	0.00
15) 4-Methylphenol-d8	8.657	113	169521	8.305	ng/u1	0.00
21) Nitrobenzene-d5	9.146	128	142057	17.542	ng/u1	0.00
24) 2-Nitrophenol-d4	9.857	143	147091	17.014	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	246872	14.765	ng/u1	0.00
31) 4-Chloroaniline-d4	10.934	131	223024	8.850	ng/u1	0.00
46) Dimethylphthalate-d6	14.016	166	774579	18.317	ng/u1	0.00
49) Acenaphthylene-d8	14.304	160	821882	17.128	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	54165	6.627	ng/u1	0.00
60) Fluorene-d10	15.604	176	647222	17.701	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.734	200	26877	4.336	ng/u1	0.00
73) Anthracene-d10	17.475	188	957684	20.315	ng/u1	0.00
81) Pyrene-d10	19.716	212	1134573	21.035	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.839	264	1242595	20.407	ng/u1	0.00
Target Compounds						
16) Acetophenone	8.799	105	90559	2.834	ng/u1	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017220.D
Acq On : 18 Sep 2023 23:42
Operator : MA/JU
Sample : 04330-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF8

Quant Time: Sep 19 01:02:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 16 03:18:48 2023
Response via : Initial Calibration

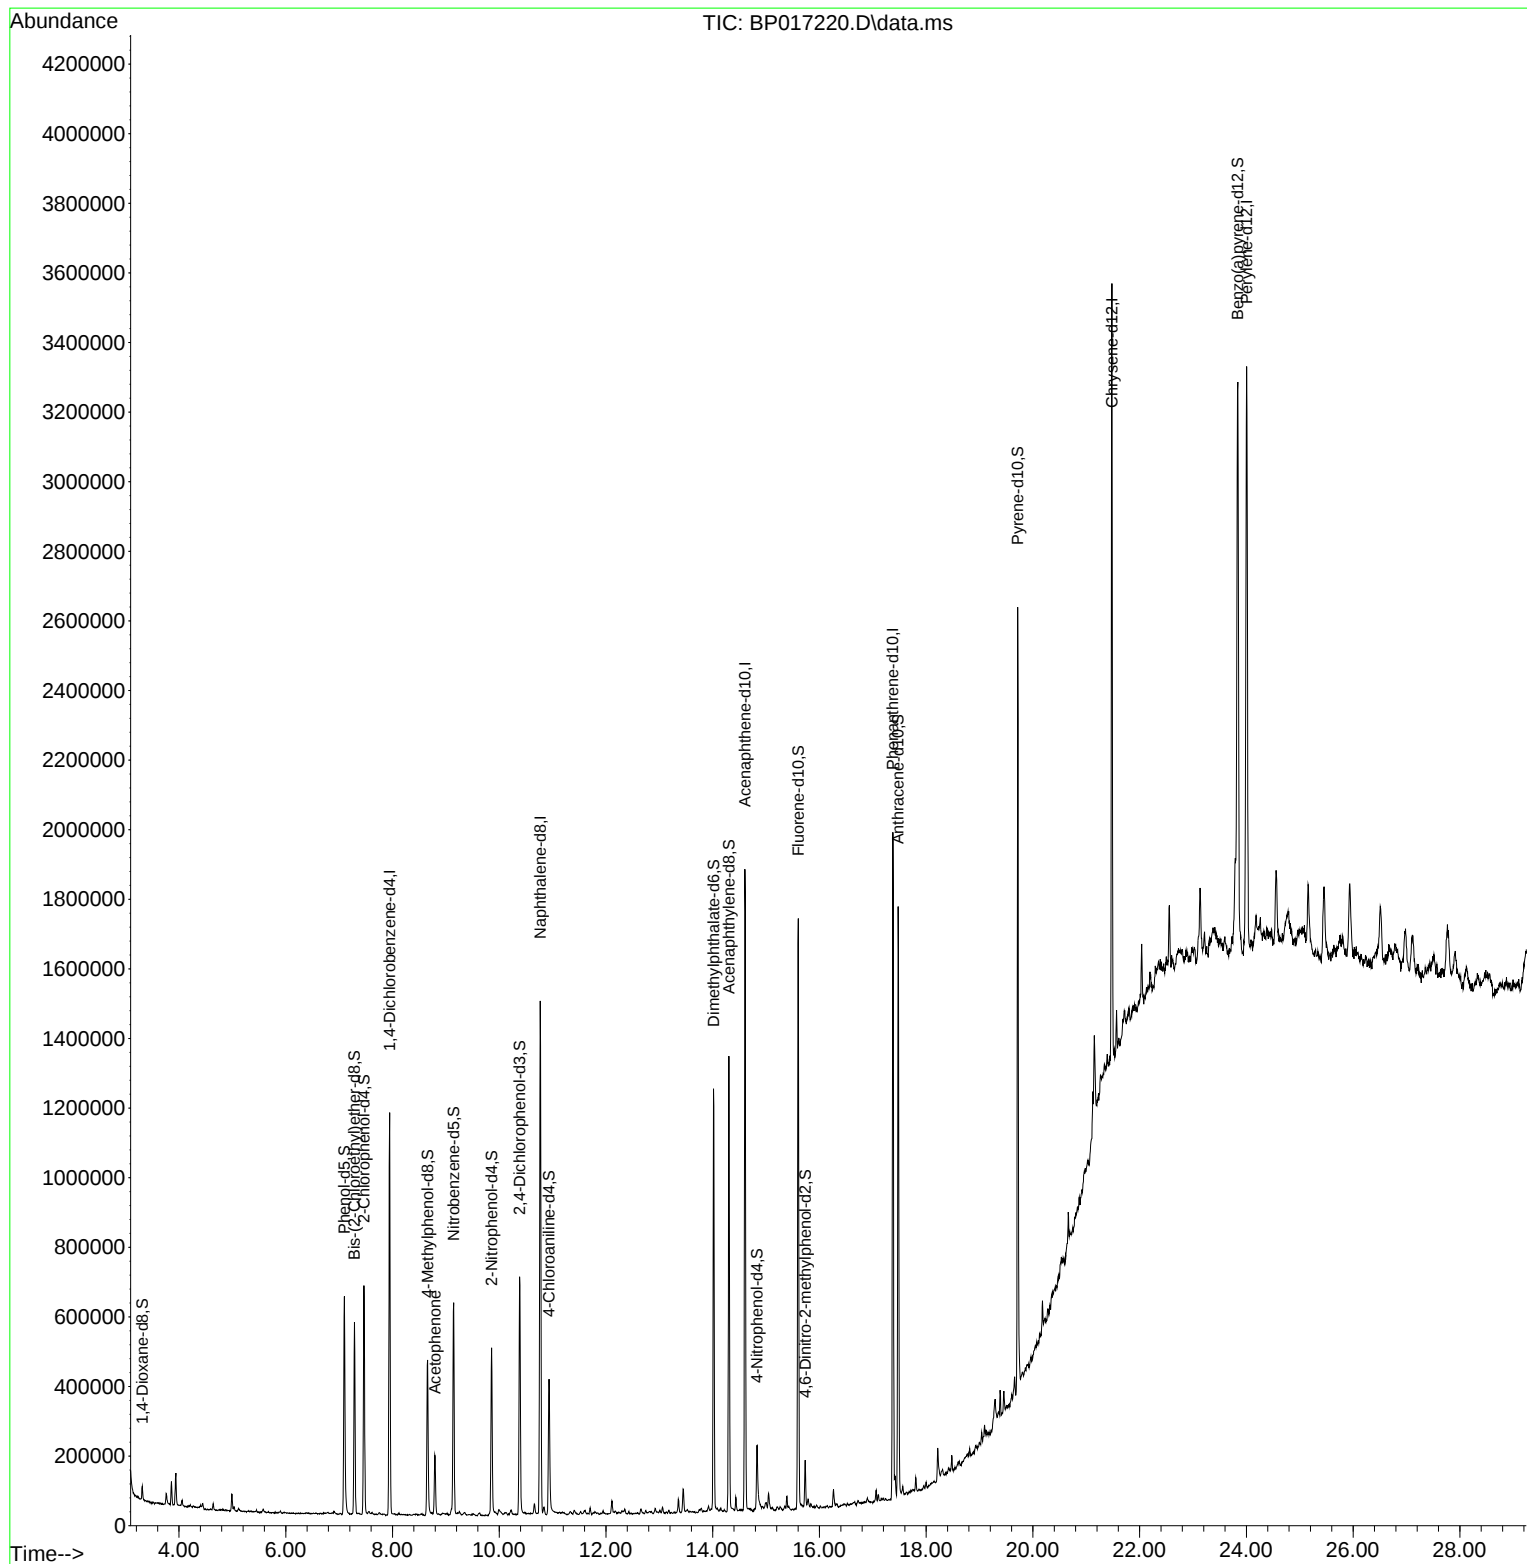

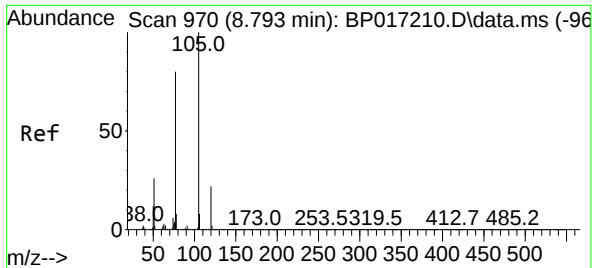

#16
 Acetophenone
 Concen: 2.834 ng/ul
 RT: 8.799 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BP017220.D
 Acq: 18 Sep 2023 23:42

Instrument :
 BNA_P
 ClientSampleId :
 EZYF8

Tgt Ion:	105	Resp:	90559
Ion	Ratio	Lower	Upper
105	100		
77	82.0	63.0	94.4
51	26.9	20.5	30.7

