

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017225.D
 Acq On : 19 Sep 2023 02:32
 Operator : MA/JU
 Sample : 04332-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE4

Quant Time: Sep 19 03:26:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 16 03:18:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	194852	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	740843	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.604	164	407369	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.375	188	892177	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	913578	20.000	ng/u1	0.00
88) Perylene-d12	24.004	264	1099266	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	14603	3.149	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.099	99	227513	14.360	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	150161	15.163	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	196032	15.509	ng/u1	0.00
15) 4-Methylphenol-d8	8.657	113	153608	11.698	ng/u1	0.00
21) Nitrobenzene-d5	9.146	128	91025	17.547	ng/u1	0.00
24) 2-Nitrophenol-d4	9.857	143	92667	16.732	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	160341	14.970	ng/u1	0.00
31) 4-Chloroaniline-d4	10.934	131	108417	6.716	ng/u1	0.00
46) Dimethylphthalate-d6	14.016	166	439744	15.169	ng/u1	0.00
49) Acenaphthylene-d8	14.304	160	529759	16.105	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	32415	5.785	ng/u1	0.00
60) Fluorene-d10	15.598	176	399608	15.942	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	29969	6.012	ng/u1	0.00
73) Anthracene-d10	17.475	188	642478	16.949	ng/u1	0.00
81) Pyrene-d10	19.716	212	802241	16.744	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	846316	16.312	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.793	105	73680	3.585	ng/u1#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017225.D
Acq On : 19 Sep 2023 02:32
Operator : MA/JU
Sample : 04332-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE4

Quant Time: Sep 19 03:26:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 16 03:18:48 2023
Response via : Initial Calibration

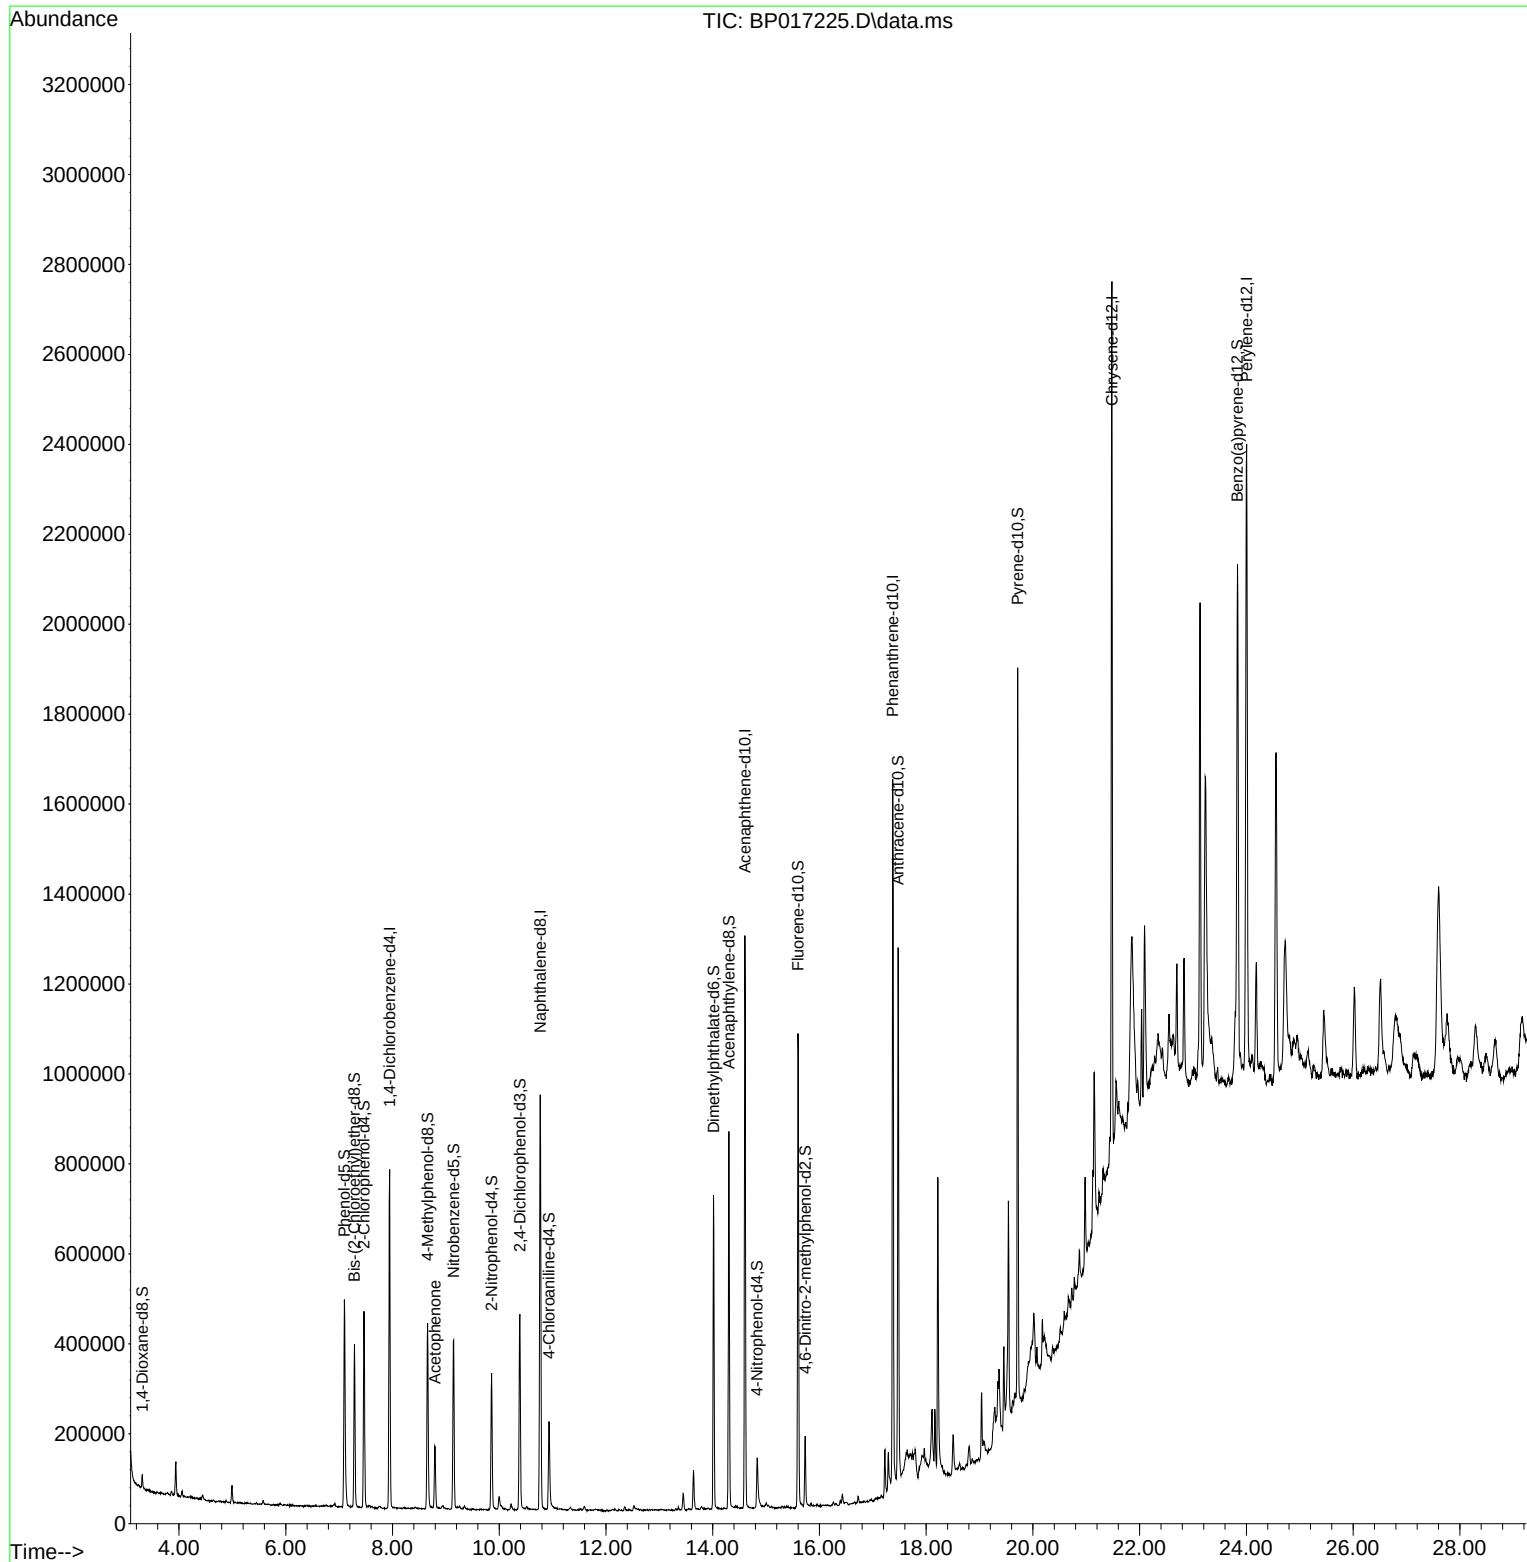

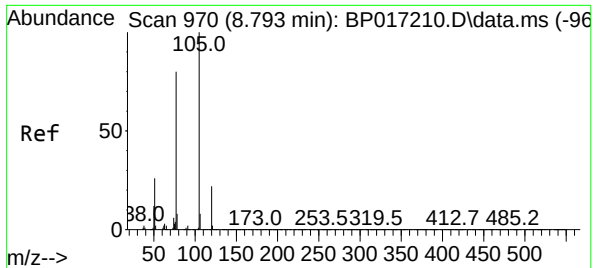

#16
 Acetophenone
 Concen: 3.585 ng/ul
 RT: 8.793 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP017225.D
 Acq: 19 Sep 2023 02:32

Instrument :
 BNA_P
 ClientSampleId :
 C0AE4

Tgt Ion:	105	Resp:	73680
Ion Ratio	Lower	Upper	
105	100		
77	80.2	63.0	94.4
51	30.8	20.5	30.7#

