

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017198.D
 Acq On : 18 Sep 2023 11:06
 Operator : MA/JU
 Sample : PB155449BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK449

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	33	37	44	rVB	58350	73175	1.62%	0.157%
2	3.740	107	111	129	rBV	706622	1068856	23.62%	2.299%
3	4.052	160	164	168	rBV3	12804	16663	0.37%	0.036%
4	6.281	537	543	544	rBV6	3015	5207	0.12%	0.011%
5	7.093	674	681	691	rBV	831113	1272924	28.13%	2.737%
6	7.281	707	713	725	rVB	684200	1064975	23.54%	2.290%
7	7.464	737	744	758	rBV	817493	1291321	28.54%	2.777%
8	7.940	818	825	835	rBV	705512	1087564	24.04%	2.339%
9	8.652	938	946	963	rBV	987533	1584909	35.03%	3.408%
10	9.140	1022	1029	1039	rBV	782152	1253917	27.71%	2.697%
11	9.858	1143	1151	1164	rBV	610712	1014543	22.42%	2.182%
12	10.381	1231	1240	1254	rBV	932072	1595280	35.26%	3.431%
13	10.769	1298	1306	1314	rBV	963369	1591792	35.18%	3.423%
14	10.928	1324	1333	1348	rBV	1000600	1711467	37.83%	3.681%
15	11.822	1477	1485	1486	rBV7	4442	9246	0.20%	0.020%
16	12.352	1569	1575	1584	rVB3	16365	33287	0.74%	0.072%
17	13.446	1757	1761	1765	rBV6	4747	7200	0.16%	0.015%
18	13.563	1777	1781	1785	rBV6	4070	7126	0.16%	0.015%
19	14.016	1852	1858	1868	rBV	1856330	2513258	55.55%	5.405%
20	14.304	1900	1907	1922	rBV	2027209	2855892	63.12%	6.142%
21	14.463	1931	1934	1940	rVB8	2877	5321	0.12%	0.011%
22	14.604	1949	1958	1966	rBV	1534226	2143546	47.38%	4.610%
23	14.822	1988	1995	2010	rBV	548654	973794	21.52%	2.094%
24	15.598	2121	2127	2143	rBV	2548102	3726541	82.36%	8.014%
25	15.728	2143	2149	2163	rVV	617715	826494	18.27%	1.777%
26	15.840	2164	2168	2174	rVB3	12207	20037	0.44%	0.043%
27	16.663	2305	2308	2313	rVB7	2905	4771	0.11%	0.010%
28	17.040	2369	2372	2377	rVB7	5089	6818	0.15%	0.015%
29	17.375	2422	2429	2437	rBV	1881918	2559039	56.56%	5.503%
30	17.475	2440	2446	2463	rVV	2922924	4064513	89.83%	8.741%
31	19.286	2750	2754	2759	rBV2	29705	44253	0.98%	0.095%
32	19.357	2762	2766	2771	rVV2	27811	44742	0.99%	0.096%
33	19.716	2821	2827	2837	rBV	3615883	4524450	100.00%	9.730%
34	21.475	3121	3126	3136	rBV	1636895	2205264	48.74%	4.742%
35	23.833	3520	3527	3541	rVB2	1623224	3273386	72.35%	7.039%
36	23.998	3549	3555	3569	rVB	984767	2018741	44.62%	4.341%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017198.D
Acq On : 18 Sep 2023 11:06
Operator : MA/JU
Sample : PB155449BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK449

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 46500312

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017198.D
Acq On : 18 Sep 2023 11:06
Operator : MA/JU
Sample : PB155449BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK449

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

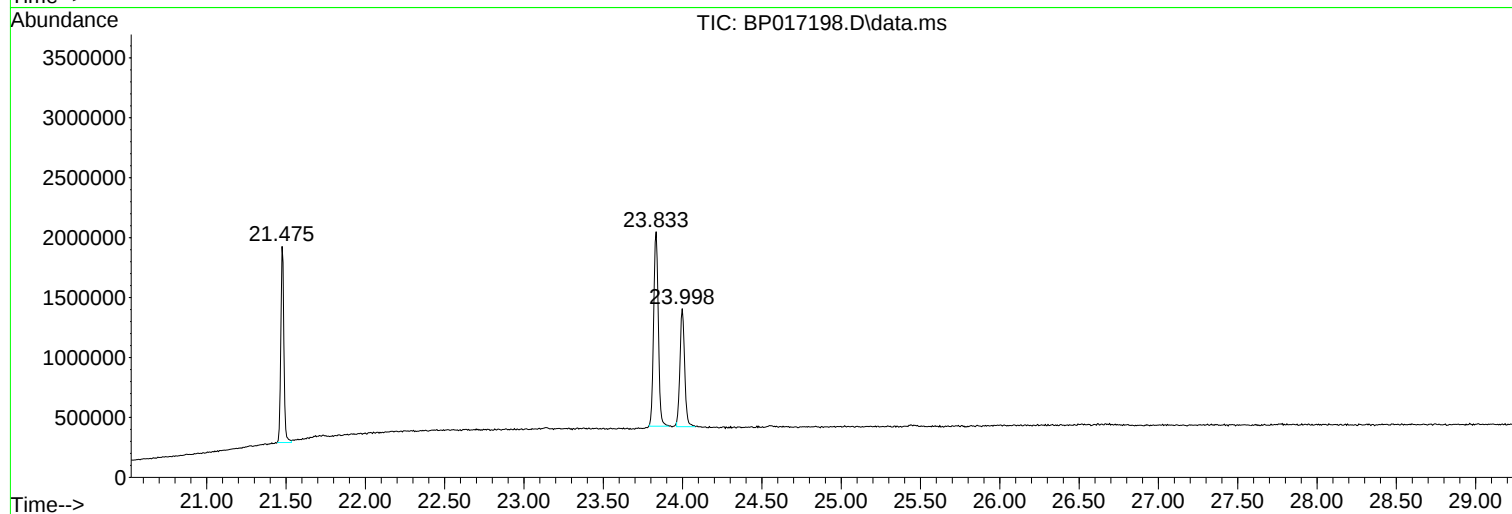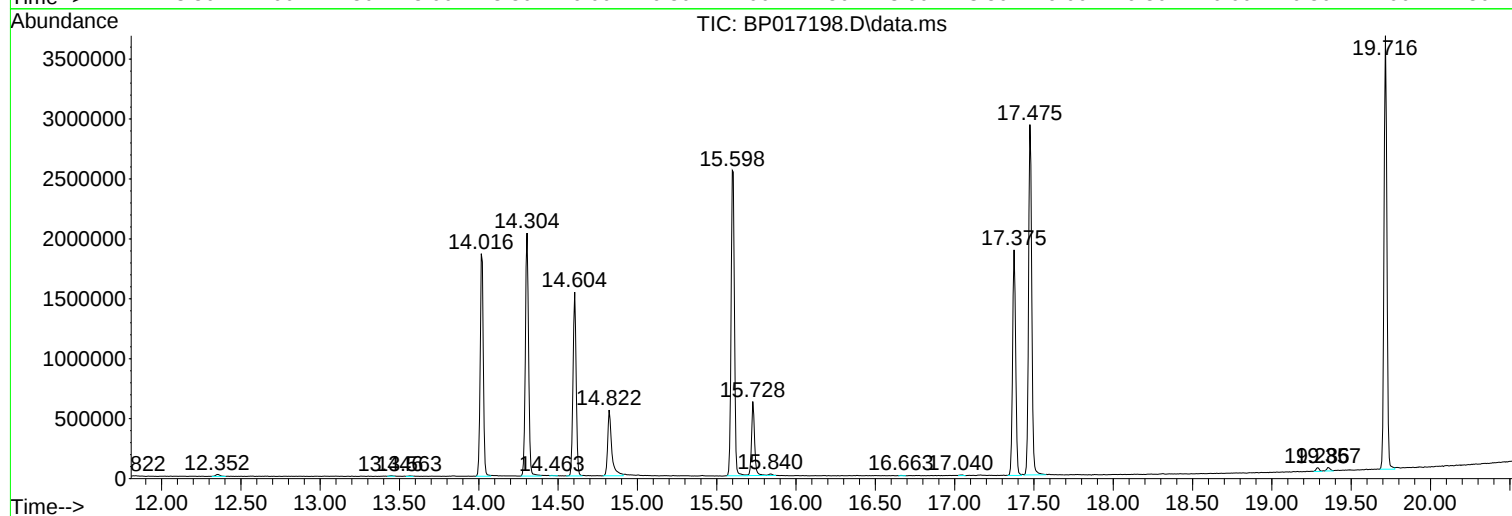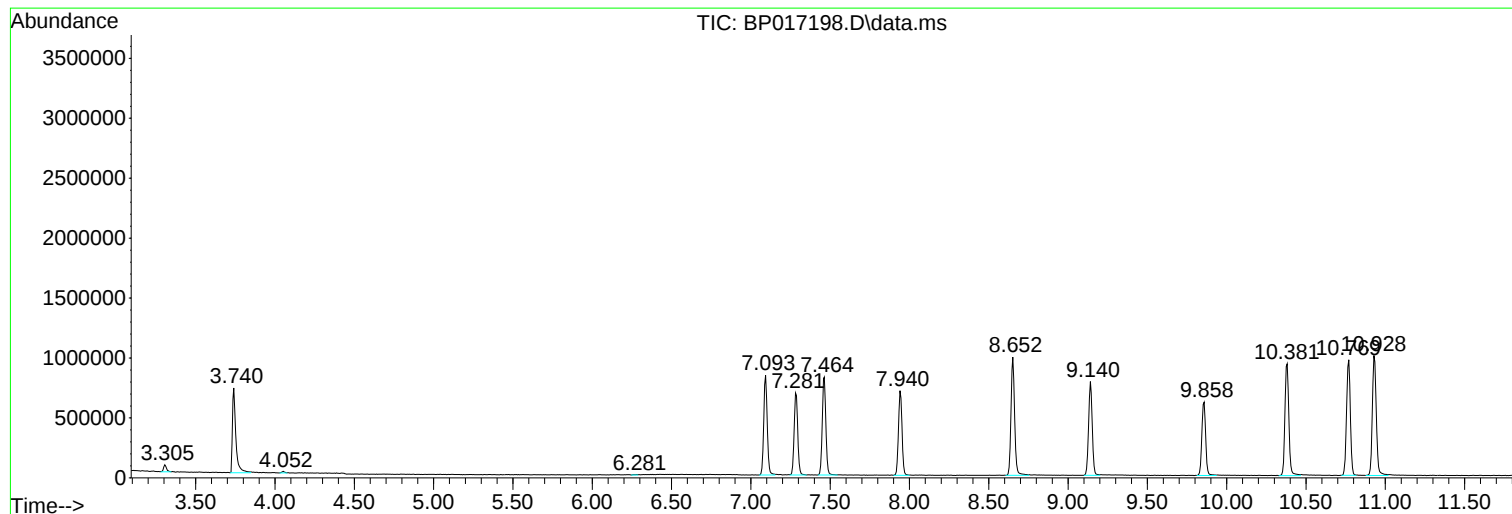

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017198.D
Acq On : 18 Sep 2023 11:06
Operator : MA/JU
Sample : PB155449BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK449

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017198.D
Acq On : 18 Sep 2023 11:06
Operator : MA/JU
Sample : PB155449BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK449

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------