

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017202.D
 Acq On : 18 Sep 2023 13:24
 Operator : MA/JU
 Sample : 04330-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017202.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.310	34	38	42	rBV	27144	35153	1.00%	0.094%
2	3.758	111	114	127	rVB	34509	58003	1.64%	0.155%
3	3.852	128	130	135	rVB3	14202	18309	0.52%	0.049%
4	3.940	140	145	151	rBV	61122	88419	2.50%	0.237%
5	4.058	161	165	170	rVB	19974	28890	0.82%	0.077%
6	4.281	199	203	208	rVB	27865	37407	1.06%	0.100%
7	4.440	227	230	236	rVB7	12005	16962	0.48%	0.045%
8	4.581	252	254	257	rBV4	3961	5125	0.15%	0.014%
9	4.693	269	273	278	rVB	18296	22060	0.62%	0.059%
10	4.987	319	323	329	rBV	35455	50814	1.44%	0.136%
11	5.116	341	345	350	rBV7	5012	7978	0.23%	0.021%
12	5.240	363	366	370	rBV5	2670	5172	0.15%	0.014%
13	5.575	420	423	427	rVB	6230	9235	0.26%	0.025%
14	5.869	469	473	475	rBV5	6166	8660	0.25%	0.023%
15	6.704	611	615	616	rBV4	2905	4170	0.12%	0.011%
16	6.793	626	630	633	rBV5	4098	4379	0.12%	0.012%
17	7.093	674	681	695	rBV	407393	684036	19.38%	1.834%
18	7.287	706	714	722	rBV	403895	617491	17.49%	1.655%
19	7.463	737	744	753	rBV	357218	567933	16.09%	1.522%
20	7.551	755	759	767	rVV2	13737	30057	0.85%	0.081%
21	7.751	789	793	796	rBV3	5173	7103	0.20%	0.019%
22	7.946	818	826	837	rBV	694765	1084180	30.71%	2.906%
23	8.381	897	900	901	rBV3	4183	4837	0.14%	0.013%
24	8.651	937	946	956	rBV	438283	702545	19.90%	1.883%
25	8.793	963	970	980	rVB	91089	146683	4.16%	0.393%
26	9.140	1019	1029	1041	rBV	447268	744241	21.08%	1.995%
27	9.257	1047	1049	1054	rVB6	3609	5596	0.16%	0.015%
28	9.345	1063	1064	1069	rVB5	6308	7678	0.22%	0.021%
29	9.598	1105	1107	1111	rBV5	2405	4096	0.12%	0.011%
30	9.745	1129	1132	1136	rBV6	2944	4092	0.12%	0.011%
31	9.857	1140	1151	1158	rBV	186871	317678	9.00%	0.852%
32	9.987	1169	1173	1179	rBV5	7686	14923	0.42%	0.040%
33	10.104	1191	1193	1199	rVB7	2640	3900	0.11%	0.010%
34	10.222	1207	1213	1218	rVB8	8649	14933	0.42%	0.040%
35	10.381	1233	1240	1254	rBV	349094	594344	16.84%	1.593%
36	10.663	1284	1288	1292	rVB7	5869	8819	0.25%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017202.D
 Acq On : 18 Sep 2023 13:24
 Operator : MA/JU
 Sample : 04330-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	10.769	1298	1306	1313	rBV	976904	1584529	44.89%	4.248%
38	10.934	1325	1334	1347	rBV	492356	879229	24.91%	2.357%
39	11.075	1356	1358	1363	rVB6	3390	4617	0.13%	0.012%
40	11.316	1396	1399	1402	rBV4	3825	5675	0.16%	0.015%
41	11.522	1432	1434	1439	rVB5	4469	7564	0.21%	0.020%
42	11.704	1461	1465	1469	rBV7	3970	6115	0.17%	0.016%
43	11.804	1477	1482	1485	rBV6	2579	4752	0.13%	0.013%
44	11.845	1487	1489	1494	rVB6	4172	4961	0.14%	0.013%
45	12.110	1528	1534	1539	rBV5	8472	13489	0.38%	0.036%
46	12.357	1569	1576	1580	rBV4	10738	18603	0.53%	0.050%
47	12.428	1584	1588	1593	rBV8	4699	8981	0.25%	0.024%
48	12.745	1638	1642	1645	rVB6	2941	4093	0.12%	0.011%
49	12.857	1659	1661	1666	rVB6	3232	4496	0.13%	0.012%
50	12.922	1670	1672	1677	rVB6	4914	5950	0.17%	0.016%
51	13.057	1691	1695	1702	rBV9	7442	15213	0.43%	0.041%
52	13.357	1741	1746	1750	rBV	20861	28538	0.81%	0.077%
53	13.451	1755	1762	1779	rBV	1631762	2478172	70.21%	6.643%
54	13.557	1779	1780	1785	rVB5	5718	5725	0.16%	0.015%
55	13.786	1815	1819	1822	rVB6	5750	8658	0.25%	0.023%
56	13.839	1822	1828	1832	rBV9	3265	6554	0.19%	0.018%
57	13.922	1839	1842	1845	rVB4	5632	6348	0.18%	0.017%
58	14.016	1852	1858	1873	rBV	1113907	1516976	42.98%	4.066%
59	14.216	1889	1892	1896	rVB6	4631	6113	0.17%	0.016%
60	14.304	1899	1907	1918	rBV	1191387	1760325	49.87%	4.719%
61	14.433	1924	1929	1936	rVB2	23182	36429	1.03%	0.098%
62	14.604	1951	1958	1967	rBV	1471851	2154381	61.03%	5.775%
63	14.980	2019	2022	2023	rBV3	4822	4114	0.12%	0.011%
64	14.998	2023	2025	2028	rVV4	5652	7980	0.23%	0.021%
65	15.045	2030	2033	2042	rVB10	15233	27918	0.79%	0.075%
66	15.351	2079	2085	2086	rBV6	6403	8990	0.25%	0.024%
67	15.392	2087	2092	2100	rVV2	26988	37579	1.06%	0.101%
68	15.598	2120	2127	2145	rBV	1676084	2384247	67.55%	6.391%
69	15.792	2155	2160	2164	rVB6	11841	21868	0.62%	0.059%
70	15.839	2164	2168	2172	rVB5	7026	10855	0.31%	0.029%
71	15.945	2182	2186	2188	rBV5	7240	7908	0.22%	0.021%
72	16.022	2195	2199	2202	rVB5	7607	9827	0.28%	0.026%
73	16.198	2225	2229	2231	rBV5	4168	5822	0.16%	0.016%
74	16.263	2235	2240	2246	rVV	51367	84879	2.40%	0.228%
75	16.322	2248	2250	2254	rVB4	8679	9157	0.26%	0.025%
76	16.427	2263	2268	2273	rBV2	14336	31971	0.91%	0.086%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017202.D
 Acq On : 18 Sep 2023 13:24
 Operator : MA/JU
 Sample : 04330-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

77	16.604	2294	2298	2306	rBV	28876	55367	1.57%	0.148%
78	16.722	2313	2318	2323	rBV2	25126	44251	1.25%	0.119%
79	16.892	2343	2347	2353	rBV4	30560	49899	1.41%	0.134%
80	17.057	2372	2375	2379	rBV	32381	37542	1.06%	0.101%
81	17.104	2379	2383	2386	rVB3	20255	28023	0.79%	0.075%
82	17.374	2422	2429	2434	rBV	1929714	2705148	76.64%	7.252%
83	17.416	2434	2436	2440	rVV	74847	88575	2.51%	0.237%
84	17.474	2440	2446	2457	rVV	1673815	2393821	67.82%	6.417%
85	17.804	2498	2502	2508	rVB2	47892	59655	1.69%	0.160%
86	17.998	2531	2535	2539	rBV2	30735	38769	1.10%	0.104%
87	18.216	2568	2572	2579	rBV2	116229	195408	5.54%	0.524%
88	18.480	2614	2617	2622	rVB	39899	47926	1.36%	0.128%
89	19.039	2709	2712	2714	rBV3	26789	30534	0.87%	0.082%
90	19.092	2718	2721	2724	rBV3	43027	67757	1.92%	0.182%
91	19.133	2724	2728	2731	rVB	170549	194079	5.50%	0.520%
92	19.257	2747	2749	2750	rBV2	31424	23126	0.66%	0.062%
93	19.351	2761	2765	2767	rBV	163654	181095	5.13%	0.485%
94	19.380	2767	2770	2775	rVB	205844	261247	7.40%	0.700%
95	19.451	2779	2782	2787	rBV4	53172	64696	1.83%	0.173%
96	19.710	2821	2826	2836	rBV	2533916	3529824	100.00%	9.462%
97	20.174	2903	2905	2910	rVB3	53758	51326	1.45%	0.138%
98	21.474	3121	3126	3131	rBV	2092264	2767267	78.40%	7.418%
99	23.827	3520	3526	3540	rVB2	1260537	2733332	77.44%	7.327%
100	23.992	3548	3554	3563	rVB	1191272	2460341	69.70%	6.595%




Sum of corrected areas: 37304510

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017202.D
Acq On : 18 Sep 2023 13:24
Operator : MA/JU
Sample : 04330-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

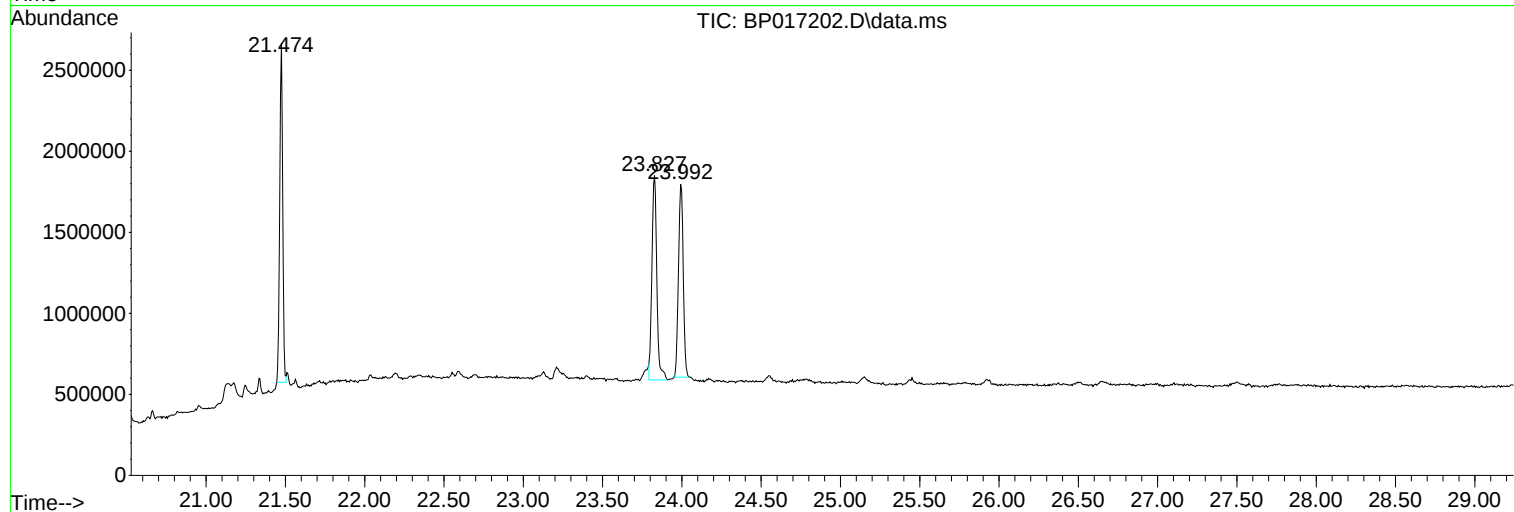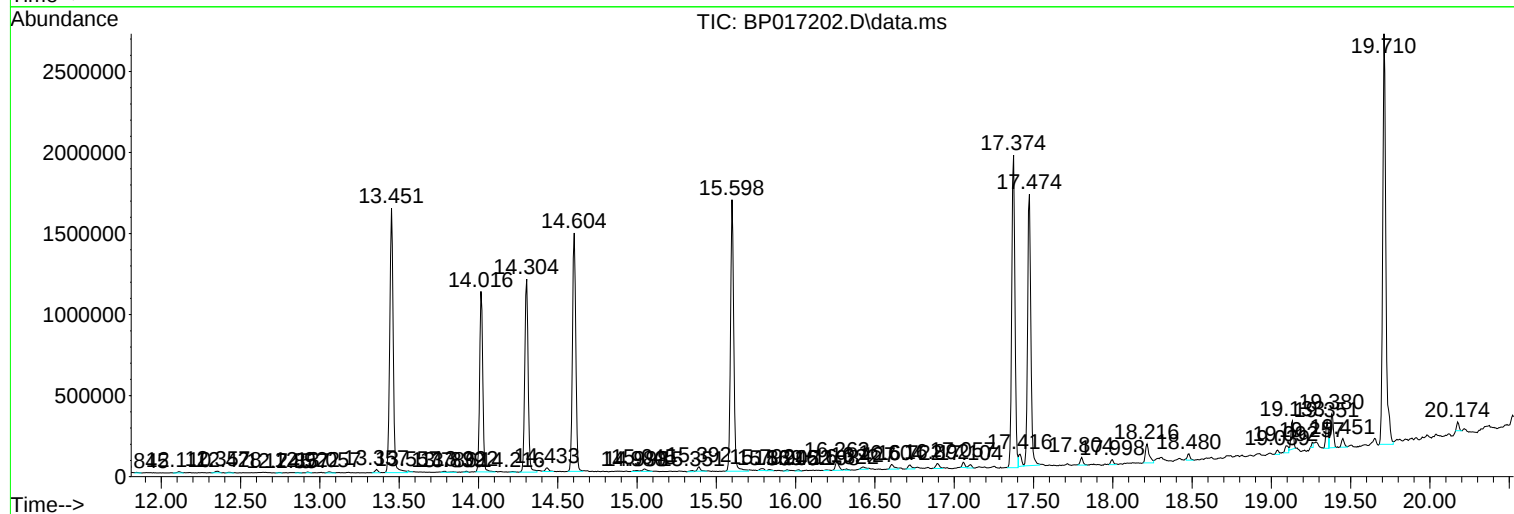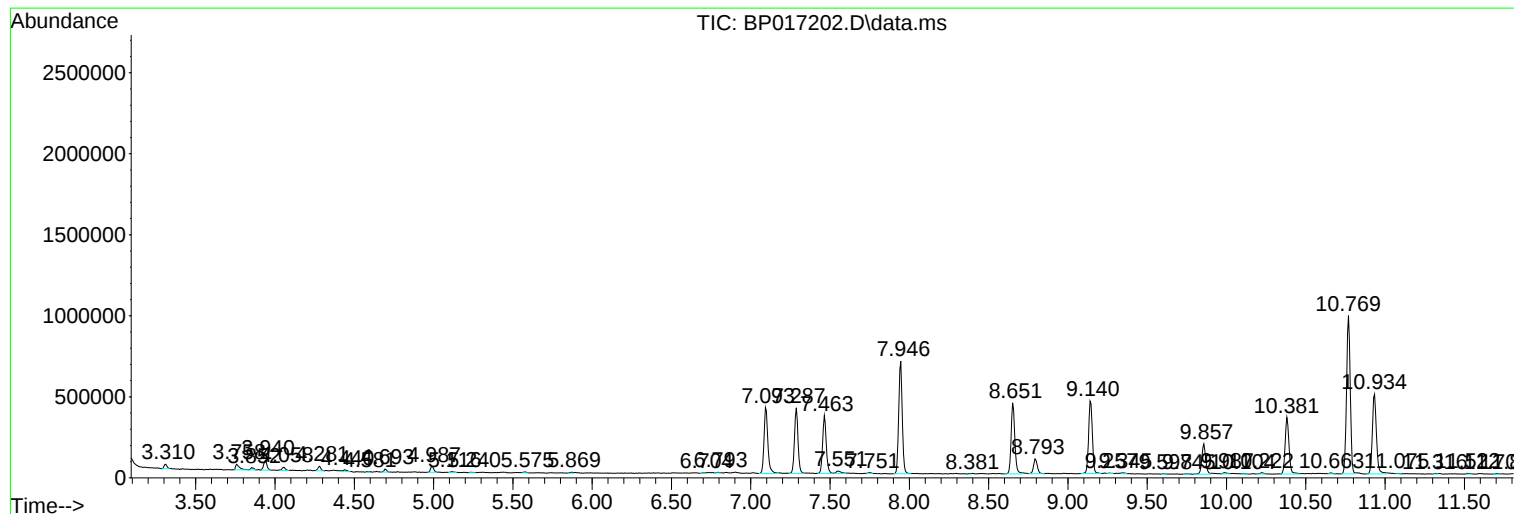

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017202.D
Acq On : 18 Sep 2023 13:24
Operator : MA/JU
Sample : 04330-21
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
EZY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2,4,7,9-Tetramethyl-5-decyn... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
13.451	23.01 ng/ul	2478170	Acenaphthene-d10		14.604	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2,4,7,9-Tetramethyl-5-decyn-4,7-...		226	C14H26O2	000126-86-3	91
2	2,4,7,9-Tetramethyl-5-decyn-4,7-...		226	C14H26O2	000126-86-3	90
3	Metacetamol		151	C8H9NO2	000621-42-1	59
4	Benzenamine, 4-propoxy-		151	C9H13NO	004469-80-1	59
5	Pyridine, 2-butyl-, 1-oxide		151	C9H13NO	031396-32-4	59

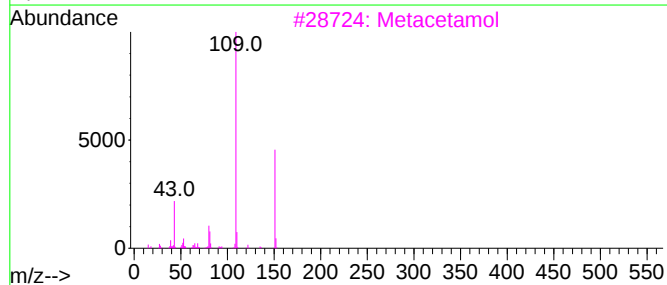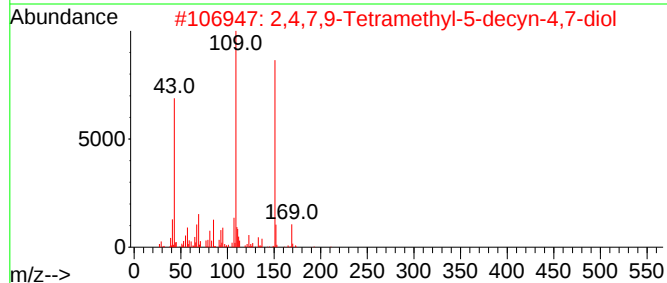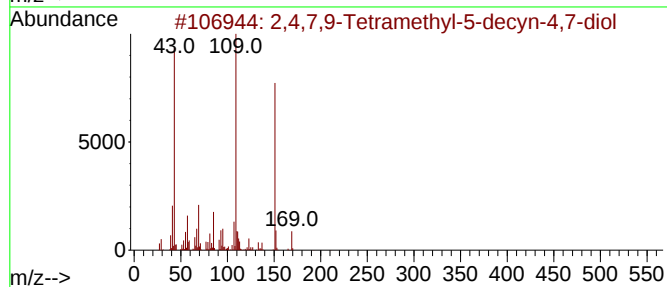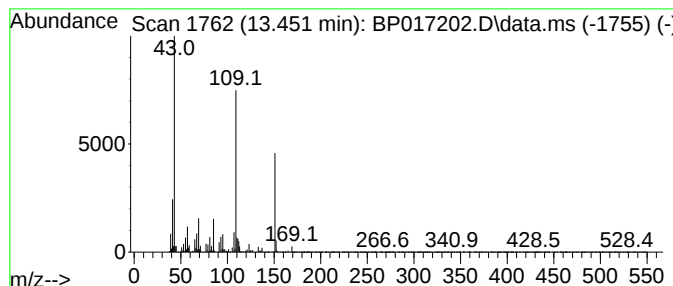

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017202.D
Acq On : 18 Sep 2023 13:24
Operator : MA/JU
Sample : 04330-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2,4,7,9-Tetrame...	13.451	23.0	ng/ul	2478170	3	14.604	2154380	20.0