

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017211.D
 Acq On : 18 Sep 2023 18:33
 Operator : MA/JU
 Sample : PB155579BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK579

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017211.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	34	37	46	rVB	70260	91039	1.70%	0.150%
2	3.740	108	111	131	rBV	948896	1395964	25.99%	2.296%
3	4.052	161	164	168	rBV	15161	18295	0.34%	0.030%
4	7.093	674	681	695	rBV	1099033	1702718	31.70%	2.801%
5	7.287	707	714	727	rVB	914382	1376081	25.62%	2.264%
6	7.464	737	744	759	rBV	1120833	1710530	31.85%	2.814%
7	7.946	817	826	835	rBV	982996	1559505	29.04%	2.565%
8	8.652	939	946	963	rBV	1318385	2105344	39.20%	3.463%
9	9.140	1022	1029	1039	rBV	1016253	1655104	30.82%	2.723%
10	9.858	1142	1151	1166	rBV	853141	1386603	25.82%	2.281%
11	10.381	1231	1240	1250	rBV	1266534	2115698	39.39%	3.480%
12	10.769	1297	1306	1315	rBV	1389180	2299241	42.81%	3.782%
13	10.928	1325	1333	1347	rBV	1289257	2235811	41.63%	3.678%
14	12.352	1569	1575	1581	rBV2	21493	36120	0.67%	0.059%
15	13.446	1757	1761	1765	rBV5	15174	22515	0.42%	0.037%
16	13.569	1777	1782	1786	rBV8	5230	10393	0.19%	0.017%
17	14.016	1850	1858	1870	rBV	2309697	3210569	59.78%	5.281%
18	14.099	1870	1872	1877	rVB6	3260	5650	0.11%	0.009%
19	14.304	1899	1907	1920	rBV	2665671	3763173	70.07%	6.190%
20	14.604	1951	1958	1969	rBV	2173009	3076791	57.29%	5.061%
21	14.822	1988	1995	2015	rBV	807583	1373309	25.57%	2.259%
22	15.598	2121	2127	2140	rBV	3314130	4725827	87.99%	7.774%
23	15.728	2143	2149	2164	rVV	940955	1214634	22.62%	1.998%
24	15.834	2164	2167	2174	rVB4	14801	24107	0.45%	0.040%
25	16.175	2220	2225	2230	rBV9	3932	9263	0.17%	0.015%
26	17.040	2368	2372	2376	rVB8	5550	9702	0.18%	0.016%
27	17.163	2386	2393	2398	rBV4	7074	15291	0.28%	0.025%
28	17.375	2422	2429	2439	rBV	2582248	3558369	66.25%	5.853%
29	17.475	2439	2446	2458	rBV	3678442	5060465	94.22%	8.324%
30	18.310	2585	2588	2591	rBV3	4607	5984	0.11%	0.010%
31	19.286	2750	2754	2758	rBV3	41381	54979	1.02%	0.090%
32	19.351	2761	2765	2770	rVV	33322	50462	0.94%	0.083%
33	19.716	2821	2827	2836	rBV	4230262	5370875	100.00%	8.835%
34	21.475	3121	3126	3136	rBV	2190074	2835464	52.79%	4.664%
35	23.833	3520	3527	3540	rVB2	1959982	4012220	74.70%	6.600%
36	23.998	3549	3555	3567	rVB	1321095	2694697	50.17%	4.433%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017211.D
Acq On : 18 Sep 2023 18:33
Operator : MA/JU
Sample : PB155579BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK579

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 60792792

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017211.D
Acq On : 18 Sep 2023 18:33
Operator : MA/JU
Sample : PB155579BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK579

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

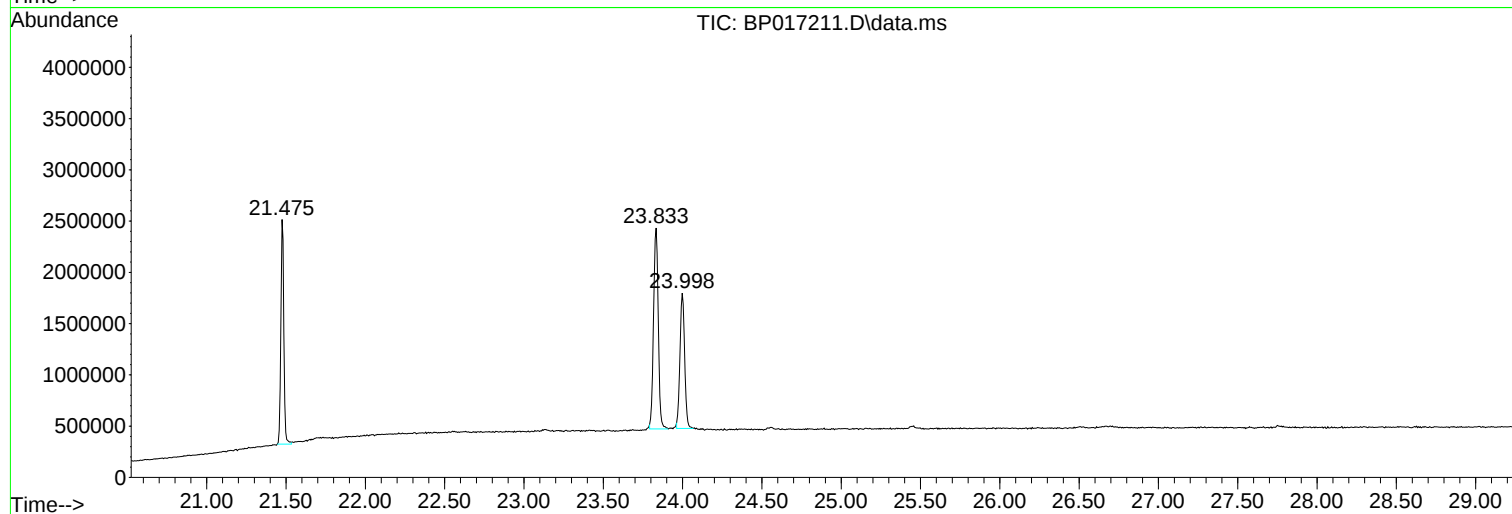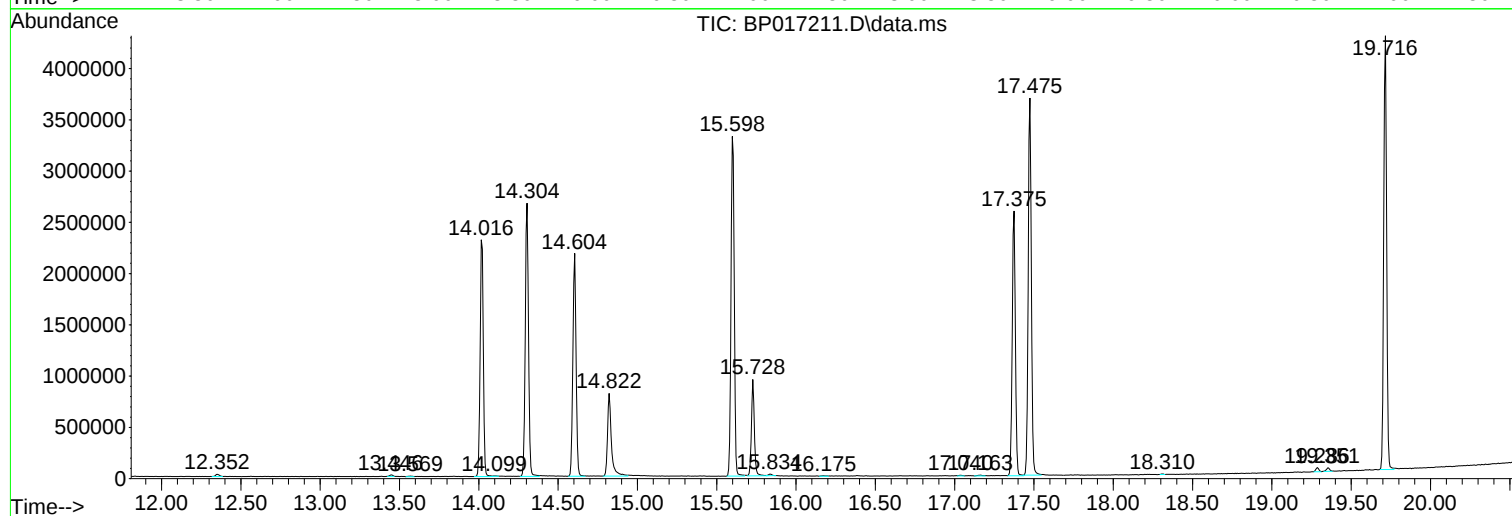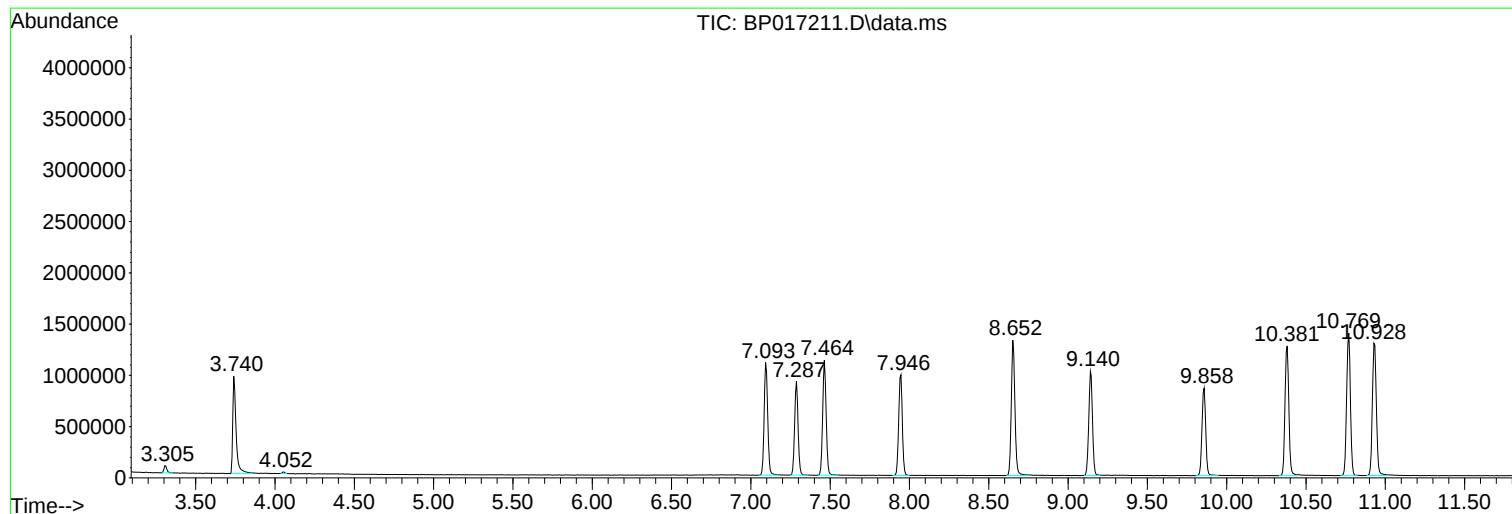

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017211.D
Acq On : 18 Sep 2023 18:33
Operator : MA/JU
Sample : PB155579BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK579

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017211.D
Acq On : 18 Sep 2023 18:33
Operator : MA/JU
Sample : PB155579BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK579

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------