

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017213.D
 Acq On : 18 Sep 2023 19:42
 Operator : MA/JU
 Sample : 04330-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	35	37	45	rVB	29138	42275	1.60%	0.160%
2	3.758	111	114	119	rBV2	39952	51768	1.96%	0.196%
3	3.858	127	131	139	rVB	66686	91467	3.47%	0.346%
4	3.940	140	145	150	rVB	74303	116011	4.40%	0.439%
5	4.052	162	164	170	rVB2	15465	21027	0.80%	0.079%
6	4.640	260	264	269	rBV3	12500	17680	0.67%	0.067%
7	4.993	319	324	327	rBV	41244	58814	2.23%	0.222%
8	5.111	341	344	349	rVB6	8754	13662	0.52%	0.052%
9	5.452	399	402	407	rVB5	6181	9437	0.36%	0.036%
10	5.570	420	422	429	rVB	6886	11575	0.44%	0.044%
11	7.093	675	681	695	rBV	422805	728084	27.61%	2.753%
12	7.287	708	714	723	rBV	382083	580422	22.01%	2.194%
13	7.464	738	744	754	rBV	457527	733482	27.81%	2.773%
14	7.552	756	759	760	rBV3	5783	7348	0.28%	0.028%
15	7.758	790	794	800	rBV5	6684	11050	0.42%	0.042%
16	7.946	818	826	834	rBV	1031220	1596191	60.53%	6.034%
17	8.652	940	946	957	rBV	285866	496454	18.82%	1.877%
18	8.793	963	970	980	rVB	151932	247635	9.39%	0.936%
19	9.140	1018	1029	1038	rBV	417380	704329	26.71%	2.663%
20	9.258	1046	1049	1054	rVB7	6088	9788	0.37%	0.037%
21	9.858	1141	1151	1162	rBV	340322	579892	21.99%	2.192%
22	9.987	1166	1173	1177	rBV3	14251	27653	1.05%	0.105%
23	10.222	1207	1213	1218	rBV2	10264	18236	0.69%	0.069%
24	10.381	1233	1240	1250	rBV	474880	804028	30.49%	3.040%
25	10.658	1281	1287	1293	rVB7	7856	15644	0.59%	0.059%
26	10.769	1298	1306	1314	rBV	1401959	2258201	85.63%	8.537%
27	10.840	1314	1318	1324	rVB6	10618	18504	0.70%	0.070%
28	10.934	1327	1334	1345	rBV	243966	473617	17.96%	1.791%
29	11.522	1431	1434	1438	rBV6	5097	8021	0.30%	0.030%
30	11.599	1440	1447	1455	rVV9	7941	21292	0.81%	0.080%
31	11.705	1459	1465	1470	rVB6	8913	15012	0.57%	0.057%
32	11.840	1486	1488	1493	rVB6	4813	8042	0.30%	0.030%
33	11.904	1493	1499	1504	rBV9	4384	9870	0.37%	0.037%
34	12.110	1529	1534	1540	rBV8	14588	24110	0.91%	0.091%
35	12.175	1540	1545	1550	rVV6	7844	15065	0.57%	0.057%
36	12.257	1554	1559	1563	rVV8	3776	8198	0.31%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017213.D
 Acq On : 18 Sep 2023 19:42
 Operator : MA/JU
 Sample : 04330-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	12.352	1572	1575	1580	rVB4	9487	14205	0.54%	0.054%
38	12.510	1599	1602	1607	rBV7	4750	7955	0.30%	0.030%
39	12.922	1666	1672	1676	rBV8	8164	17545	0.67%	0.066%
40	13.063	1692	1696	1700	rBV5	11146	15220	0.58%	0.058%
41	13.181	1713	1716	1721	rBV7	5609	8106	0.31%	0.031%
42	13.357	1741	1746	1752	rBV4	16032	30970	1.17%	0.117%
43	13.451	1756	1762	1767	rVV	58780	96758	3.67%	0.366%
44	14.016	1853	1858	1864	rBV	834794	1184805	44.93%	4.479%
45	14.304	1901	1907	1915	rBV	975710	1425218	54.04%	5.388%
46	14.434	1926	1929	1938	rVB4	25336	35007	1.33%	0.132%
47	14.604	1952	1958	1967	rBV	1835687	2637233	100.00%	9.970%
48	14.834	1992	1997	2011	rBV2	89344	213949	8.11%	0.809%
49	15.046	2031	2033	2043	rVB10	38950	71269	2.70%	0.269%
50	15.604	2122	2128	2136	rBV	1229689	1795387	68.08%	6.787%
51	15.734	2145	2150	2156	rBV	126696	205512	7.79%	0.777%
52	17.375	2424	2429	2435	rBV	1858944	2634088	99.88%	9.958%
53	17.475	2442	2446	2452	rVB	1139518	1573097	59.65%	5.947%
54	19.716	2823	2827	2831	rBV	1491186	2161578	81.96%	8.172%
55	21.480	3124	3127	3133	rVB	1954442	2469862	93.65%	9.337%




Sum of corrected areas: 26451648

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017213.D
Acq On : 18 Sep 2023 19:42
Operator : MA/JU
Sample : 04330-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

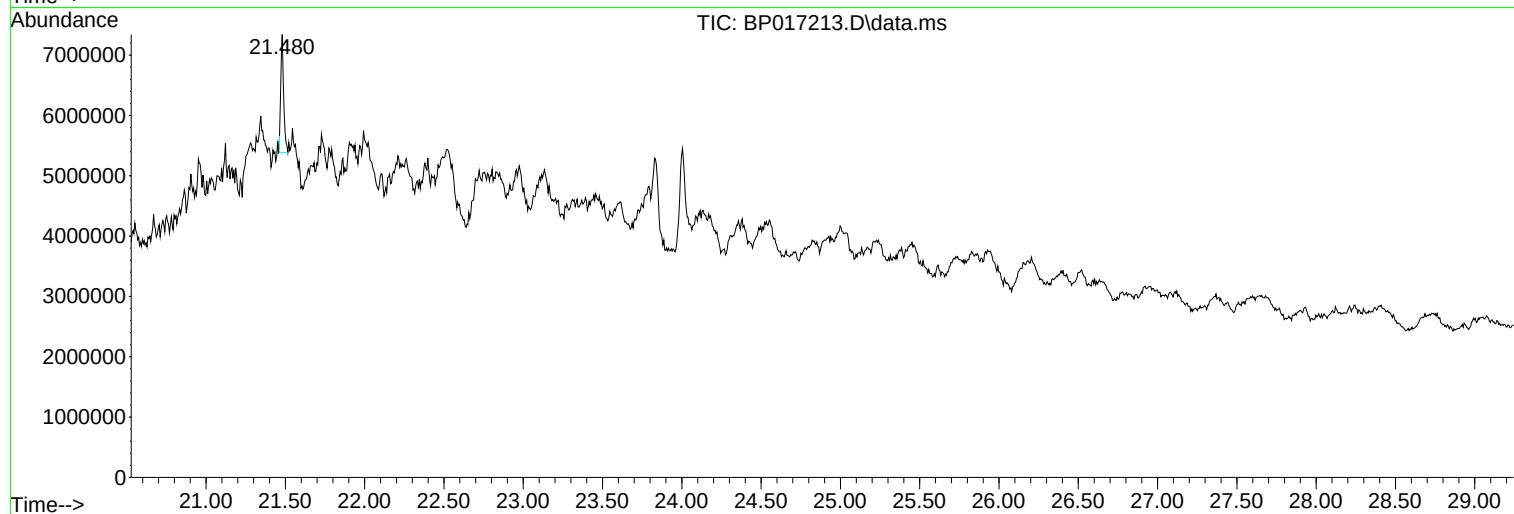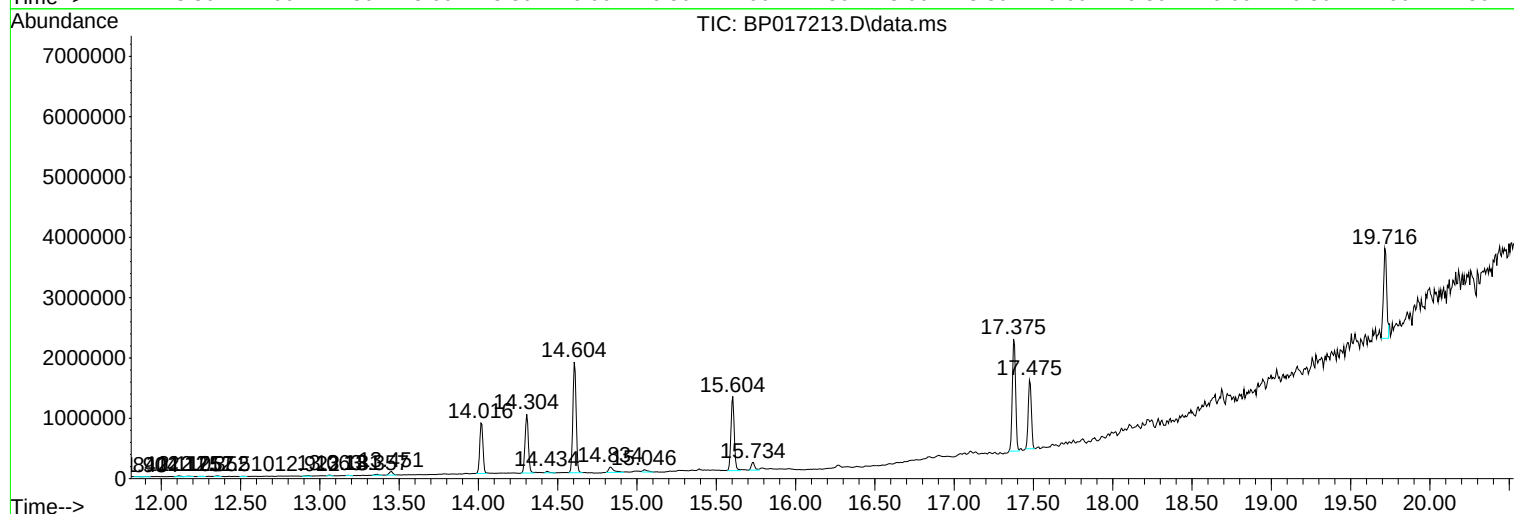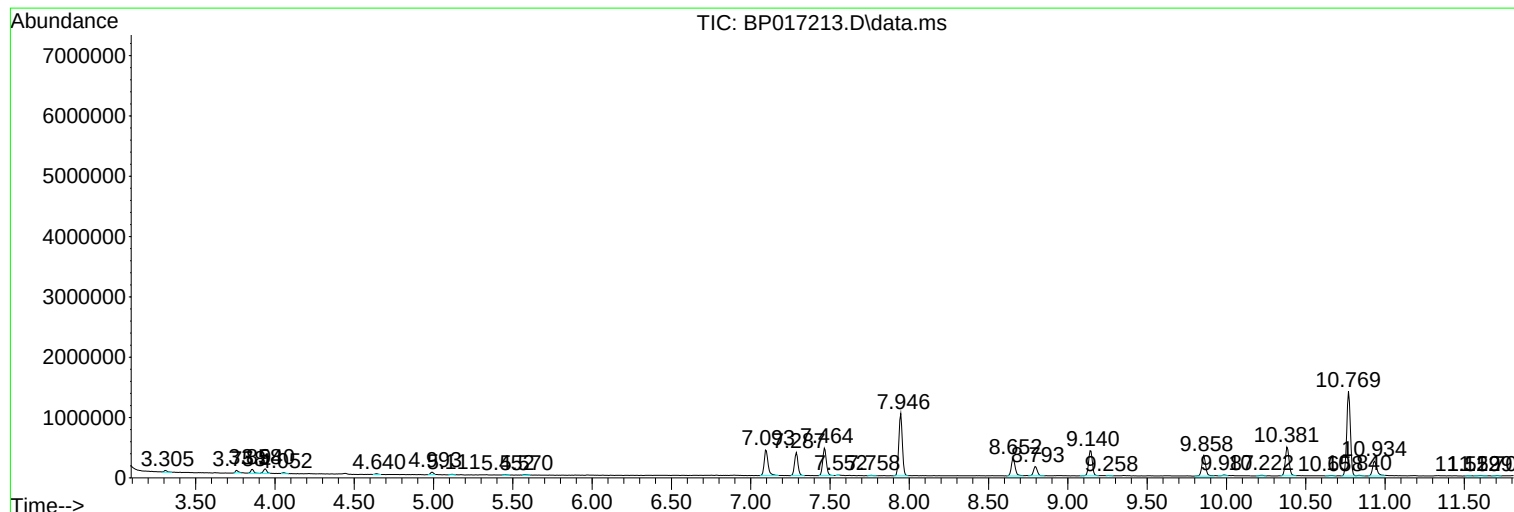

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017213.D
Acq On : 18 Sep 2023 19:42
Operator : MA/JU
Sample : 04330-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017213.D
Acq On : 18 Sep 2023 19:42
Operator : MA/JU
Sample : 04330-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
