

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017214.D
 Acq On : 18 Sep 2023 20:16
 Operator : MA/JU
 Sample : 04330-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	34	38	47	rVB	38034	62160	1.43%	0.142%
2	3.758	109	114	123	rBV3	44093	81441	1.87%	0.186%
3	3.858	127	131	137	rVV	102284	134402	3.09%	0.306%
4	3.940	140	145	154	rVB2	89034	148652	3.42%	0.339%
5	4.052	161	164	172	rVB2	20140	31889	0.73%	0.073%
6	4.446	228	231	236	rVB4	17565	24181	0.56%	0.055%
7	4.640	260	264	269	rVB2	19590	29061	0.67%	0.066%
8	4.987	319	323	337	rVB	52280	84394	1.94%	0.192%
9	5.111	341	344	351	rVV2	12669	21341	0.49%	0.049%
10	5.452	399	402	407	rVB5	6684	10829	0.25%	0.025%
11	5.575	419	423	427	rVB2	12333	17212	0.40%	0.039%
12	5.893	475	477	482	rVB5	6684	9723	0.22%	0.022%
13	6.793	624	630	632	rBV7	4011	6157	0.14%	0.014%
14	6.893	644	647	648	rBV3	9145	7980	0.18%	0.018%
15	7.093	672	681	696	rBV	608390	1065737	24.51%	2.430%
16	7.287	708	714	722	rBV	514758	785298	18.06%	1.791%
17	7.464	737	744	754	rBV	653733	1037138	23.85%	2.365%
18	7.546	754	758	767	rVB2	13945	29591	0.68%	0.067%
19	7.605	767	768	772	rBV4	3732	5219	0.12%	0.012%
20	7.752	789	793	801	rVB3	6481	12306	0.28%	0.028%
21	7.946	818	826	837	rBV	1227238	1922197	44.20%	4.383%
22	8.652	936	946	956	rBV	460397	776400	17.85%	1.771%
23	8.793	964	970	979	rBV	329903	523679	12.04%	1.194%
24	9.140	1021	1029	1039	rBV	599889	972937	22.37%	2.219%
25	9.352	1060	1065	1072	rVB10	4890	11557	0.27%	0.026%
26	9.857	1143	1151	1161	rBV	491342	827610	19.03%	1.887%
27	9.987	1167	1173	1179	rBV	35432	69030	1.59%	0.157%
28	10.228	1206	1214	1219	rBV2	20679	35926	0.83%	0.082%
29	10.322	1226	1230	1233	rBV5	3593	5201	0.12%	0.012%
30	10.381	1233	1240	1250	rVV	745973	1219256	28.04%	2.780%
31	10.652	1284	1286	1293	rVB8	5391	9214	0.21%	0.021%
32	10.769	1298	1306	1313	rVV	1717697	2795183	64.27%	6.374%
33	10.834	1315	1317	1322	rVB6	7162	9654	0.22%	0.022%
34	10.934	1327	1334	1351	rBV	321555	605048	13.91%	1.380%
35	11.328	1390	1401	1405	rBV	10305	25146	0.58%	0.057%
36	11.522	1431	1434	1439	rVB7	5912	9588	0.22%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017214.D
 Acq On : 18 Sep 2023 20:16
 Operator : MA/JU
 Sample : 04330-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	11.593	1439	1446	1452	rBV	14266	28332	0.65%	0.065%
38	11.704	1463	1465	1470	rVB6	4500	4719	0.11%	0.011%
39	11.804	1475	1482	1487	rVV7	7536	11082	0.25%	0.025%
40	11.910	1496	1500	1503	rVB6	3587	5652	0.13%	0.013%

41	12.110	1531	1534	1537	rBV4	5867	8742	0.20%	0.020%
42	12.169	1539	1544	1551	rVB3	12713	25774	0.59%	0.059%
43	12.257	1555	1559	1562	rBV5	3593	4877	0.11%	0.011%
44	12.351	1569	1575	1582	rVB2	16042	28384	0.65%	0.065%
45	12.851	1658	1660	1665	rVB6	4578	5102	0.12%	0.012%

46	12.922	1667	1672	1677	rBV9	5874	10385	0.24%	0.024%
47	13.057	1692	1695	1701	rVV8	6681	10298	0.24%	0.023%
48	13.134	1704	1708	1710	rBV5	2929	4507	0.10%	0.010%
49	13.175	1712	1715	1719	rVB5	8373	11445	0.26%	0.026%
50	13.357	1739	1746	1751	rBV9	9427	17121	0.39%	0.039%

51	13.451	1754	1762	1768	rBV	64508	110438	2.54%	0.252%
52	13.757	1806	1814	1815	rBV8	4787	9756	0.22%	0.022%
53	13.781	1815	1818	1825	rVV4	12921	20968	0.48%	0.048%
54	13.846	1827	1829	1833	rVB5	4898	5534	0.13%	0.013%
55	13.922	1835	1842	1847	rBV9	11237	26545	0.61%	0.061%

56	14.016	1852	1858	1868	rVV	1407442	1891041	43.48%	4.312%
57	14.304	1898	1907	1915	rBV	1548381	2211192	50.84%	5.042%
58	14.434	1925	1929	1935	rVB6	13480	18810	0.43%	0.043%
59	14.604	1951	1958	1970	rBV	2541900	3661681	84.20%	8.350%
60	14.828	1987	1996	2010	rBV	283949	554103	12.74%	1.264%

61	14.998	2021	2025	2029	rVV5	23201	37475	0.86%	0.085%
62	15.045	2029	2033	2039	rVB4	47161	75528	1.74%	0.172%
63	15.204	2056	2060	2066	rBV8	9653	21591	0.50%	0.049%
64	15.345	2081	2084	2087	rBV5	8465	11912	0.27%	0.027%
65	15.387	2089	2091	2094	rVV3	14499	13557	0.31%	0.031%

66	15.598	2121	2127	2135	rBV	2182357	3024221	69.54%	6.896%
67	15.728	2144	2149	2155	rBV	386673	513775	11.81%	1.172%
68	15.787	2155	2159	2165	rVB5	22415	35146	0.81%	0.080%
69	16.263	2236	2240	2246	rBV2	43704	80437	1.85%	0.183%
70	16.722	2314	2318	2322	rBV7	16990	31982	0.74%	0.073%

71	17.057	2372	2375	2379	rBV	35068	43677	1.00%	0.100%
72	17.104	2379	2383	2389	rVB	39503	62116	1.43%	0.142%
73	17.375	2423	2429	2440	rBV	3067583	4349025	100.00%	9.918%
74	17.475	2440	2446	2455	rVV2	2293209	3200043	73.58%	7.297%
75	17.804	2499	2502	2506	rVB3	56199	64531	1.48%	0.147%

76	17.998	2532	2535	2539	rBV	41204	46095	1.06%	0.105%
----	--------	------	------	------	-----	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017214.D
Acq On : 18 Sep 2023 20:16
Operator : MA/JU
Sample : 04330-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Title : SVOA CALIBRATION

77	18.216	2568	2572	2580	rBV2	216986	388457	8.93%	0.886%
78	19.716	2822	2827	2834	rBV	2782316	3612166	83.06%	8.237%
79	21.480	3123	3127	3131	rVB	2385012	3054639	70.24%	6.966%
80	24.004	3551	3556	3563	rVB	1563959	3076514	70.74%	7.016%




Sum of corrected areas: 43851712

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017214.D
Acq On : 18 Sep 2023 20:16
Operator : MA/JU
Sample : 04330-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

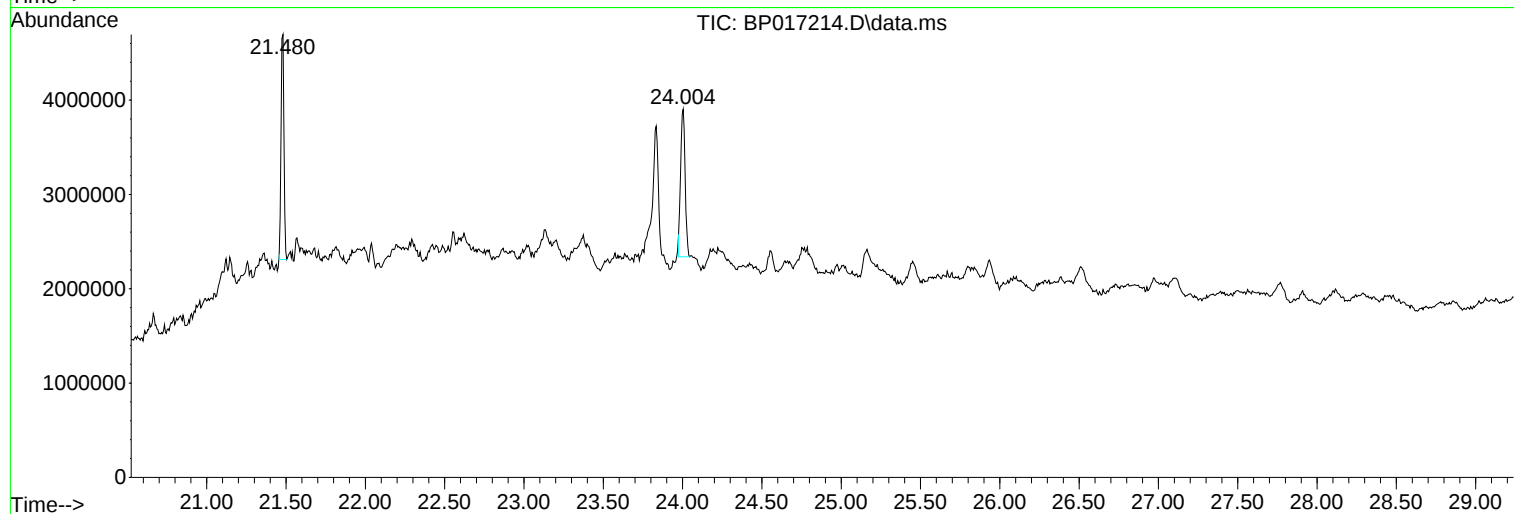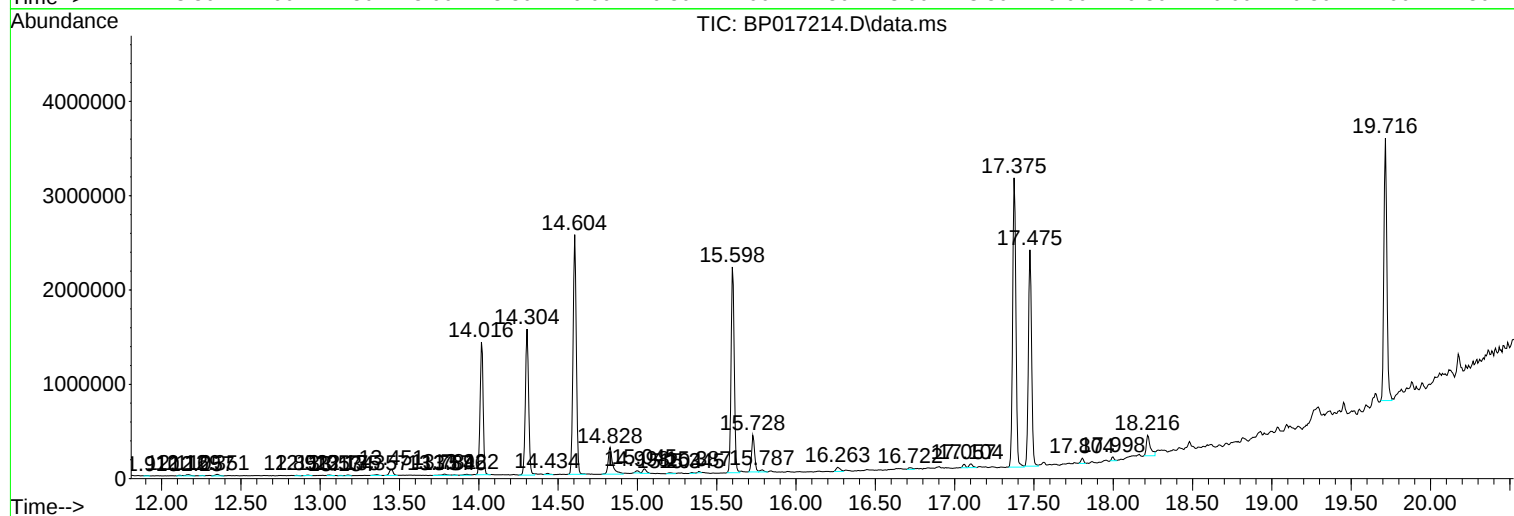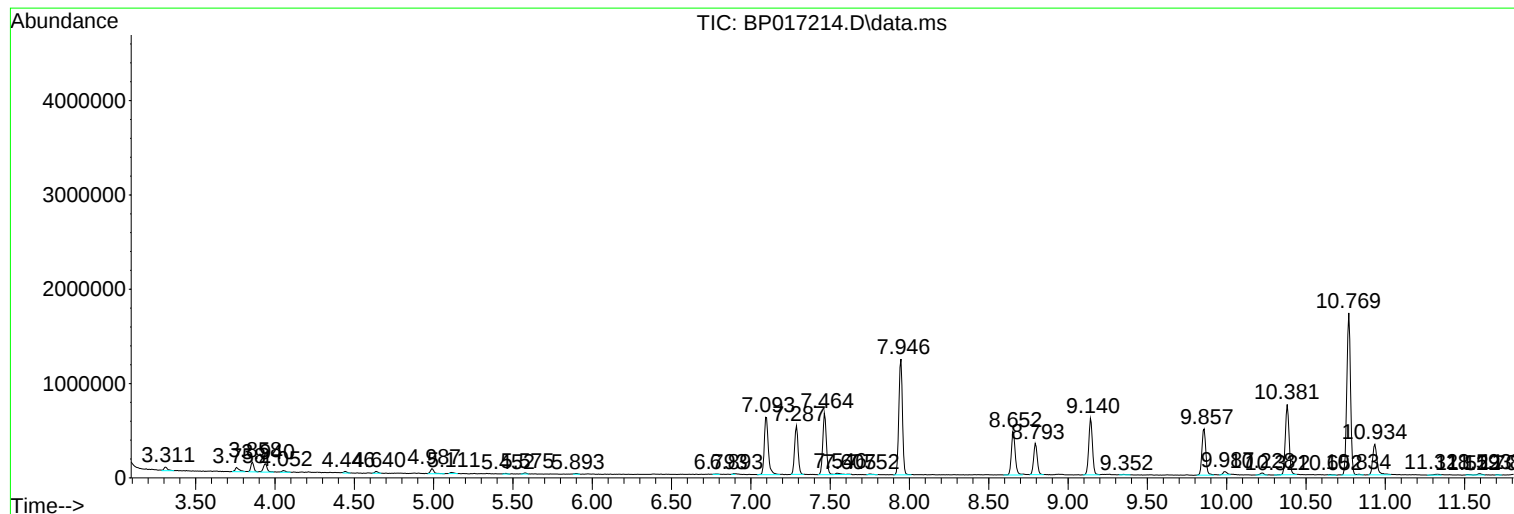

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017214.D
Acq On : 18 Sep 2023 20:16
Operator : MA/JU
Sample : 04330-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017214.D
Acq On : 18 Sep 2023 20:16
Operator : MA/JU
Sample : 04330-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------